


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
 Data File : BF130100.D
 Acq On : 02 Sep 2022 09:18
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 31 18:15:32 2022

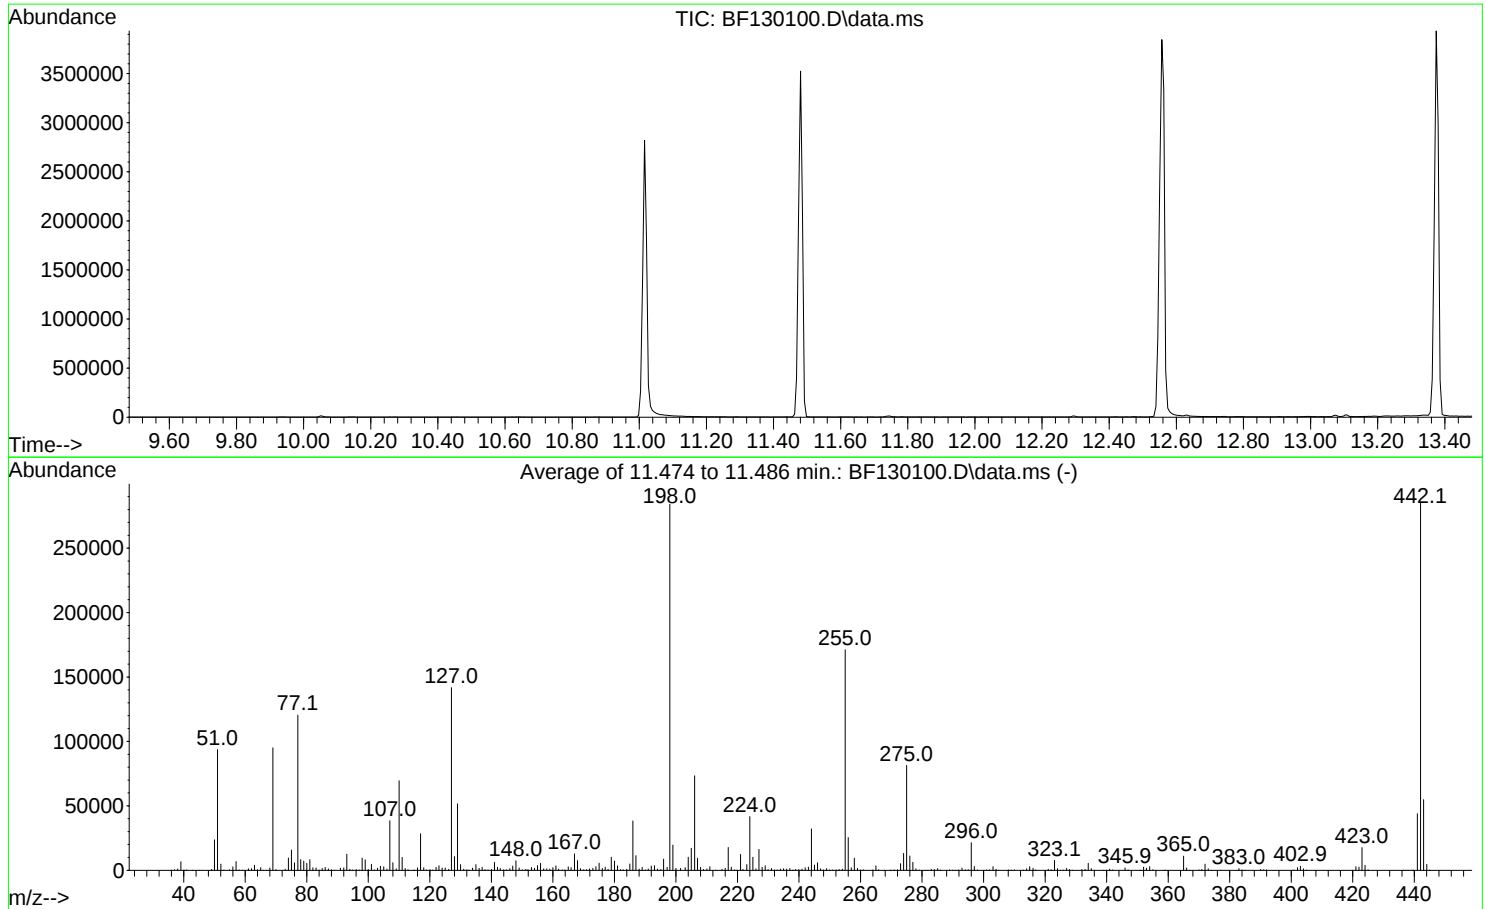




AutoFind: Scans 1562, 1563, 1564; Background Corrected with Scan 1556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	93653	PASS
68	69	0.00	2	1.9	1793	PASS
69	198	0.00	100	33.5	95053	PASS
70	69	0.00	2	0.6	548	PASS
127	198	10	80	49.9	141765	PASS
197	198	0.00	2	0.8	2302	PASS
198	198	100	100	100.0	284139	PASS
199	198	5	9	6.9	19577	PASS
275	198	10	60	28.7	81421	PASS
365	198	1	100	3.9	11011	PASS
441	198	0.01	100	15.4	43864	PASS
442	442	50	100	100.0	285501	PASS
443	442	15	24	19.2	54829	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130100.D
Acq On : 02 Sep 2022 09:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 03 06:19:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 18:15:32 2022
Response via : Initial Calibration

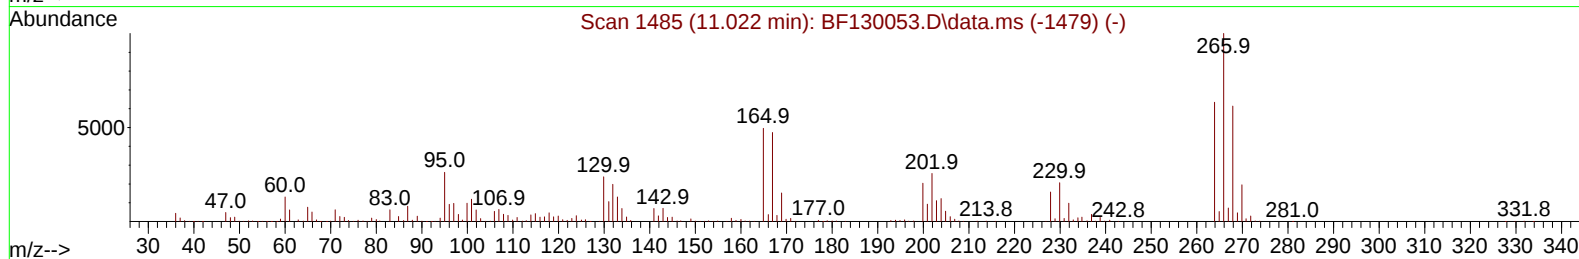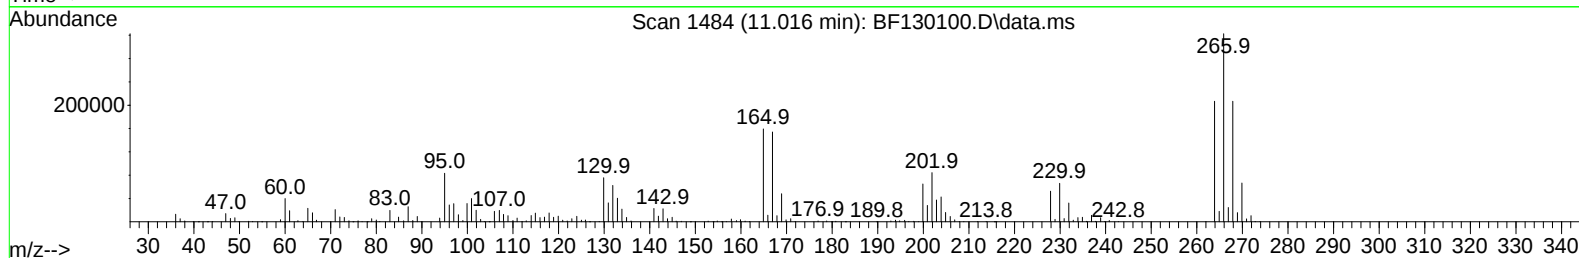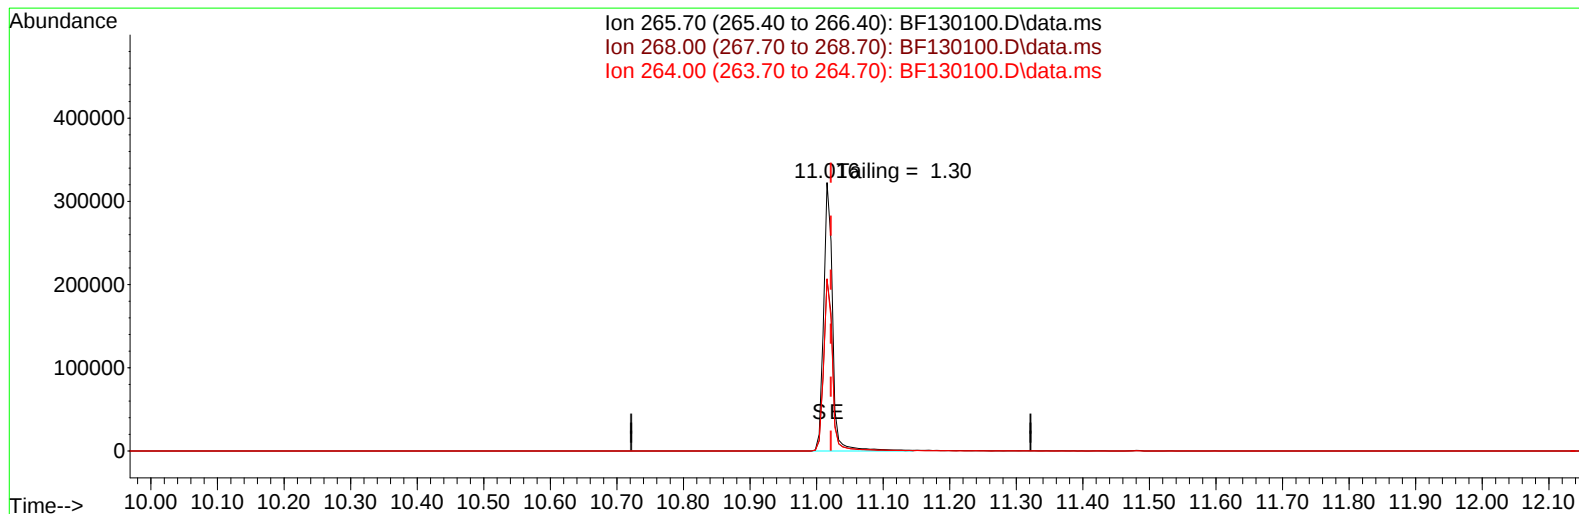

TIC: BF130100.D\data.ms

(70) Pentachlorophenol (C)

11.016min (-0.006) 479400.63 ng




response 298914

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.10
264.00	59.90	64.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130100.D
Acq On : 02 Sep 2022 09:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 03 06:19:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 18:15:32 2022
Response via : Initial Calibration

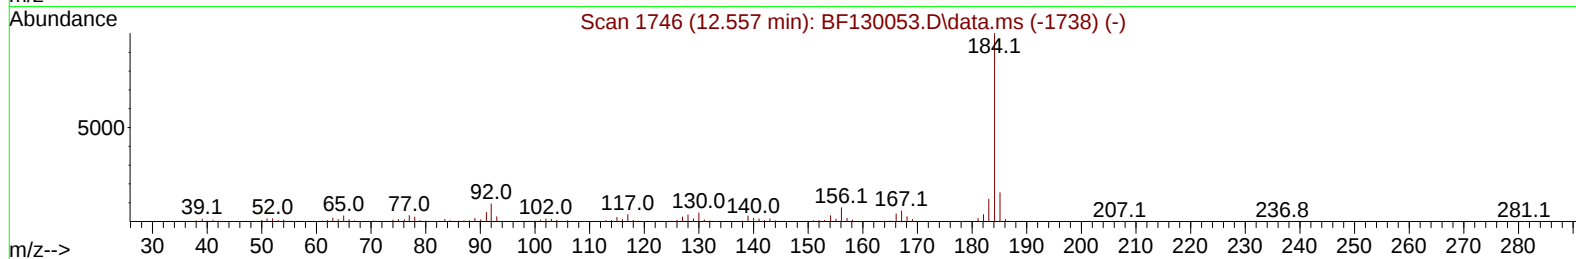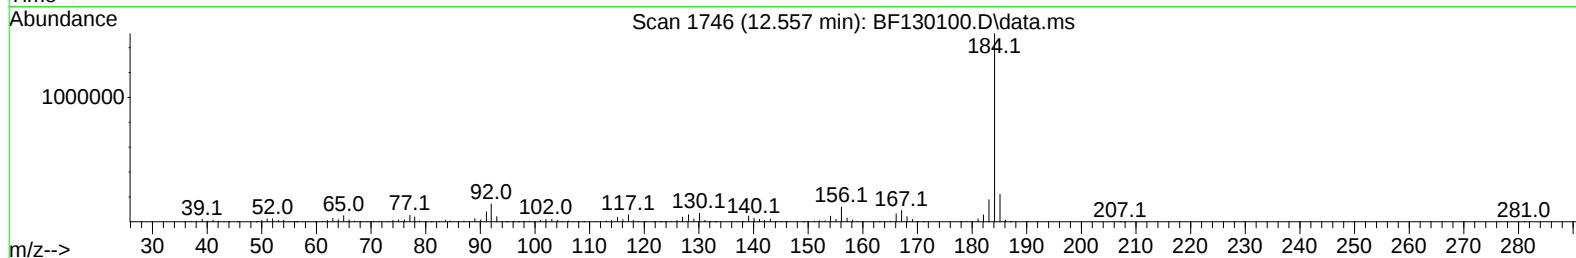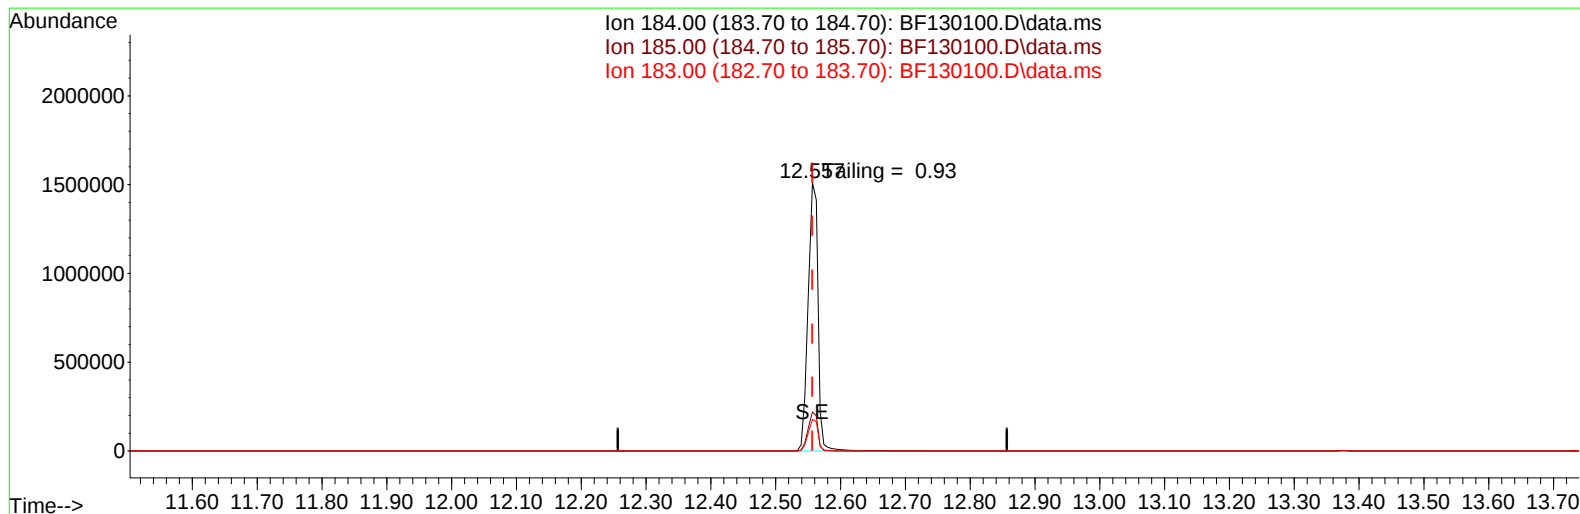

TIC: BF130100.D\data.ms

(77) Benzidine

12.557min (-0.000) 0.00 ng

response 1610034

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.54
183.00	11.80	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/2/2022	BNA_F	BF130100.D
Compound Name	Response	Retention Time
DDT	625508	13.374
DDD	5431	13.074
DDE	330	12.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5761	631269	0.91

Instrument :
BNA_F
ClientSampleId :
DFTPP