
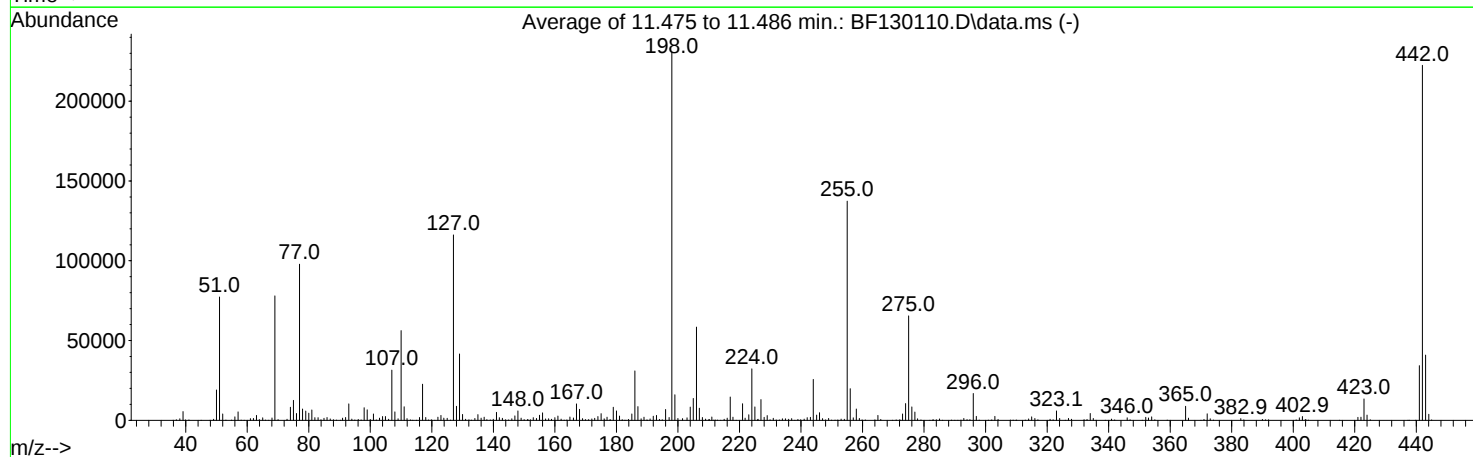


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
 Data File : BF130110.D
 Acq On : 02 Sep 2022 14:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 31 18:15:32 2022

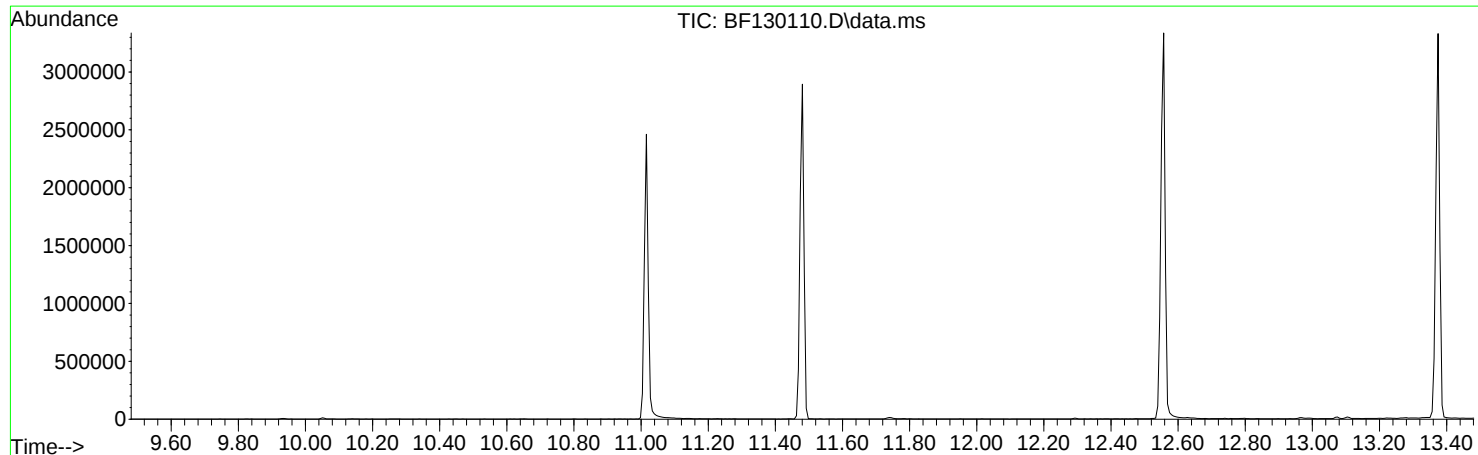




AutoFind: Scans 1562, 1563, 1564; Background Corrected with Scan 1557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	77272	PASS
68	69	0.00	2	1.9	1461	PASS
69	198	0.00	100	33.8	77965	PASS
70	69	0.00	2	0.6	497	PASS
127	198	10	80	50.4	116160	PASS
197	198	0.00	2	0.8	1792	PASS
198	198	100	100	100.0	230571	PASS
199	198	5	9	6.9	15990	PASS
275	198	10	60	28.4	65424	PASS
365	198	1	100	3.8	8763	PASS
441	198	0.01	100	14.8	34211	PASS
442	442	50	100	100.0	222531	PASS
443	442	15	24	18.4	40901	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130110.D
Acq On : 02 Sep 2022 14:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 03 06:20:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 18:15:32 2022
Response via : Initial Calibration

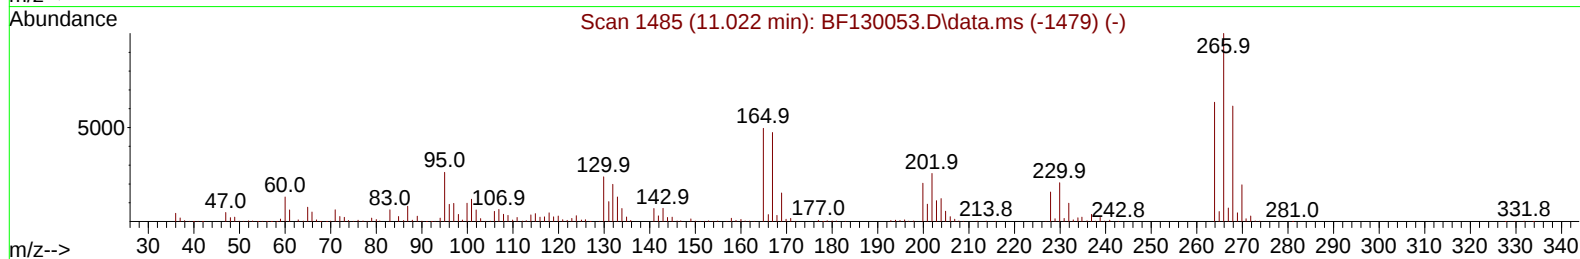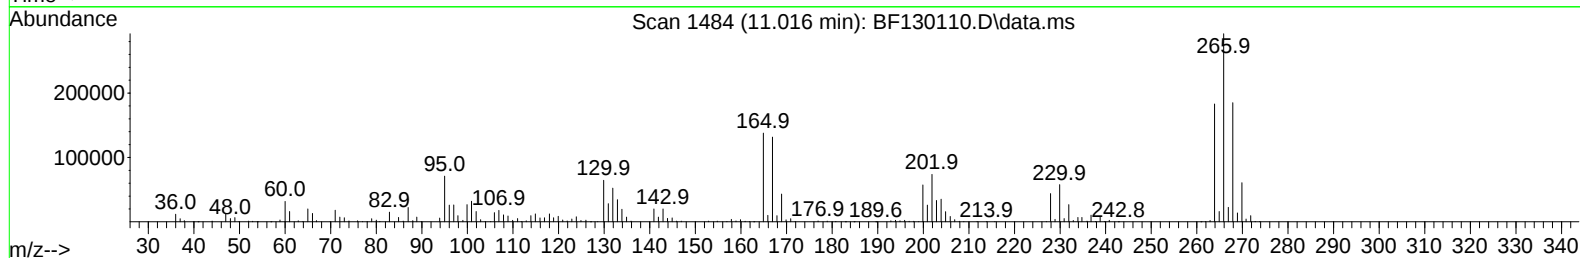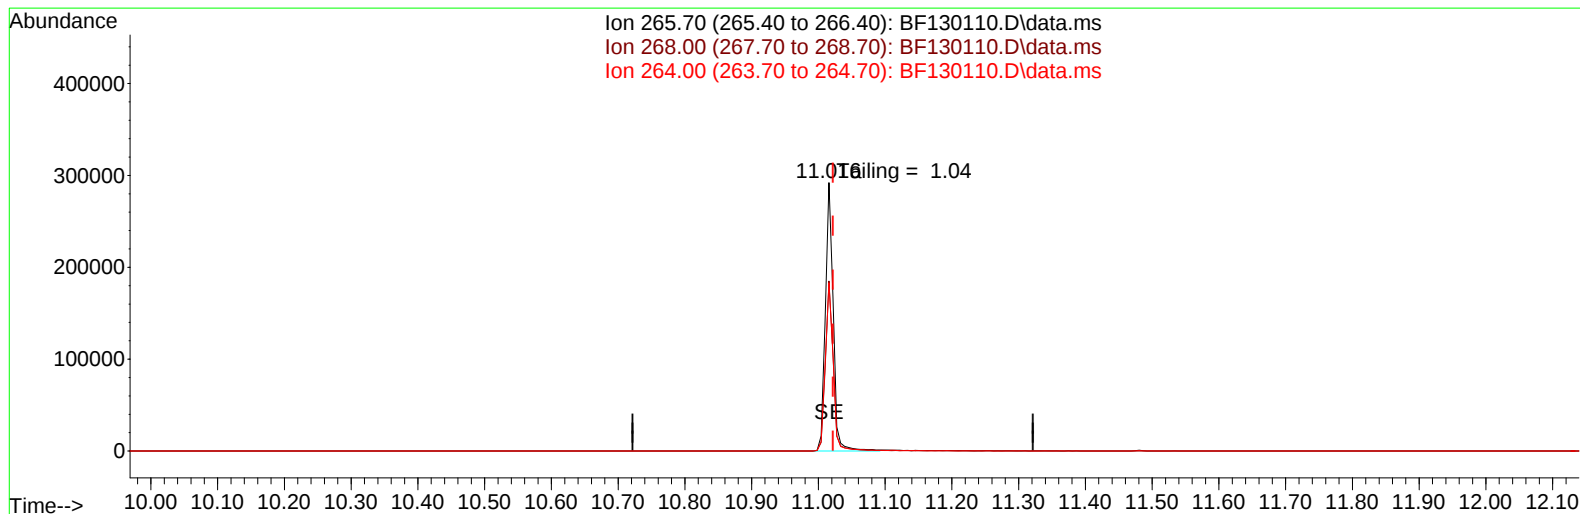

TIC: BF130110.D\data.ms

(70) Pentachlorophenol (C)

11.016min (-0.006) 31694.74 ng




response 239509

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.33
264.00	59.90	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130110.D
Acq On : 02 Sep 2022 14:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 03 06:20:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 18:15:32 2022
Response via : Initial Calibration

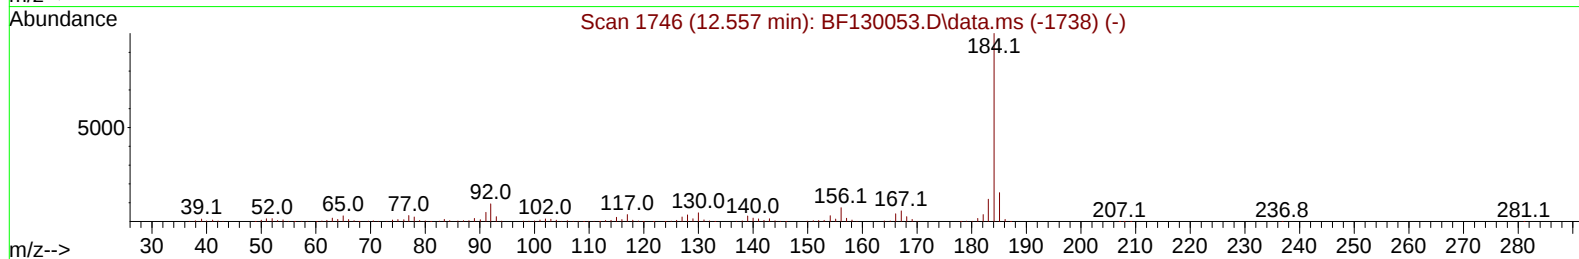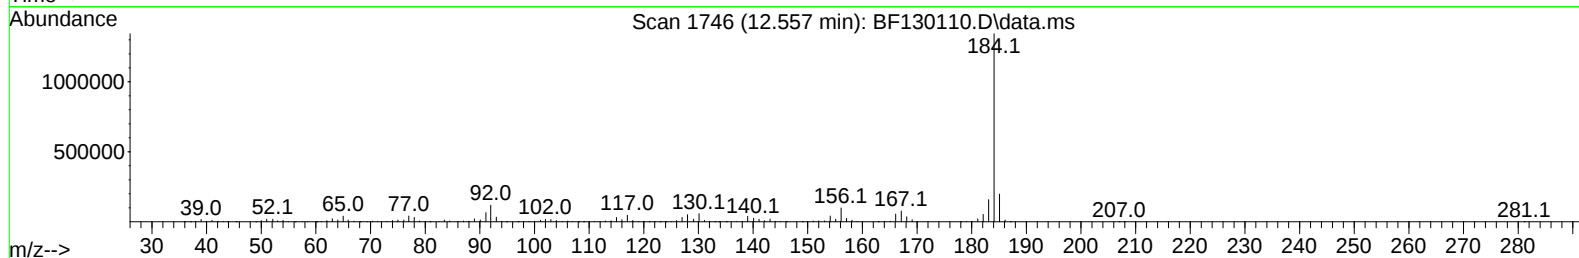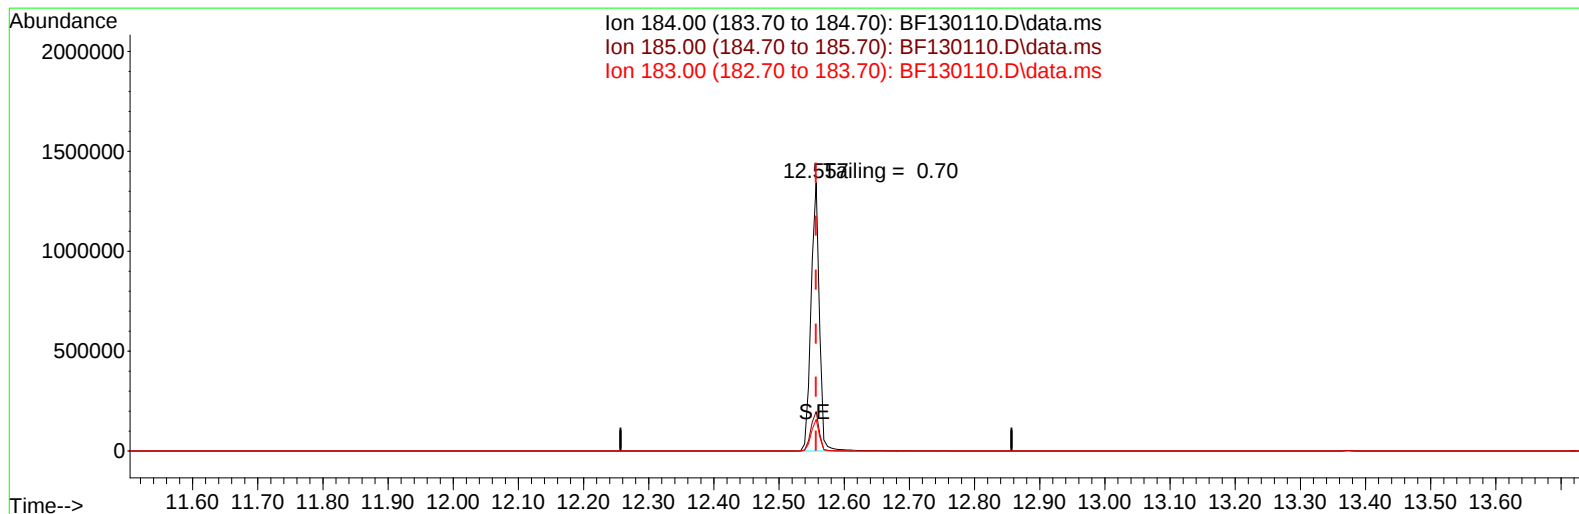

TIC: BF130110.D\data.ms

(77) Benzidine

12.557min (+ 0.000) 0.00 ng

response 1198188

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.71
183.00	11.80	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/2/2022	BNA_F	<u>BF130110.D</u>
Compound Name	Response	Retention Time
DDT	503777	13.374
DDD	5051	13.074
DDE	338	12.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5389	509166	1.06

Instrument :
BNA_F
ClientSampleId :
DFTPP