

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090319\
 Data File : BF116795.D
 Acq On : 4 Sep 2019 2:20
 Operator : HP/JU
 Sample : K4623-28
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 04 06:07:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 30 20:02:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	131280	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	525557	20.00	ng	0.00
39) Acenaphthene-d10	9.88	164	274208	20.00	ng	0.00
64) Phenanthrene-d10	11.36	188	472032	20.00	ng	0.00
76) Chrysene-d12	13.99	240	308631	20.00	ng	0.00
87) Perylene-d12	15.44	264	324209	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	981611	121.14	ng	0.01
7) Phenol-d6	6.48	99	1195220	112.33	ng	0.00
23) Nitrobenzene-d5	7.40	82	898206	97.57	ng	0.00
42) 2,4,6-Tribromophenol	10.67	330	306150	167.01	ng	0.00
45) 2-Fluorobiphenyl	9.20	172	1521619	93.61	ng	0.00
79) Terphenyl-d14	12.95	244	1584004	94.95	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.40	70	118041	16.848	ng	# 72
25) Isophorone	7.40	82	898198	48.148	ng	# 66
51) 2,6-Dinitrotoluene	9.88	165	34862	9.652	ng	# 21
57) 2,4-Dinitrotoluene	9.88	165	34862	7.894	ng	# 21
65) 4,6-Dinitro-2-methylphenol	10.67	198	633	7.759	ng	# 1
67) 4-Bromophenyl-phenylether	10.67	248	20242	4.221	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090319\
Data File : BF116795.D
Acq On : 4 Sep 2019 2:20
Operator : HP/JU
Sample : K4623-28
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 04 06:07:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

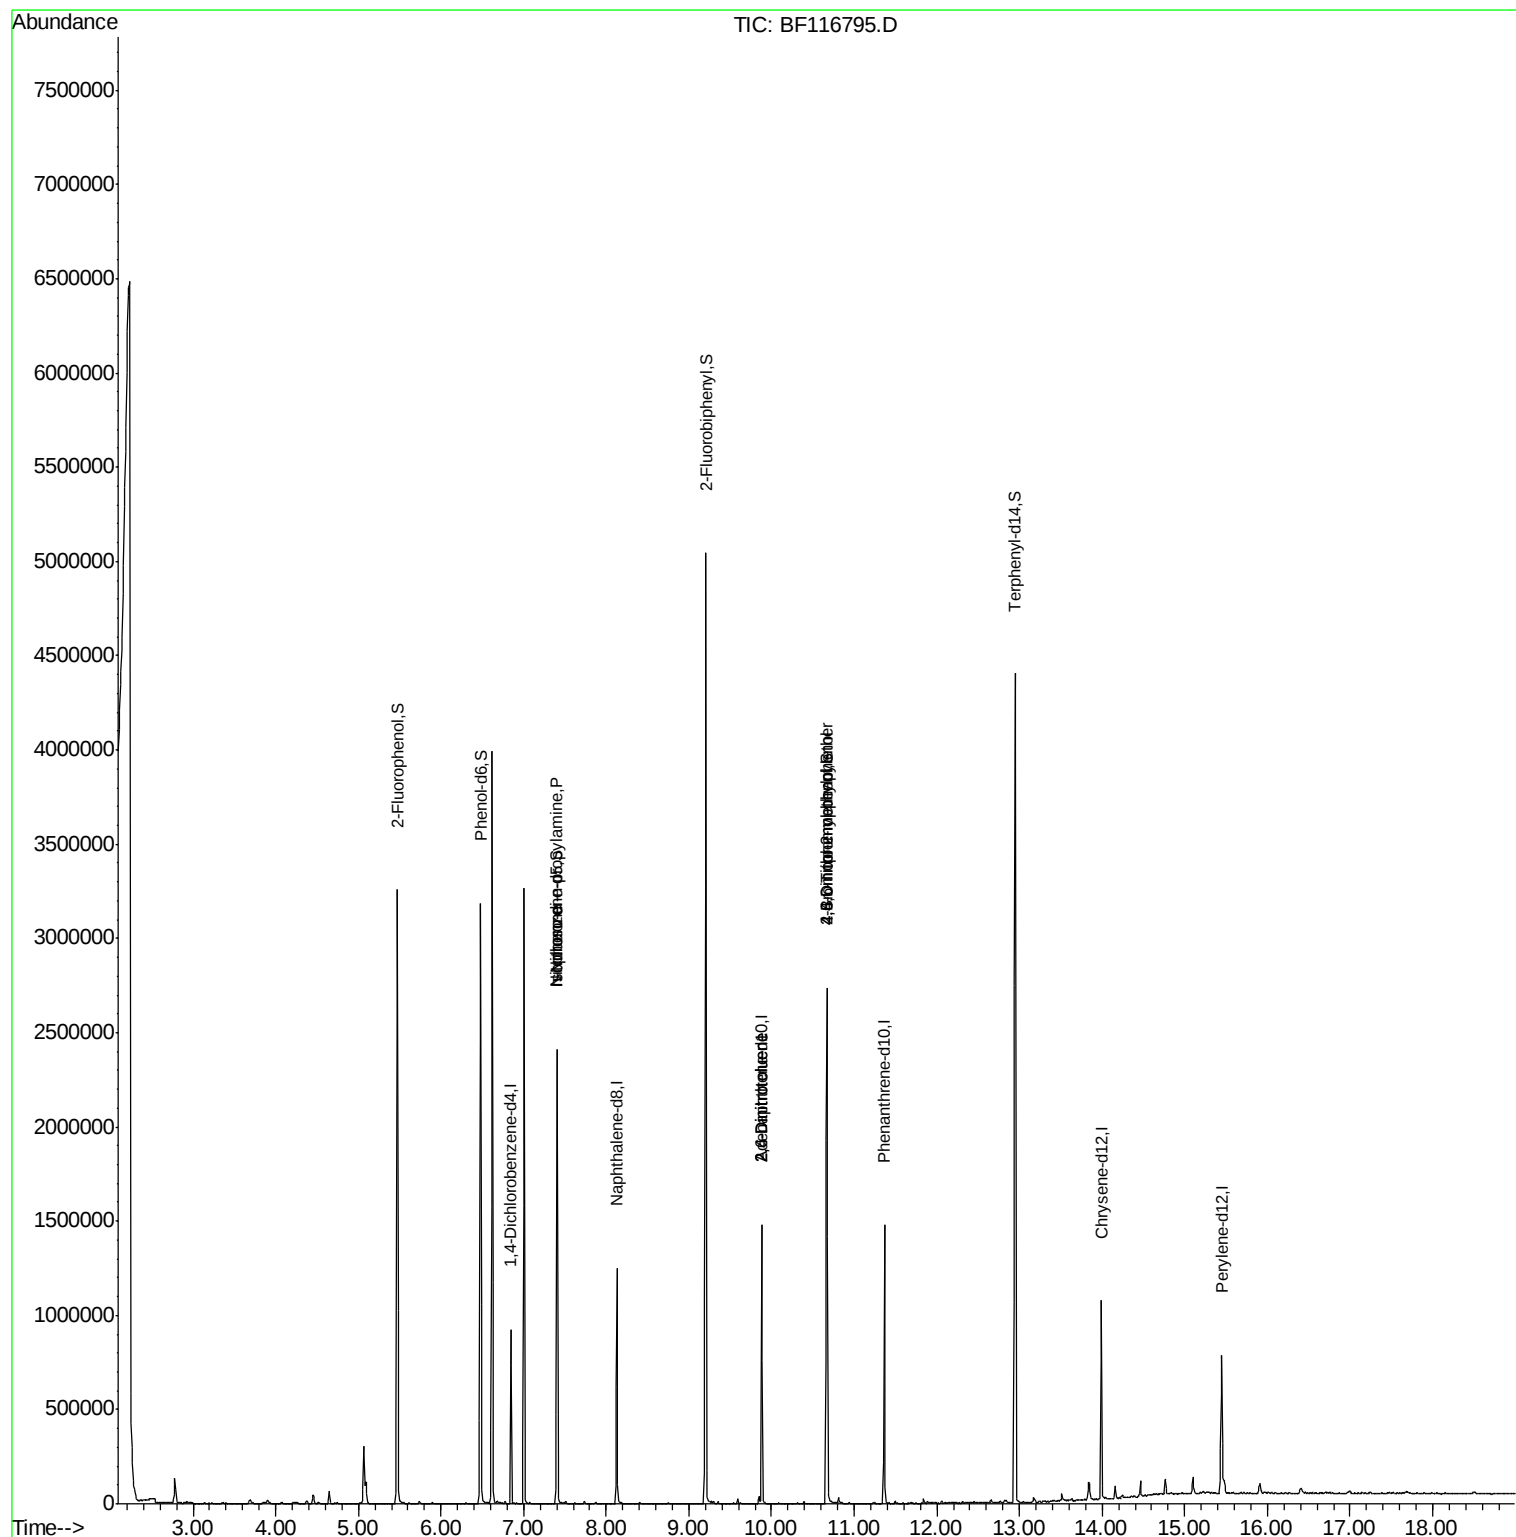







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.85 min Scan# 809
Delta R.T. -0.01 min
Lab File: BF116795.D
Acq: 4 Sep 2019 2:20

Instrument :
BNA_F
ClientSampleId :




Tot Ion	Ratio	Lower	Upper
152	100		
150	164.5	124.4	186.6
115	66.6	49.9	74.9

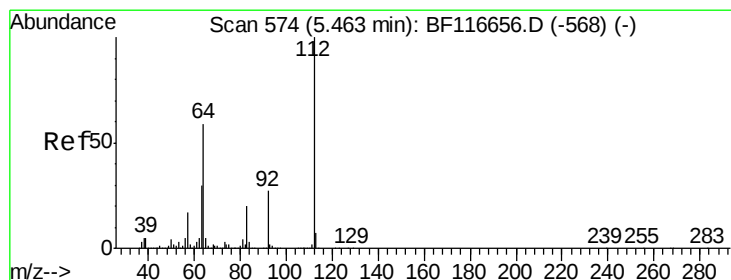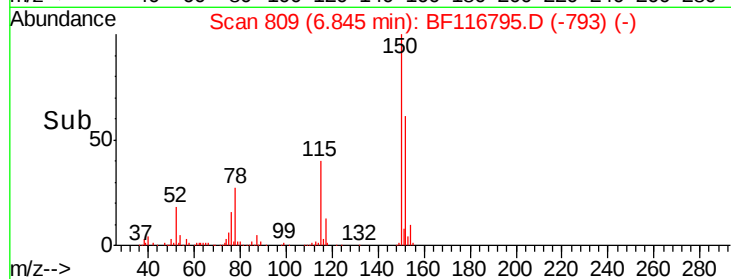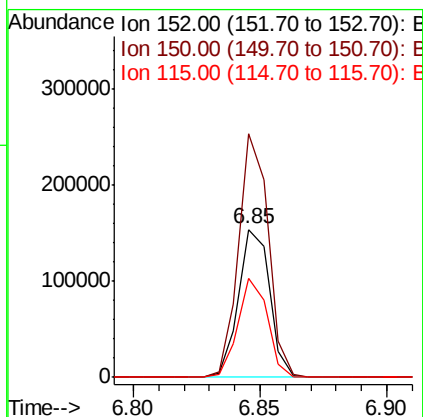

#5

2-Fluorophenol
Concen: 121.135 ng
RT: 5.47 min Scan# 576
Delta R.T. 0.01 min
Lab File: BF116795.D
Acq: 4 Sep 2019 2:20

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.2	47.1	70.7
63	28.2	24.9	37.3

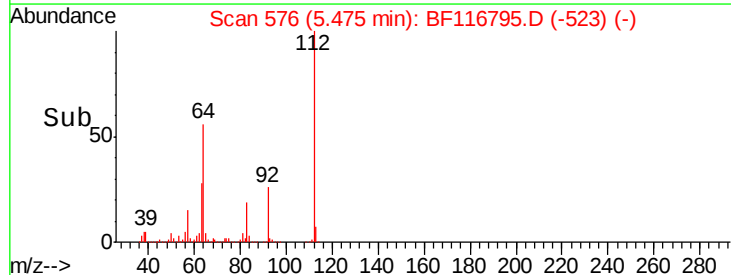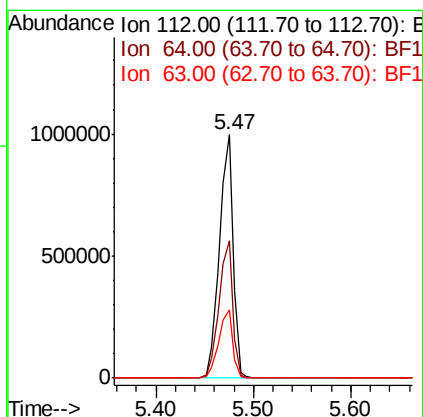



#7

Phenol-d6

Concen: 112.325 ng

RT: 6.48 min Scan# 747

Delta R.T. 0.00 min

Lab File: BF116795.D

Acq: 4 Sep 2019 2:20


Instrument :

BNA_F

ClientSampleId :

Tot Ion: 99 Resp: 1195220

Ion	Ratio	Lower	Upper
99	100		
42	14.3	13.7	20.5
71	32.9	30.8	46.2



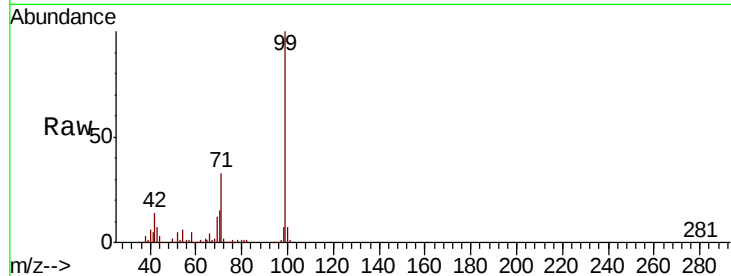


Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

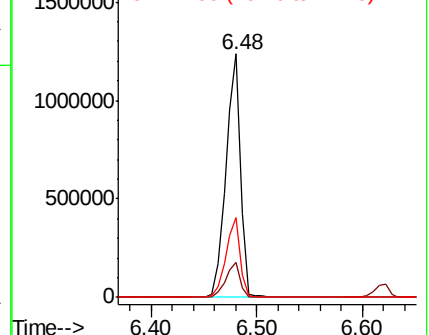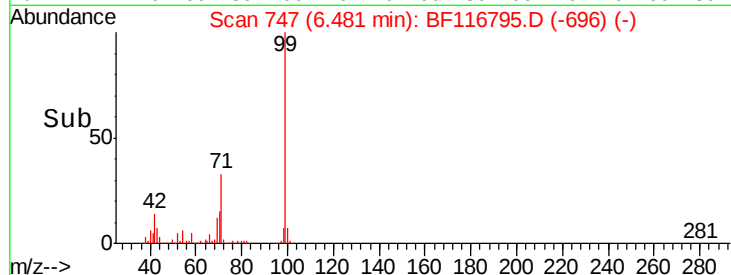

#19

n-Nitroso-di-n-propylamine

Concen: 16.848 ng

RT: 7.40 min Scan# 904


Delta R.T. 0.14 min

Lab File: BF116795.D

Acq: 4 Sep 2019 2:20

Tgt Ion: 70 Resp: 118041

Ion	Ratio	Lower	Upper
70	100		
42	37.1	43.5	65.3#
101	0.0	7.8	11.6#
130	2.2	16.6	24.8#





Abundance

Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

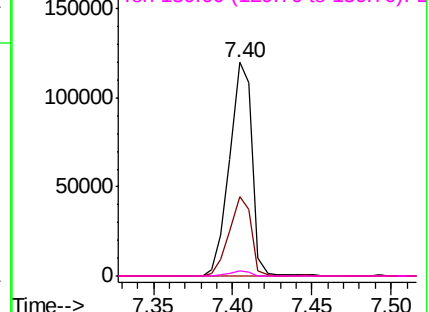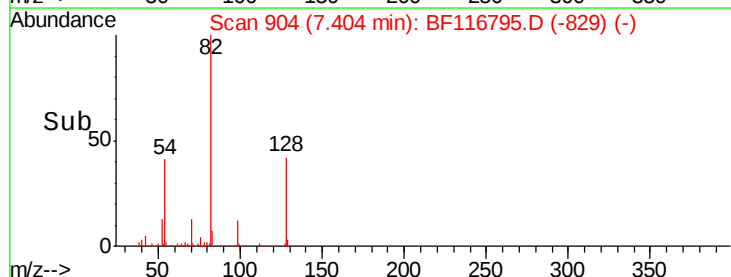



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.13 min Scan# 1027

Delta R.T. -0.01 min

Lab File: BF116795.D


Acq: 4 Sep 2019 2:20

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136	Resp:	525557
Ion Ratio	Lower	Upper
136	100	
137	10.7	8.9 13.3
54	6.2	4.8 7.2
68	5.9	4.0 6.0






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

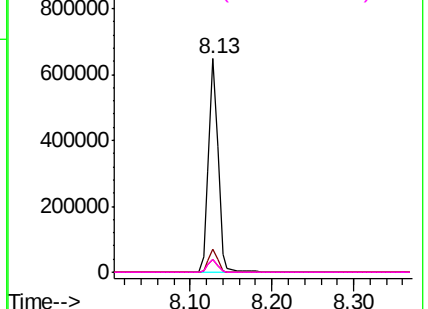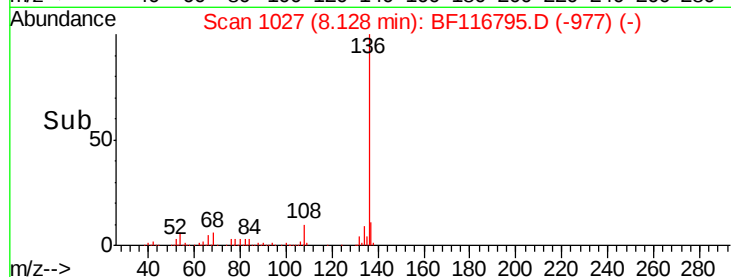

#23

Nitrobenzene-d5

Concen: 97.565 ng


RT: 7.40 min Scan# 904

Delta R.T. -0.01 min

Lab File: BF116795.D

Acq: 4 Sep 2019 2:20



Tgt Ion: 82	Resp:	898206
Ion Ratio	Lower	Upper
82	100	
128	42.3	32.8 49.2
54	40.8	36.9 55.3



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

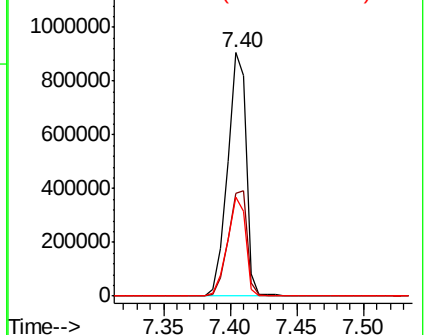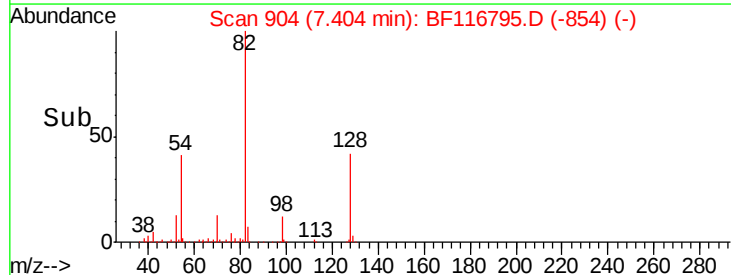



#25

Isophorone

Concen: 48.148 ng

RT: 7.40 min Scan# 904

Delta R.T. -0.26 min

Lab File: BF116795.D

Acq: 4 Sep 2019 2:20

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 898198

Ion Ratio Lower Upper

82 100

95 0.0 5.8 8.6#




138 0.0 13.5 20.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

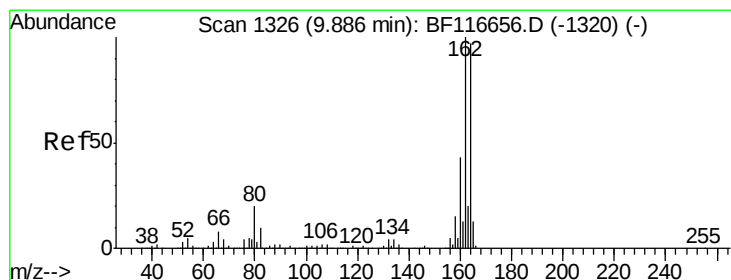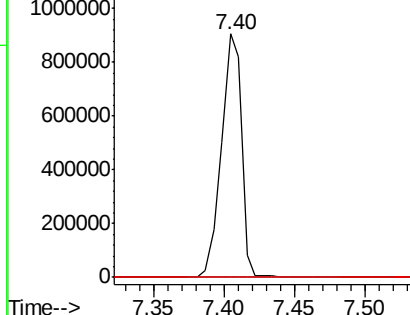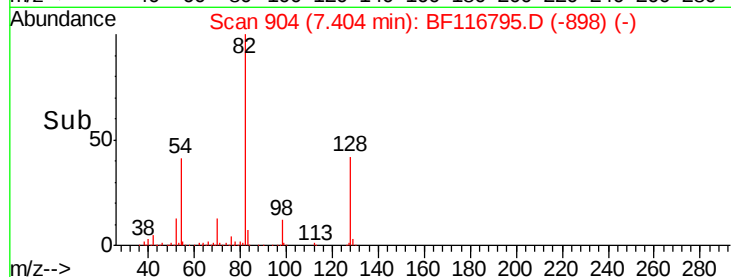

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.88 min Scan# 1325

Delta R.T. -0.01 min

Lab File: BF116795.D

Acq: 4 Sep 2019 2:20


Tgt Ion: 164 Resp: 274208

Ion Ratio Lower Upper

164 100

162 102.2 81.4 122.0



160 43.2 35.4 53.2




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

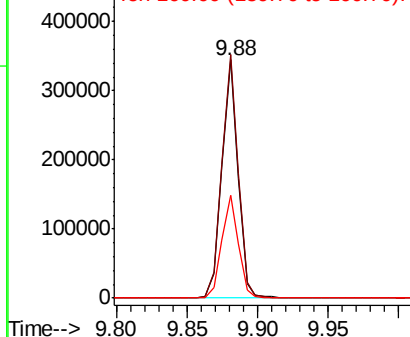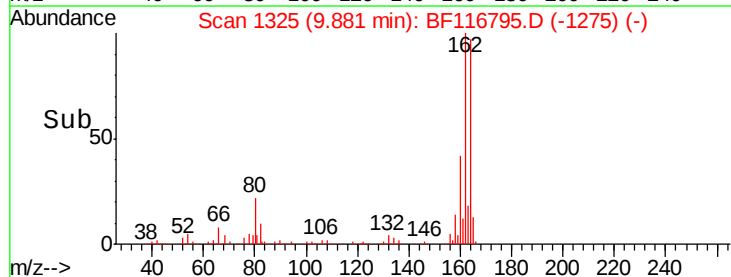


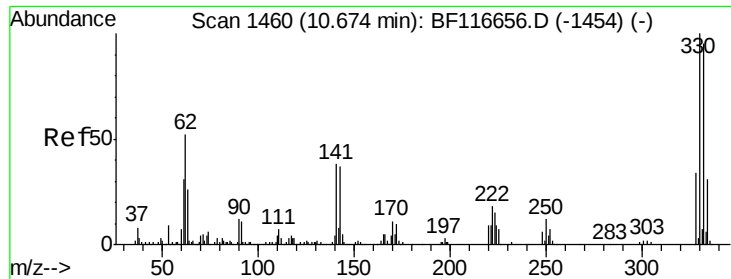




#42
 2,4,6-Tribromophenol
 Concen: 167.009 ng
 RT: 10.67 min Scan# 1459
 Delta R.T. -0.01 min
 Lab File: BF116795.D
 Acq: 4 Sep 2019 2:20

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	76.9	115.3
141	41.5	31.4	47.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

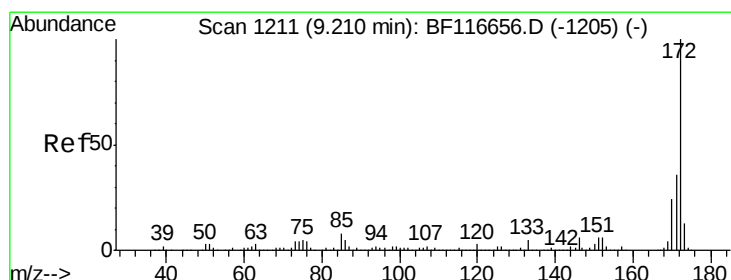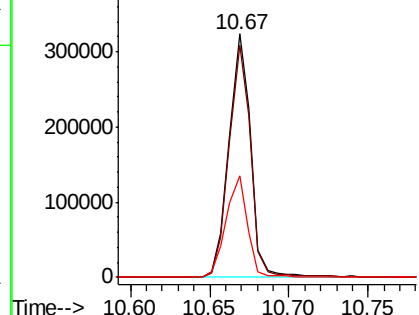
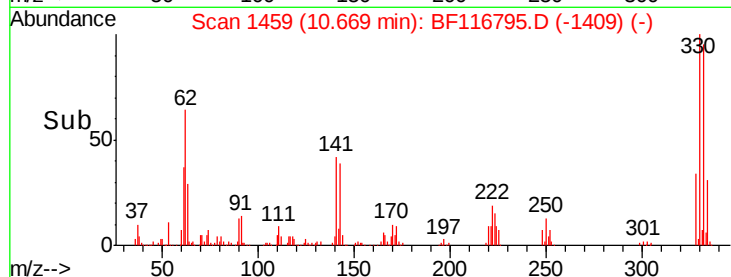



#45
 2-Fluorobiphenyl
 Concen: 93.608 ng
 RT: 9.20 min Scan# 1210
 Delta R.T. -0.00 min
 Lab File: BF116795.D
 Acq: 4 Sep 2019 2:20

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	27.8	41.6
170	23.8	18.9	28.3

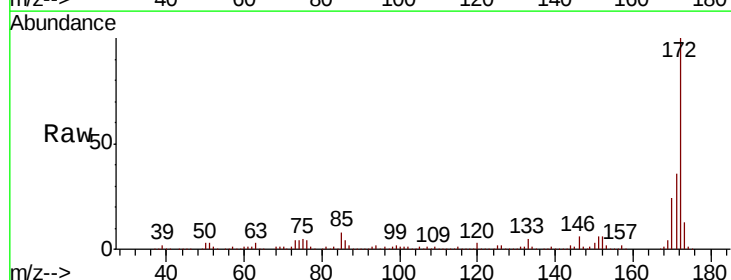

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

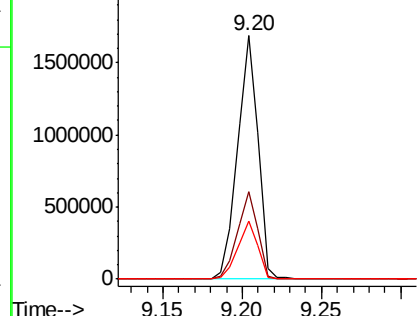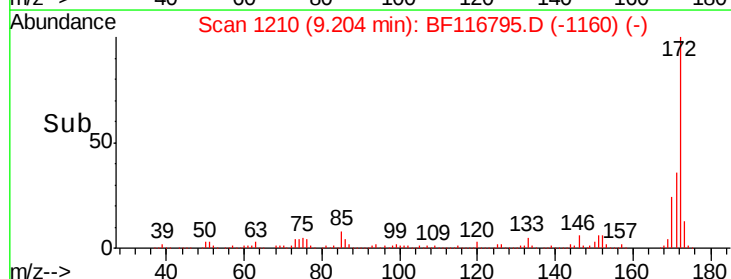


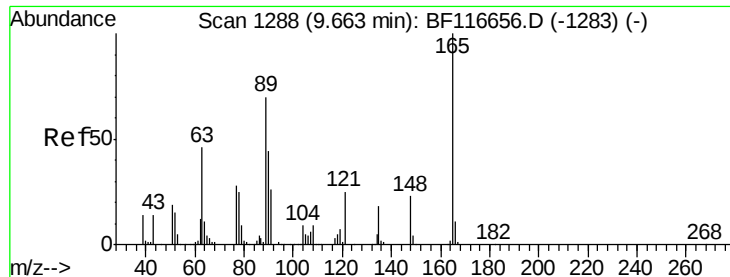




#51
 2,6-Dinitrotoluene
 Concen: 9.652 ng
 RT: 9.88 min Scan# 1325
 Delta R.T. 0.22 min
 Lab File: BF116795.D
 Acq: 4 Sep 2019 2:20

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	0.9	47.3	70.9#
89	1.8	52.5	78.7#

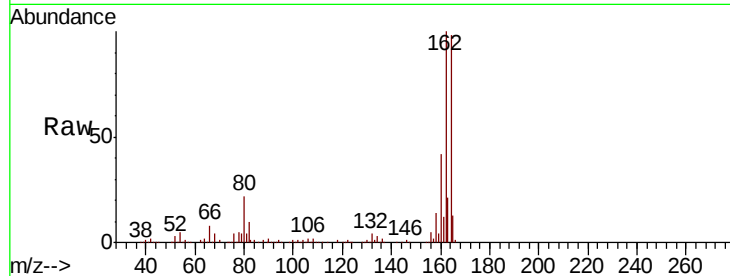


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

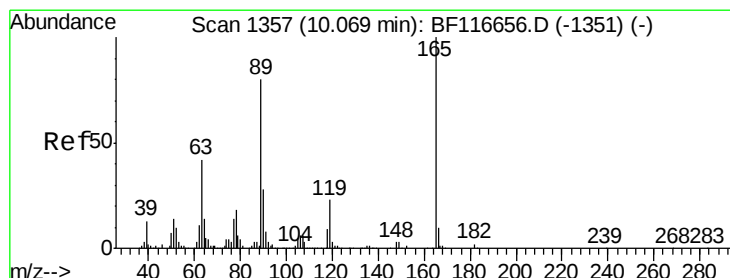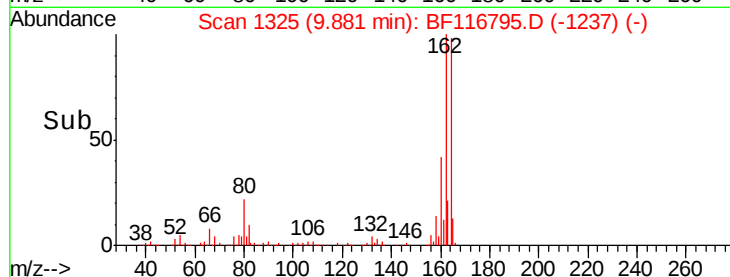
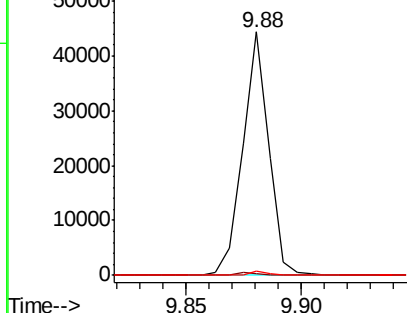



#57
 2,4-Dinitrotoluene
 Concen: 7.894 ng
 RT: 9.88 min Scan# 1325
 Delta R.T. -0.19 min
 Lab File: BF116795.D
 Acq: 4 Sep 2019 2:20

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.9	36.4	54.6#
89	1.8	62.6	94.0#
182	0.0	2.1	3.1#

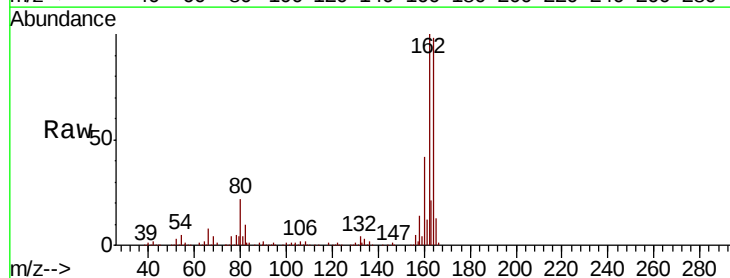

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E



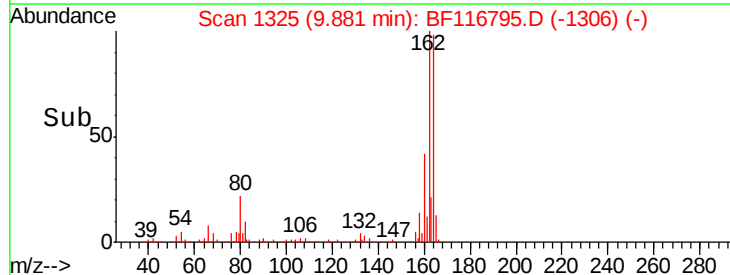
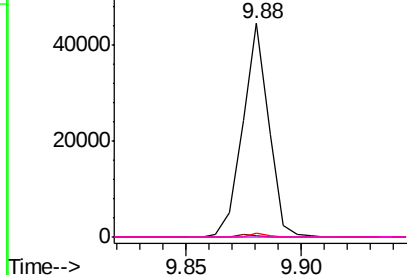


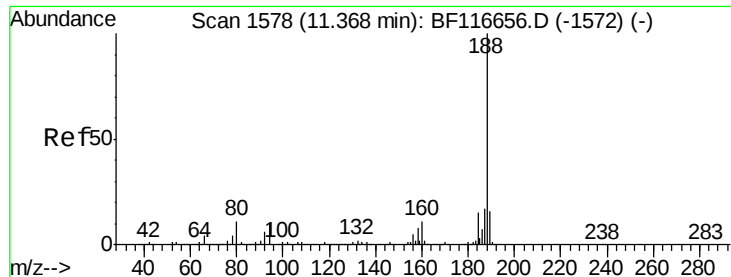

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1577
Delta R.T. -0.01 min
Lab File: BF116795.D
Acq: 4 Sep 2019 2:20




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
188	100		
94	10.7	7.3	10.9
80	11.9	8.4	12.6

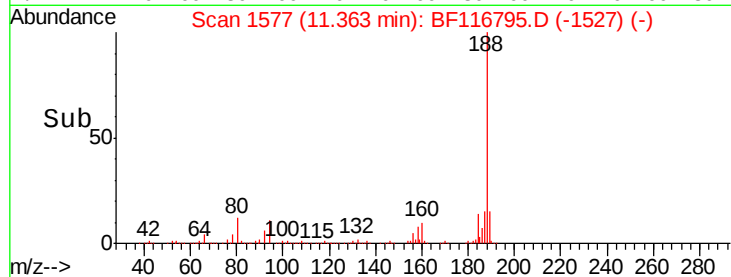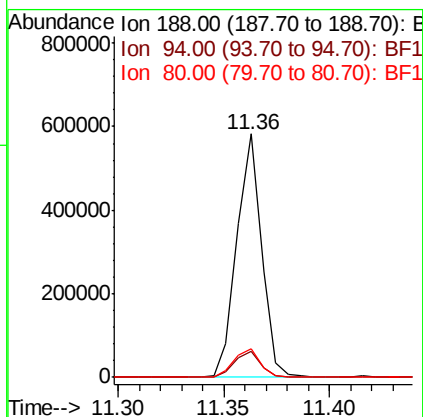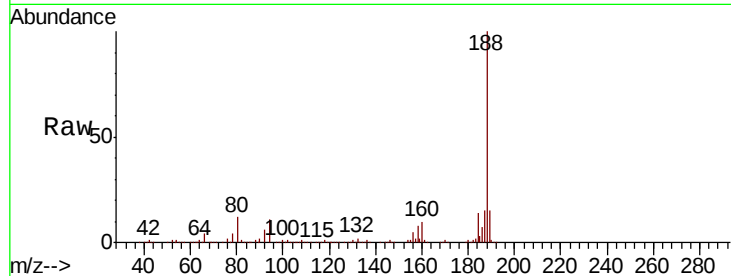

#65
4,6-Dinitro-2-methylphenol
Concen: 7.759 ng
RT: 10.67 min Scan# 1459
Delta R.T. 0.19 min
Lab File: BF116795.D
Acq: 4 Sep 2019 2:20

Tgt Ion	Ratio	Lower	Upper
198	100		
51	154.9	18.4	58.4#
105	217.0	22.9	62.9#

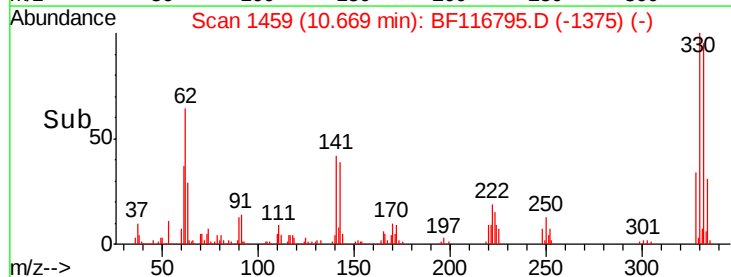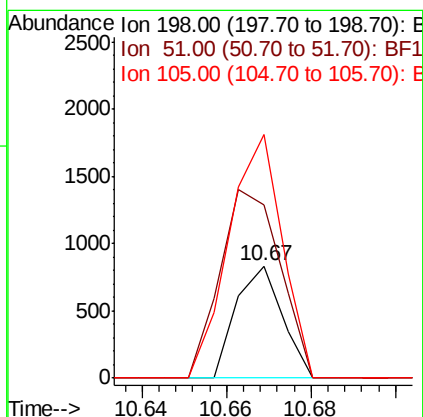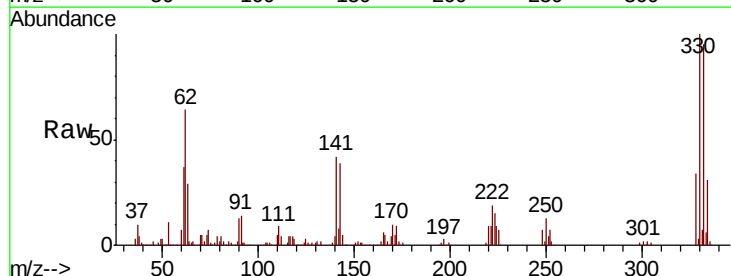


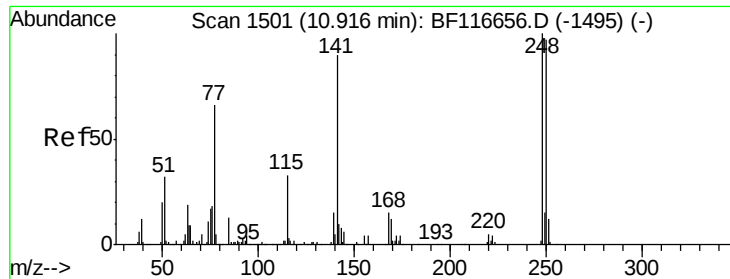




#67
4-Bromophenyl-phenylether
Concen: 4.221 ng
RT: 10.67 min Scan# 1459
Delta R.T. -0.25 min
Lab File: BF116795.D
Acq: 4 Sep 2019 2:20

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 20242
Ion Ratio Lower Upper
248 100
250 196.4 77.8 116.8#
141 631.5 75.9 113.9#

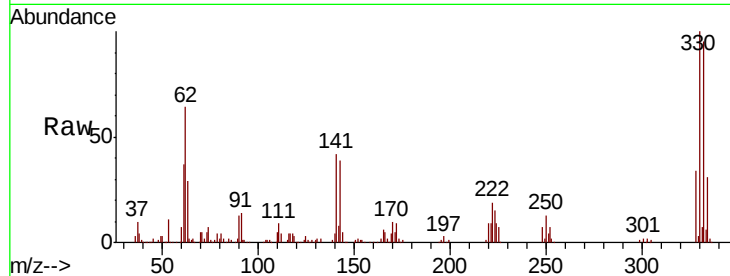


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

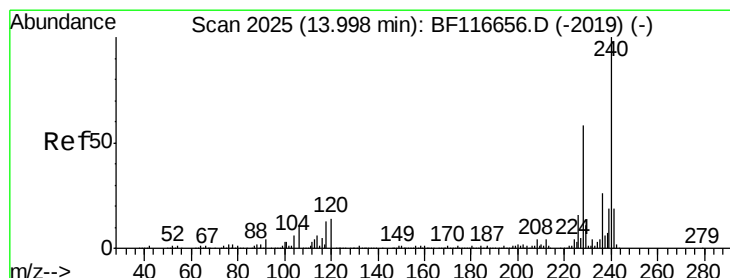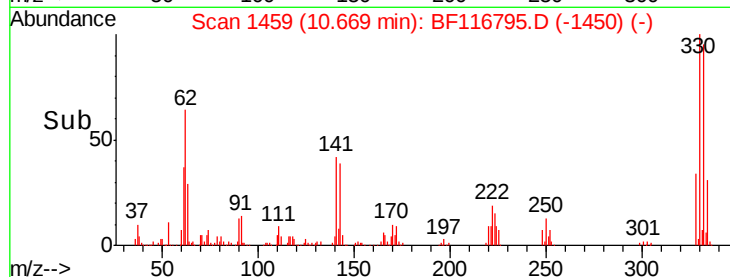
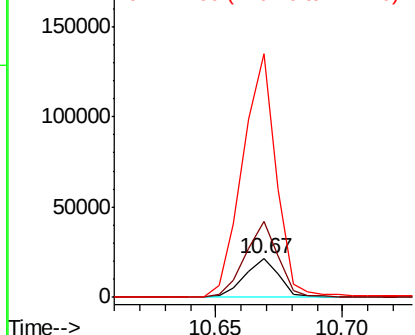


#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.99 min Scan# 2024
Delta R.T. -0.01 min
Lab File: BF116795.D
Acq: 4 Sep 2019 2:20

Tgt Ion:240 Resp: 308631
Ion Ratio Lower Upper
240 100
120 13.9 9.1 13.7#
236 26.5 21.1 31.7

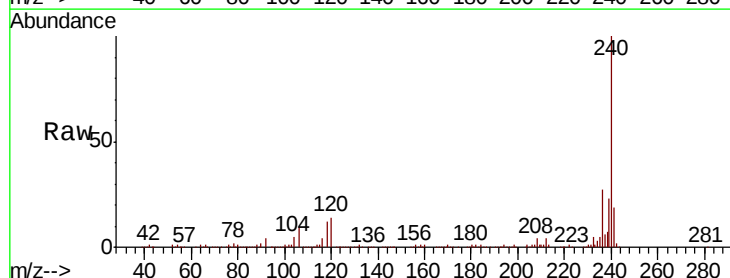

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

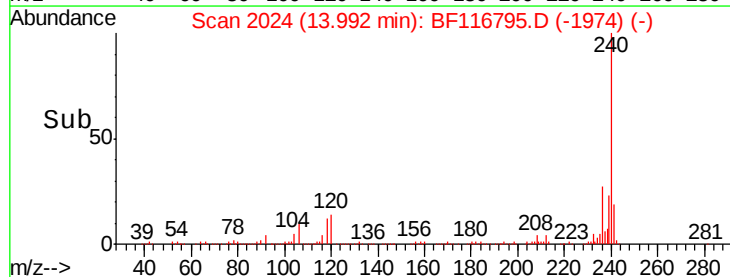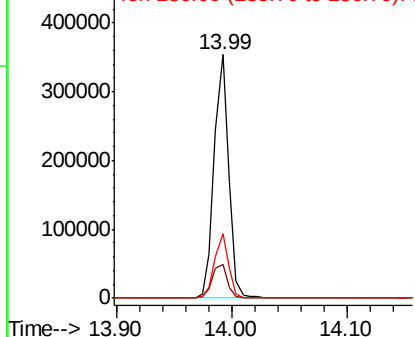



#79

Terphenyl-d14

Concen: 94.946 ng

RT: 12.95 min Scan# 1846

Delta R.T. -0.01 min

Lab File: BF116795.D

Acq: 4 Sep 2019 2:20

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 1584004

Ion Ratio Lower Upper

244 100

212 7.1 6.1 9.1




122 16.1 10.2 15.4#

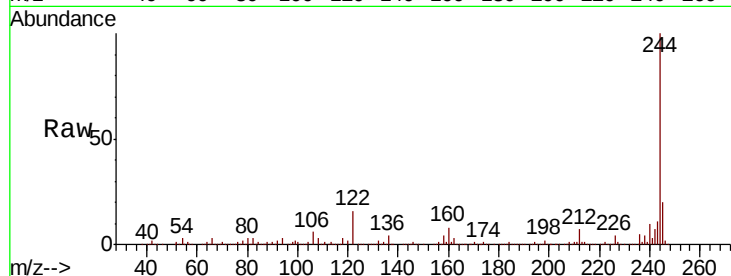

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

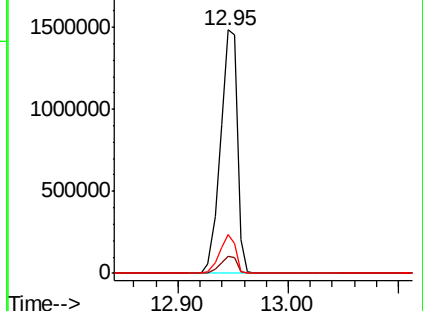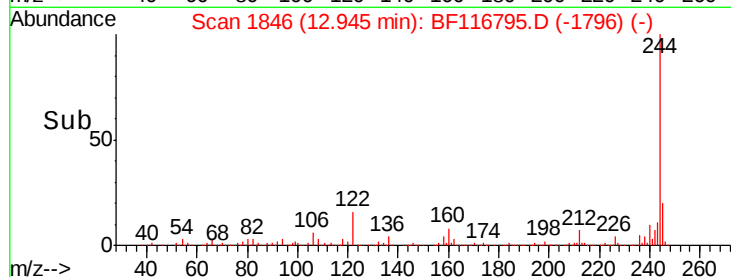

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.44 min Scan# 2271

Delta R.T. 0.00 min

Lab File: BF116795.D

Acq: 4 Sep 2019 2:20


Tgt Ion:264 Resp: 324209

Ion Ratio Lower Upper

264 100

260 23.2 18.3 27.5

265 21.5 16.5 24.7



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

