

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090319\
 Data File : BF116801.D
 Acq On : 4 Sep 2019 5:00
 Operator : HP/JU
 Sample : K4643-30
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 04 06:09:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 30 20:02:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	139665	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	553424	20.00	ng	0.00
39) Acenaphthene-d10	9.88	164	283785	20.00	ng	0.00
64) Phenanthrene-d10	11.36	188	482211	20.00	ng	0.00
76) Chrysene-d12	13.99	240	329902	20.00	ng	0.00
87) Perylene-d12	15.44	264	340407	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	966796	112.14	ng	0.00
7) Phenol-d6	6.48	99	1183305	104.53	ng	0.00
23) Nitrobenzene-d5	7.40	82	859639	88.67	ng	0.00
42) 2,4,6-Tribromophenol	10.67	330	283969	149.68	ng	0.00
45) 2-Fluorobiphenyl	9.20	172	1447343	86.03	ng	0.00
79) Terphenyl-d14	12.94	244	1513226	84.85	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.40	70	111686	14.984	ng	# 71
25) Isophorone	7.40	82	859618	43.760	ng	# 66
50) Dimethylphthalate	9.59	163	136832	6.984	ng	# 99
57) 2,4-Dinitrotoluene	9.88	165	35888	7.852	ng	# 21
65) 4,6-Dinitro-2-methylphenol	10.67	198	465	7.672	ng	# 1
67) 4-Bromophenyl-phenylether	10.67	248	18950	3.868	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090319\
Data File : BF116801.D
Acq On : 4 Sep 2019 5:00
Operator : HP/JU
Sample : K4643-30
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 04 06:09:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

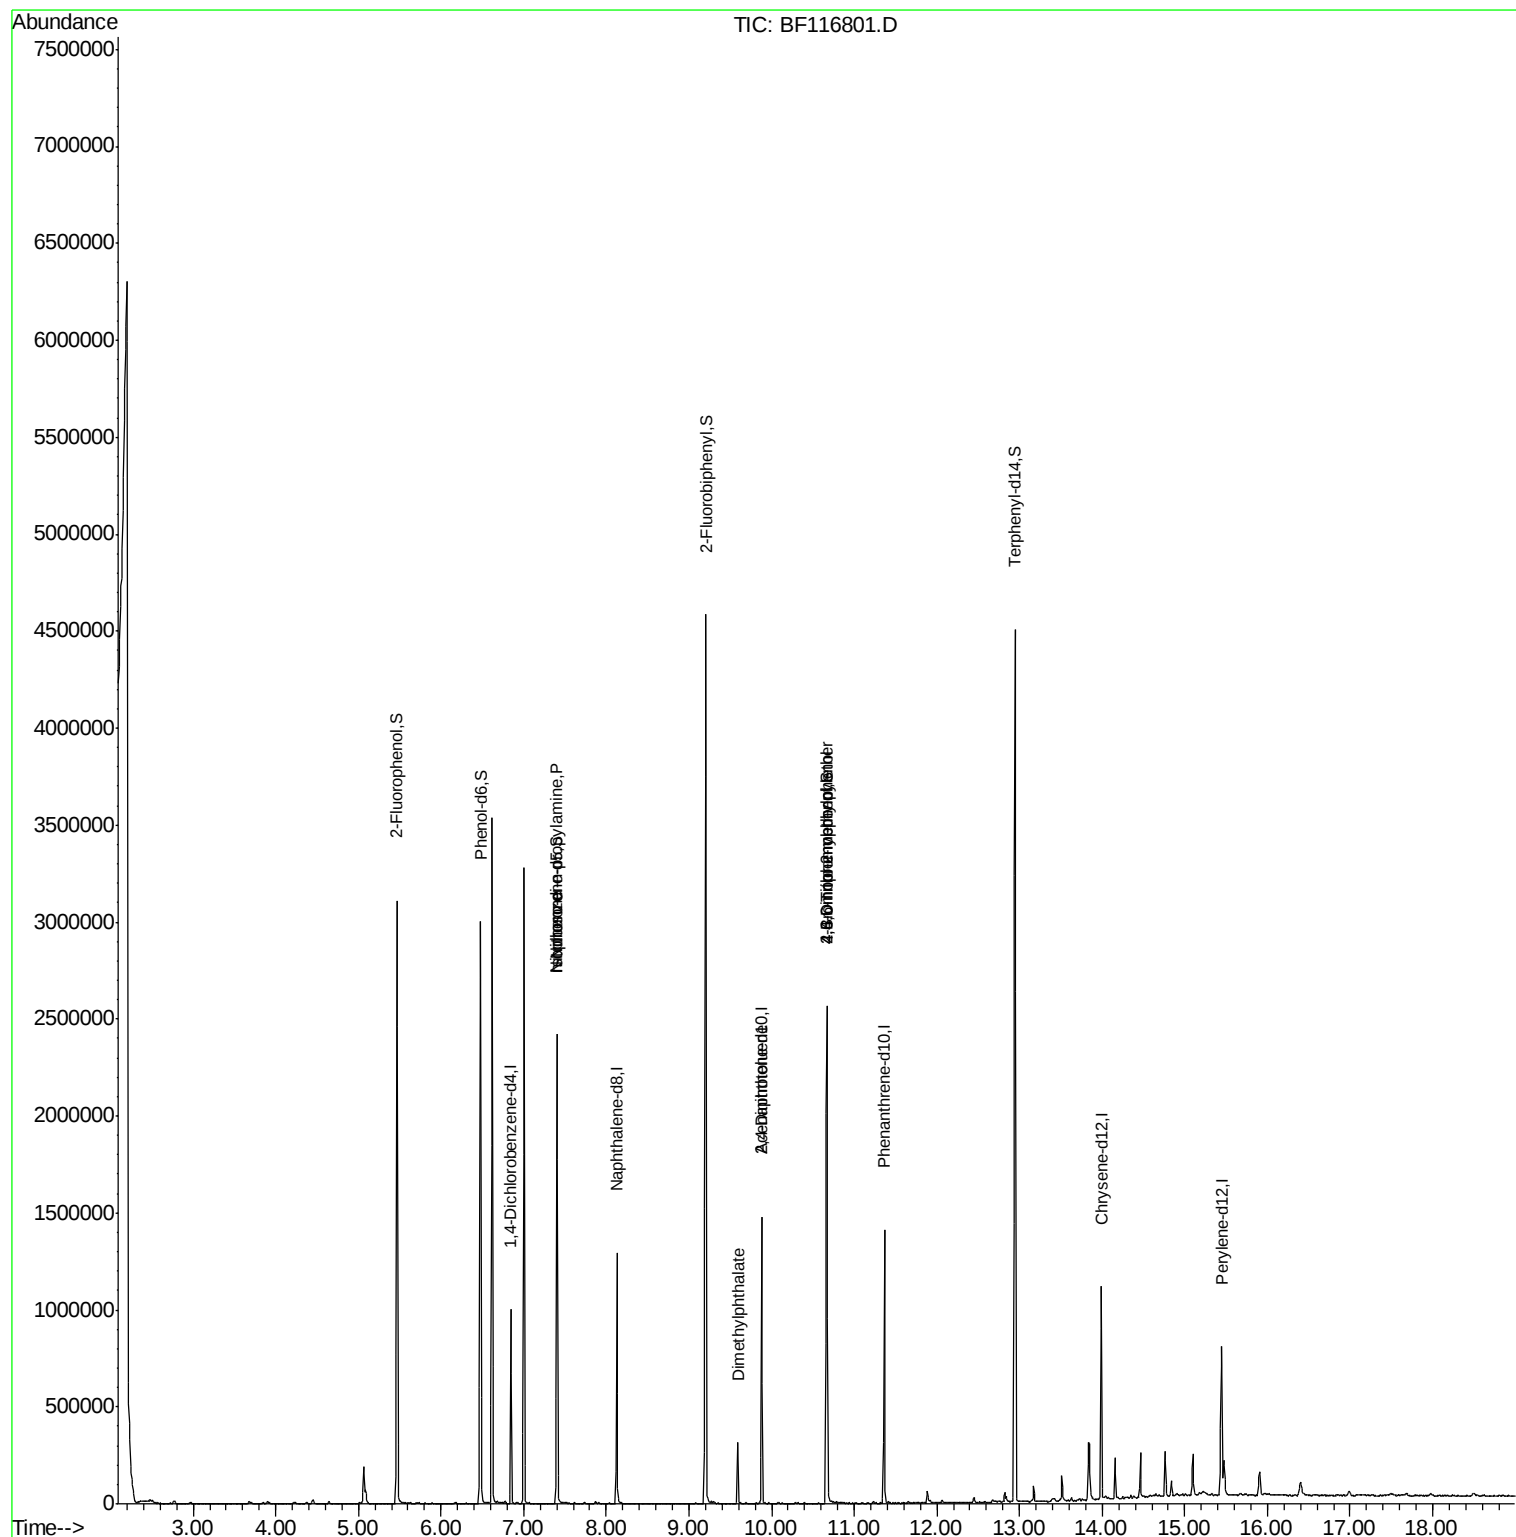




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.85 min Scan# 809
Delta R.T. -0.01 min
Lab File: BF116801.D
Acq: 4 Sep 2019 5:00

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.5	124.4	186.6
115	62.9	49.9	74.9


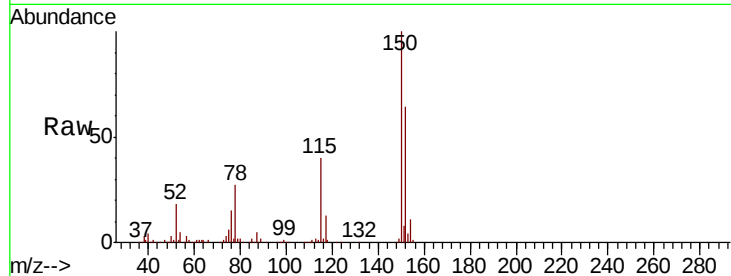


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

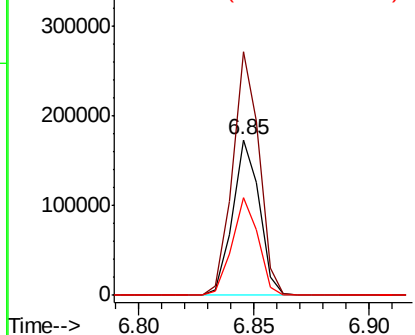

#5

2-Fluorophenol
Concen: 112.144 ng
RT: 5.47 min Scan# 575
Delta R.T. 0.01 min
Lab File: BF116801.D
Acq: 4 Sep 2019 5:00

Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.7	47.1	70.7
63	29.0	24.9	37.3






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

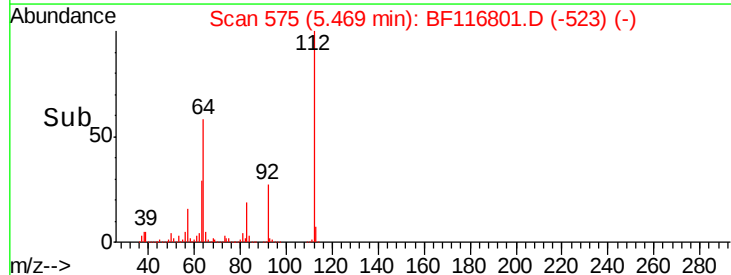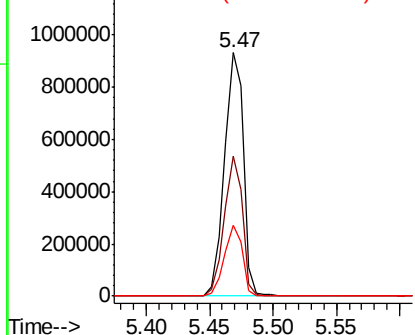



#7

Phenol-d6

Concen: 104.529 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.00 min

Lab File: BF116801.D

Acq: 4 Sep 2019 5:00

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 1183305

Ion Ratio Lower Upper




99 100

42 13.7 13.7 20.5

71 31.5 30.8 46.2

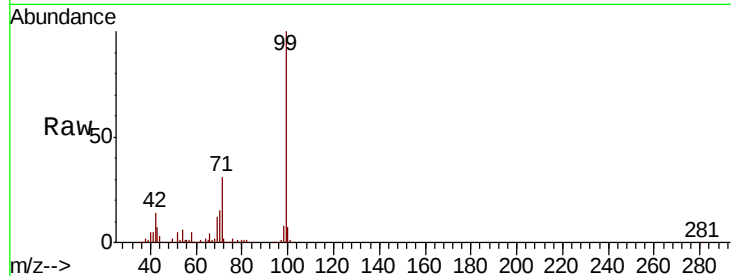

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

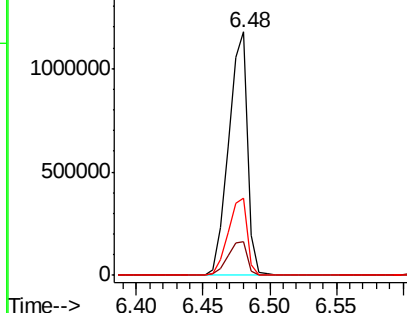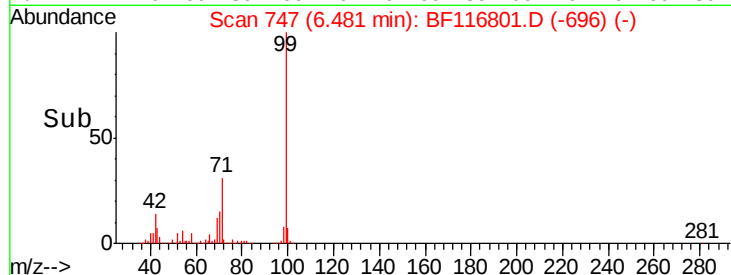

#19

n-Nitroso-di-n-propylamine

Concen: 14.984 ng

RT: 7.40 min Scan# 904

Delta R.T. 0.14 min

Lab File: BF116801.D

Acq: 4 Sep 2019 5:00

Tgt Ion: 70 Resp: 111686


Ion Ratio Lower Upper

70 100



42 36.1 43.5 65.3#

101 0.0 7.8 11.6#

130 2.1 16.6 24.8#

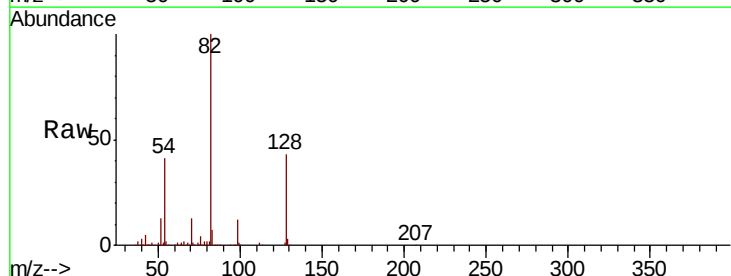

Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): BF1
Ion 130.00 (129.70 to 130.70): BF1

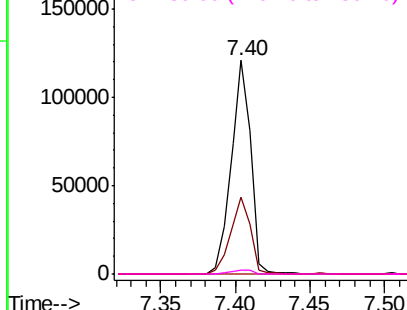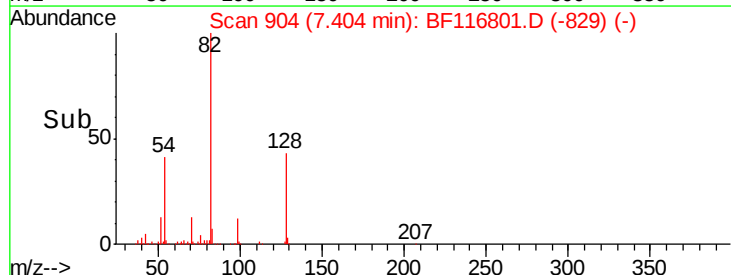







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.13 min Scan# 1027
Delta R.T. -0.01 min
Lab File: BF116801.D
Acq: 4 Sep 2019 5:00

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	553424	
Ion Ratio	Lower	Upper	
136 100			
137 10.9	8.9	13.3	
54 6.0	4.8	7.2	
68 6.0	4.0	6.0	

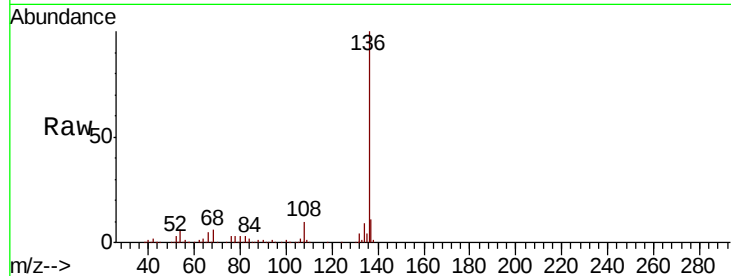


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

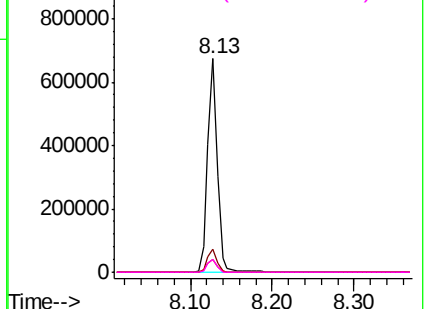




#23
Nitrobenzene-d5
Concen: 88.674 ng
RT: 7.40 min Scan# 904
Delta R.T. -0.01 min
Lab File: BF116801.D
Acq: 4 Sep 2019 5:00

Tgt	Ion: 82	Resp:	859639
Ion	Ratio	Lower	Upper
82	100		
128	43.4	32.8	49.2
54	41.1	36.9	55.3

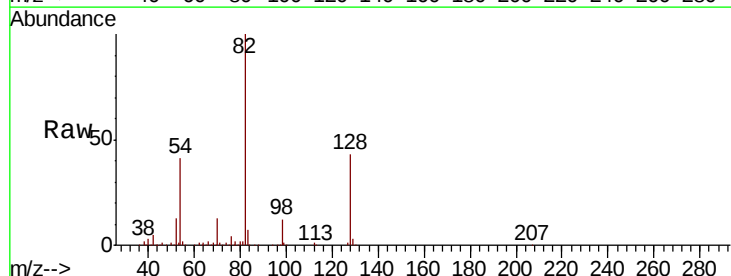

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

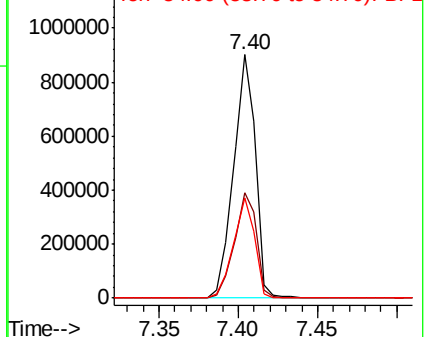



#25

Isophorone

Concen: 43.760 ng

RT: 7.40 min Scan# 904

Delta R.T. -0.26 min

Lab File: BF116801.D

Acq: 4 Sep 2019 5:00

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 859618

Ion Ratio Lower Upper

82 100

95 0.0 5.8 8.6#




138 0.0 13.5 20.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

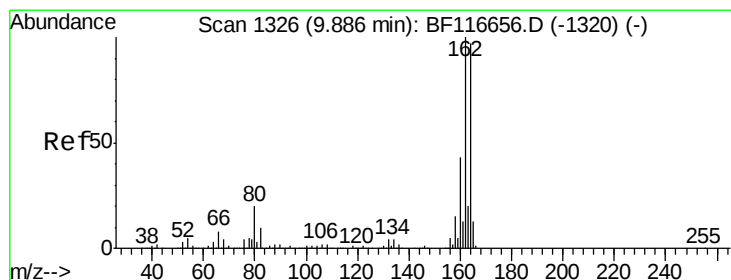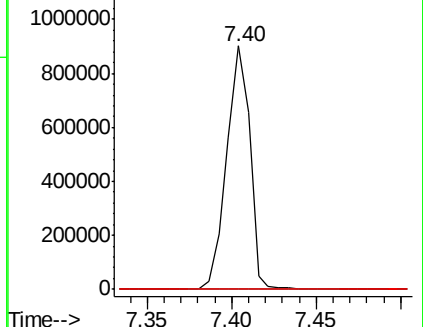

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.88 min Scan# 1325

Delta R.T. -0.01 min

Lab File: BF116801.D

Acq: 4 Sep 2019 5:00


Tgt Ion: 164 Resp: 283785

Ion Ratio Lower Upper

164 100

162 103.3 81.4 122.0



160 43.3 35.4 53.2




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

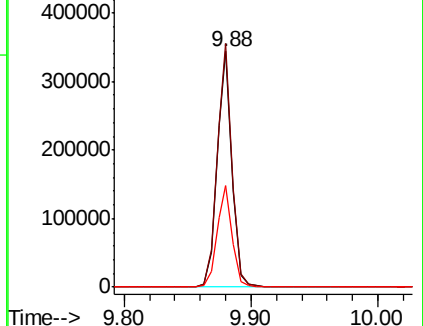


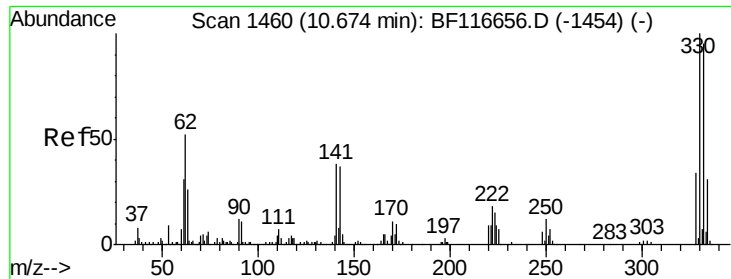

#42
 2,4,6-Tribromophenol
 Concen: 149.681 ng
 RT: 10.67 min Scan# 1459
 Delta R.T. -0.01 min
 Lab File: BF116801.D
 Acq: 4 Sep 2019 5:00

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.8	76.9	115.3
141	40.9	31.4	47.2






Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

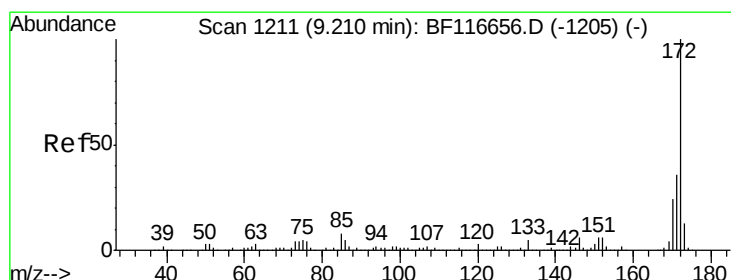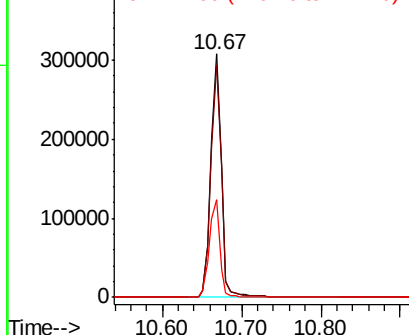

#45
 2-Fluorobiphenyl
 Concen: 86.034 ng
 RT: 9.20 min Scan# 1210
 Delta R.T. -0.01 min
 Lab File: BF116801.D
 Acq: 4 Sep 2019 5:00

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.0	27.8	41.6
170	24.0	18.9	28.3


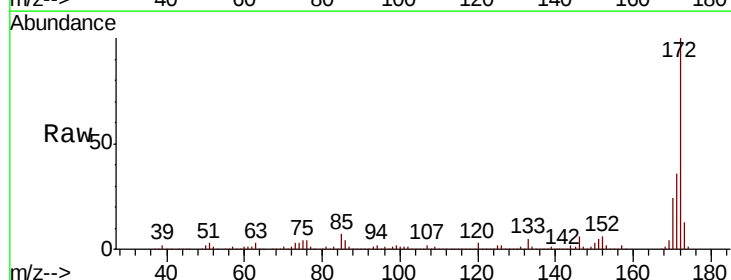



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

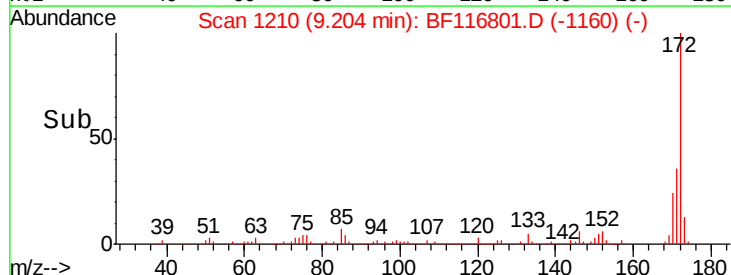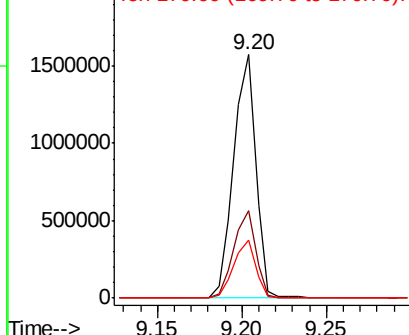

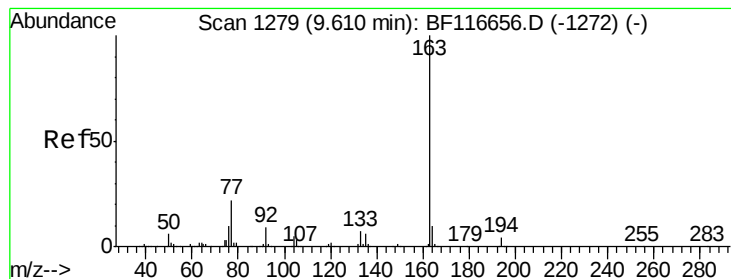

#50

Dimethylphthalate

Concen: 6.984 ng

RT: 9.59 min Scan# 1276

Delta R.T. -0.02 min

Lab File: BF116801.D

Acq: 4 Sep 2019 5:00

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 136832

Ion Ratio Lower Upper

163 100

194 3.7 2.8 4.2




164 10.4 8.6 12.8



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

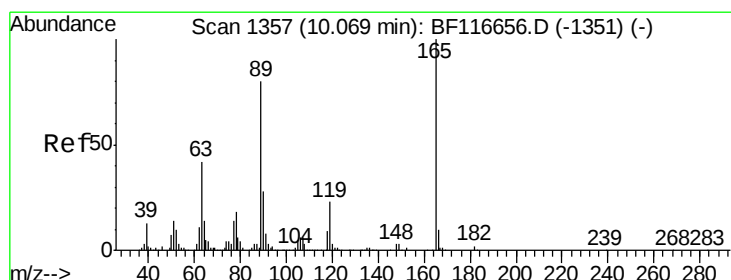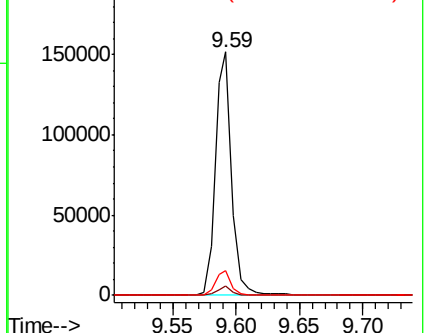

#57

2,4-Dinitrotoluene

Concen: 7.852 ng

RT: 9.88 min Scan# 1325

Delta R.T. -0.19 min

Lab File: BF116801.D

Acq: 4 Sep 2019 5:00

Tgt Ion:165 Resp: 35888


Ion Ratio Lower Upper

165 100

63 1.1 36.4 54.6#

89 1.5 62.6 94.0#

182 0.0 2.1 3.1#





Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

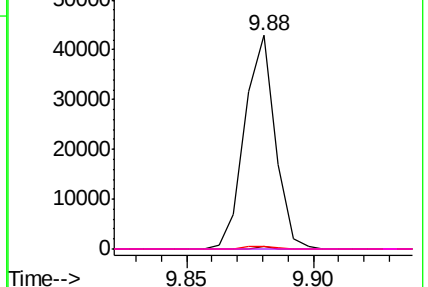







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1577
Delta R.T. -0.01 min
Lab File: BF116801.D
Acq: 4 Sep 2019 5:00

Instrument :
BNA_F
ClientSampleId :

Tot Ion:188 Resp: 482211
Ion Ratio Lower Upper
188 100
94 10.8 7.3 10.9
80 11.4 8.4 12.6




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1


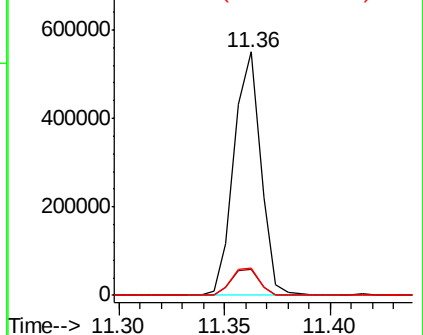



#65
4,6-Dinitro-2-methylphenol
Concen: 7.672 ng
RT: 10.67 min Scan# 1459
Delta R.T. 0.19 min
Lab File: BF116801.D
Acq: 4 Sep 2019 5:00

Tgt Ion:198 Resp: 465
Ion Ratio Lower Upper
198 100
51 154.9 18.4 58.4#
105 207.3 22.9 62.9#



Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF1
Ion 105.00 (104.70 to 105.70): E

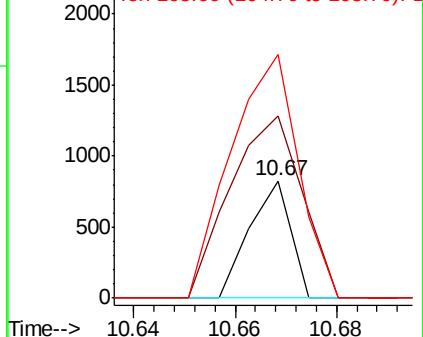


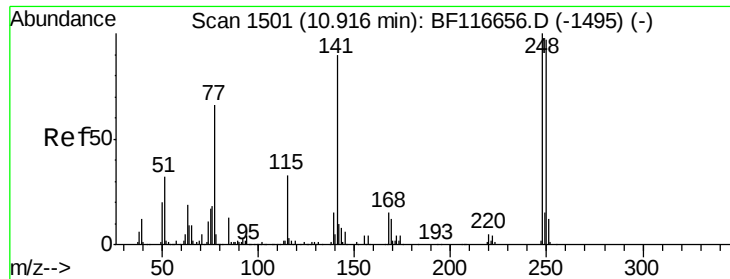




#67
4-Bromophenyl-phenylether
Concen: 3.868 ng
RT: 10.67 min Scan# 1459
Delta R.T. -0.25 min
Lab File: BF116801.D
Acq: 4 Sep 2019 5:00

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 18950
Ion Ratio Lower Upper
248 100
250 183.5 77.8 116.8#
141 567.4 75.9 113.9#

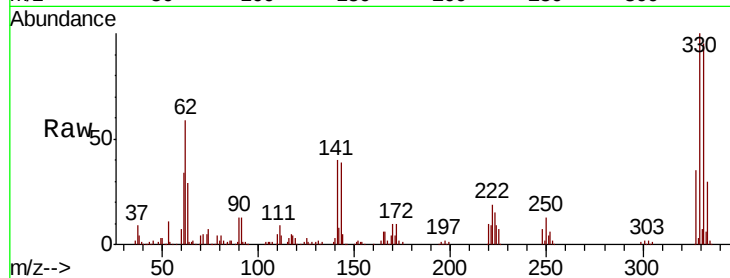


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

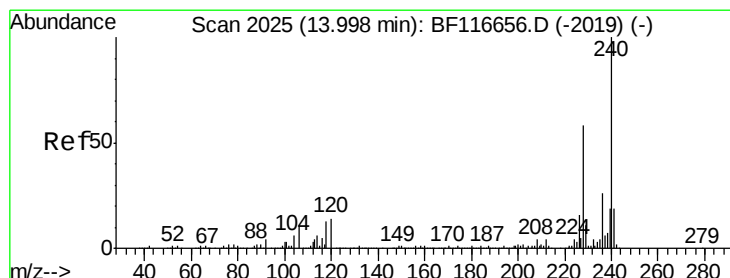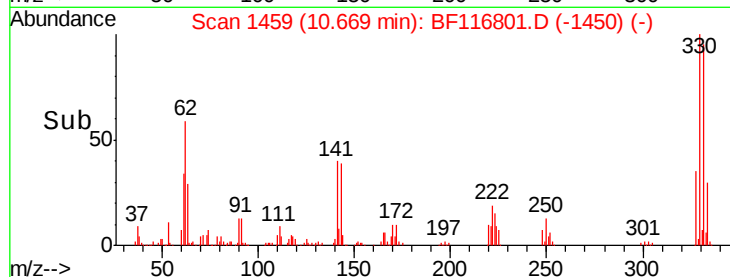
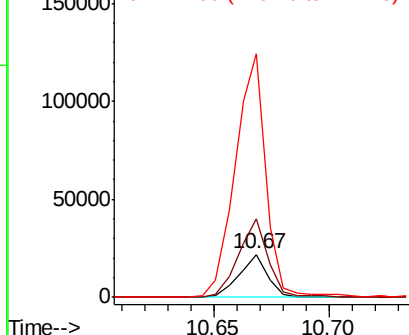


#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.99 min Scan# 2024
Delta R.T. -0.01 min
Lab File: BF116801.D
Acq: 4 Sep 2019 5:00

Tgt Ion:240 Resp: 329902
Ion Ratio Lower Upper
240 100
120 13.3 9.1 13.7
236 26.3 21.1 31.7

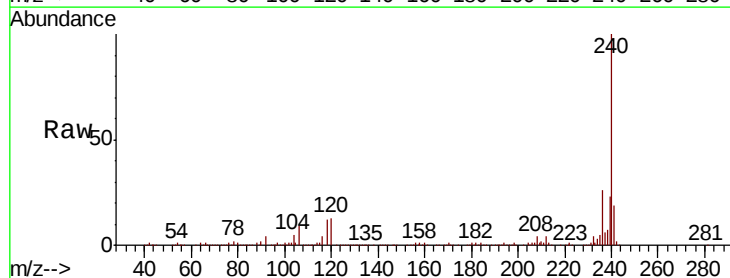

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



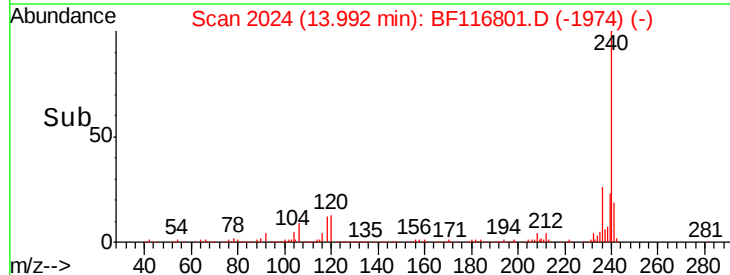
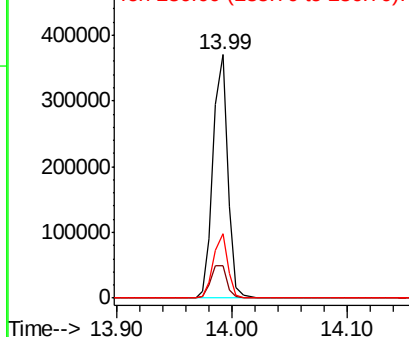




#79
 Terphenyl-d14
 Concen: 84.855 ng
 RT: 12.94 min Scan# 1846
 Delta R.T. -0.01 min
 Lab File: BF116801.D
 Acq: 4 Sep 2019 5:00

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:244 Resp: 1513226
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.1 9.1
 122 15.7 10.2 15.4#

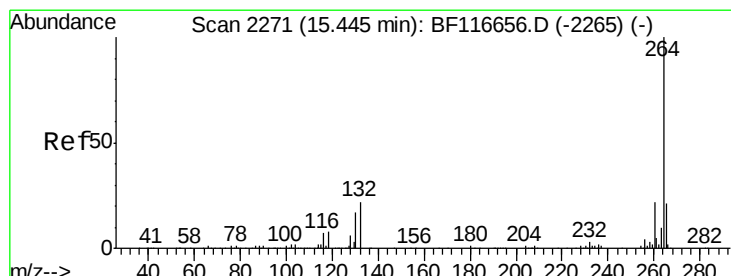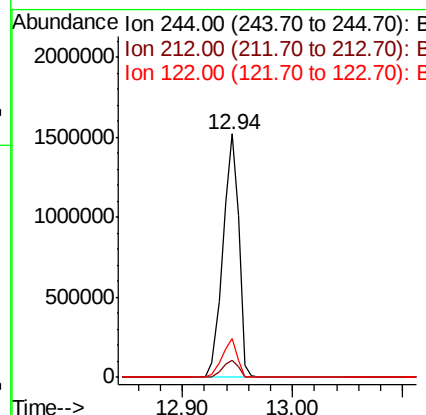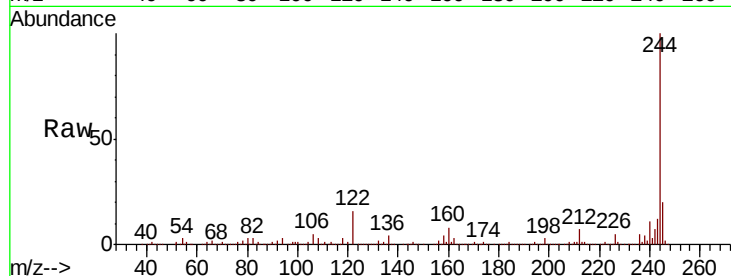

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.44 min Scan# 2271
 Delta R.T. -0.00 min
 Lab File: BF116801.D
 Acq: 4 Sep 2019 5:00

Tgt Ion:264 Resp: 340407
 Ion Ratio Lower Upper
 264 100
 260 24.2 18.3 27.5
 265 22.4 16.5 24.7

