


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090319\
 Data File : BF116763.D
 Acq On : 3 Sep 2019 10:40
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 20:02:30 2019

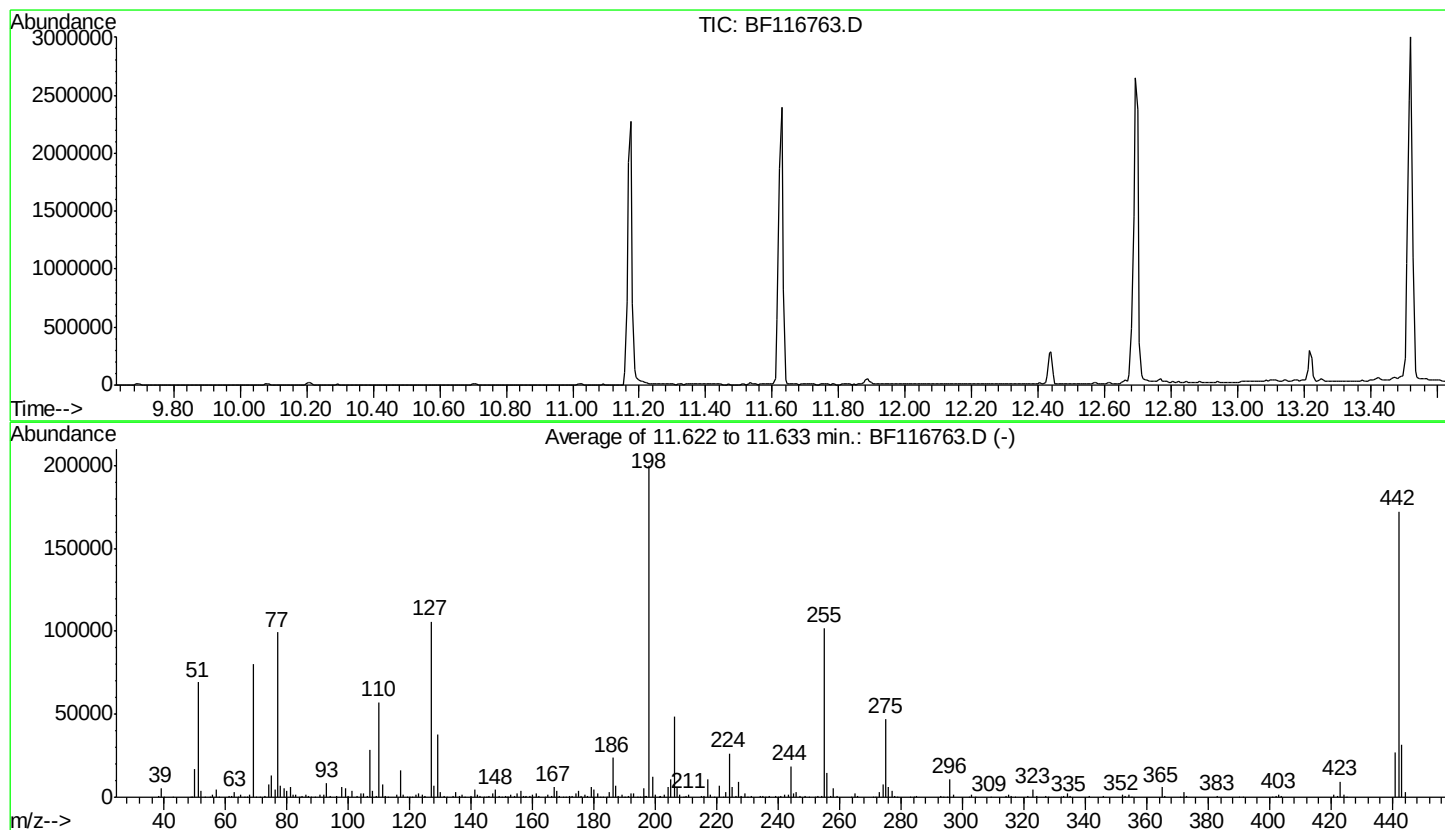

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	69437	PASS
68	69	0.00	2	1.5	1193	PASS
69	198	0.00	100	40.2	80319	PASS
70	69	0.00	2	0.1	48	PASS
127	198	10	80	52.9	105874	PASS
197	198	0.00	2	0.5	928	PASS
198	198	100	100	100.0	199976	PASS
199	198	5	9	6.3	12640	PASS
275	198	10	60	23.7	47453	PASS
365	198	1	100	3.0	5992	PASS
441	198	0.01	100	13.4	26698	PASS
442	198	50	100	86.2	172453	PASS
443	442	15	24	18.2	31333	PASS