

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090419\
 Data File : BF116818.D
 Acq On : 4 Sep 2019 16:27
 Operator : HP/JU
 Sample : K4601-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T12-F1-F4-(0-2.7)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	570	575	578	rBV	1705064	1555886	77.91%	10.214%
2	6.481	742	747	755	rBV	1765945	1794381	89.85%	11.779%
3	6.622	766	771	774	rBV	2030626	1775463	88.91%	11.655%
4	6.845	806	809	813	rBV	483240	435319	21.80%	2.858%
5	7.004	832	836	840	rBV	1545970	1339836	67.09%	8.795%
6	7.404	899	904	907	rBV	1106913	1077967	53.98%	7.076%
7	8.127	1023	1027	1030	rBV	697919	571091	28.60%	3.749%
8	8.839	1146	1148	1154	rVB	46778	41090	2.06%	0.270%
9	9.204	1206	1210	1213	rBV	2515309	1996984	100.00%	13.109%
10	9.592	1273	1276	1280	rBV	219162	171924	8.61%	1.129%
11	9.880	1319	1325	1329	rBV	790652	665725	33.34%	4.370%
12	10.080	1356	1359	1363	rBV2	36368	41564	2.08%	0.273%
13	10.292	1393	1395	1397	rBV3	28549	30763	1.54%	0.202%
14	10.357	1402	1406	1408	rBV4	36534	58035	2.91%	0.381%
15	10.669	1455	1459	1462	rBV	1105696	1022367	51.20%	6.711%
16	11.368	1575	1578	1580	rBV	510120	442794	22.17%	2.907%
17	12.951	1844	1847	1850	rVB	1325105	1208952	60.54%	7.936%
18	14.004	2024	2026	2029	rVB	427698	333040	16.68%	2.186%
19	15.033	2198	2201	2209	rVB	168300	294487	14.75%	1.933%
20	15.456	2269	2273	2276	rBV	317388	375578	18.81%	2.466%


Sum of corrected areas: 15233246

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090419\
Data File : BF116818.D
Acq On : 4 Sep 2019 16:27
Operator : HP/JU
Sample : K4601-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T12-F1-F4-(0-2.7)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

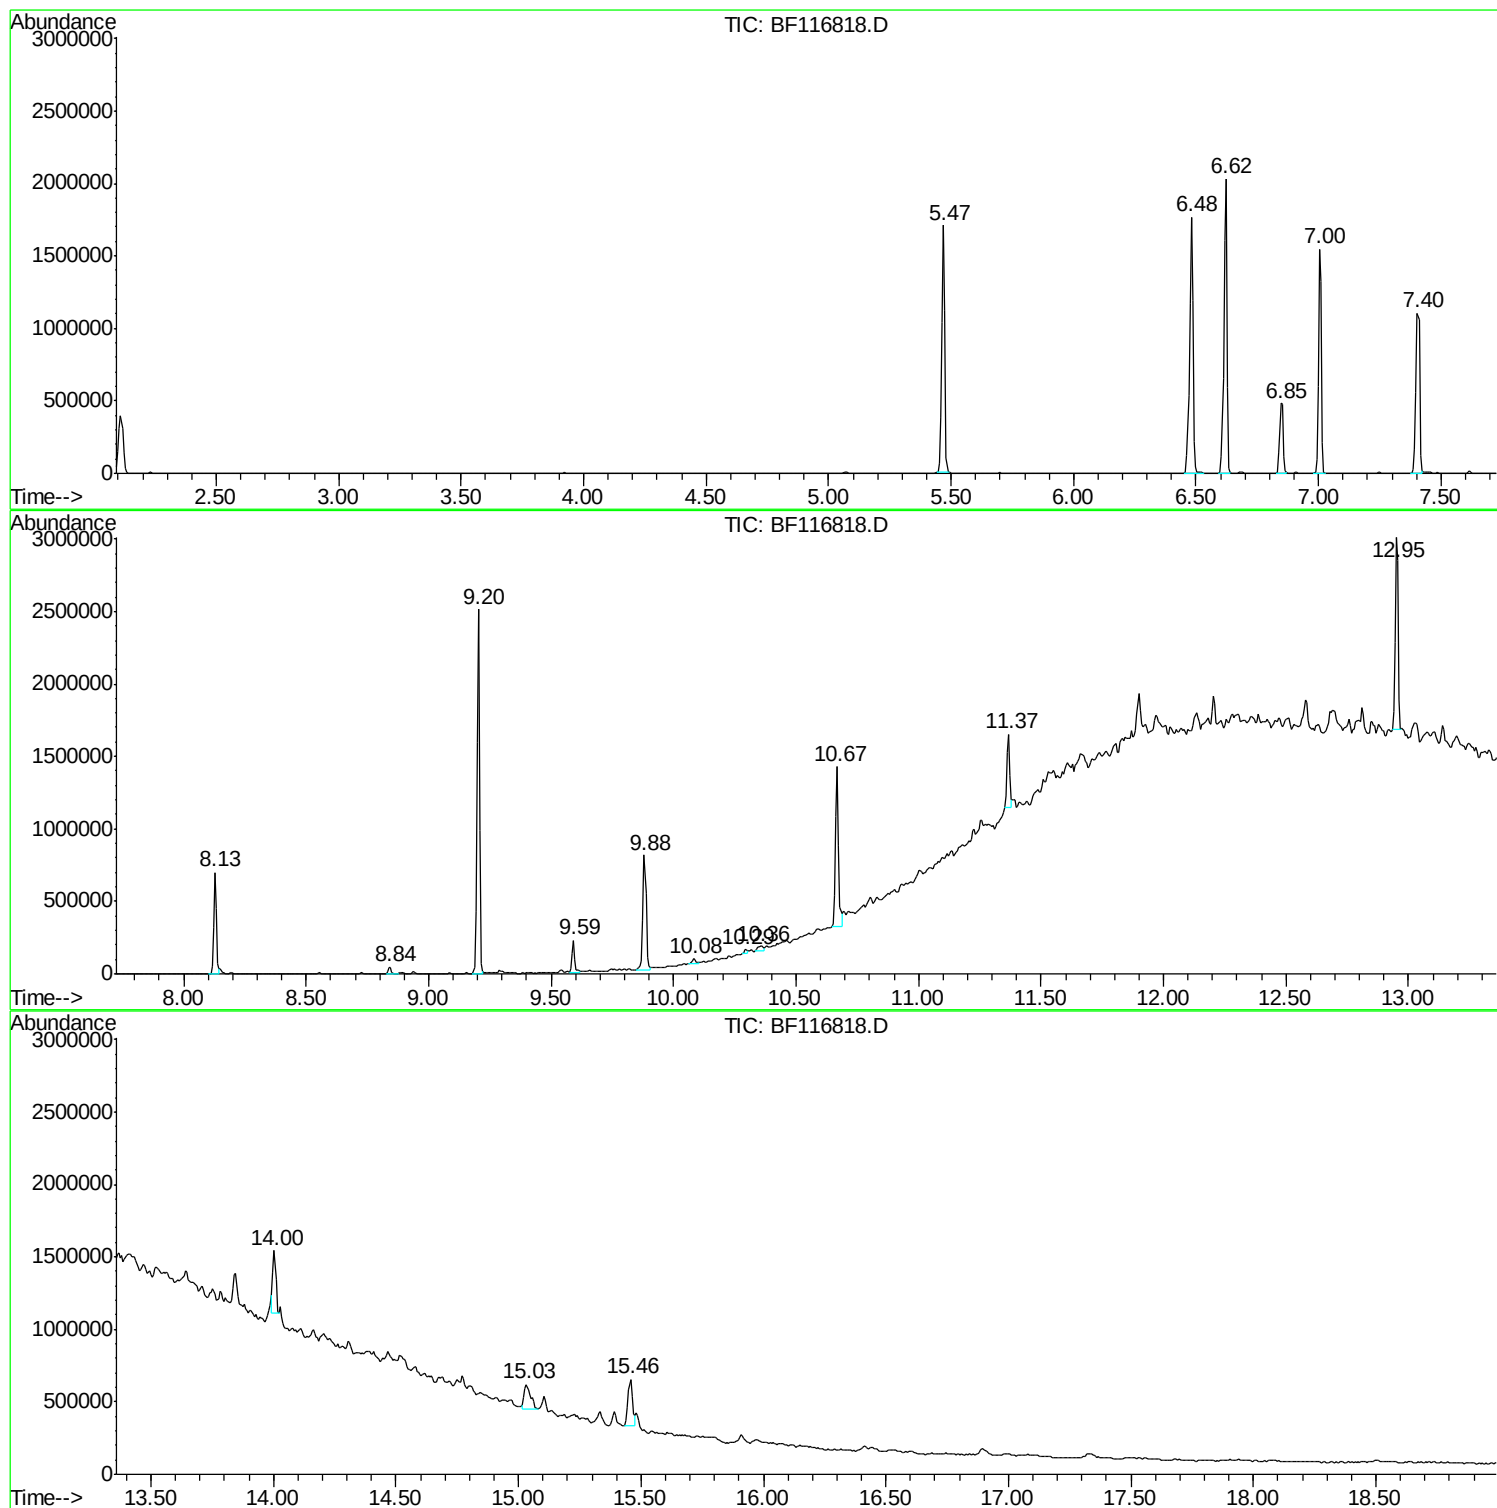

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090419\
Data File : BF116818.D
Acq On : 4 Sep 2019 16:27
Operator : HP/JU
Sample : K4601-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T12-F1-F4-(0-2.7)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	81.57 ng	1775460	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
4		Xenon	132	Xe	007440-63-3	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

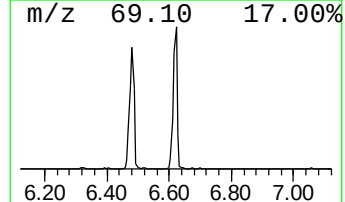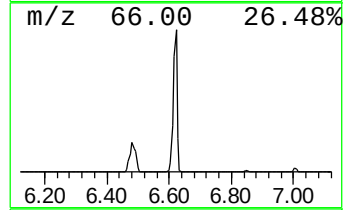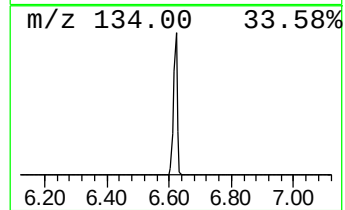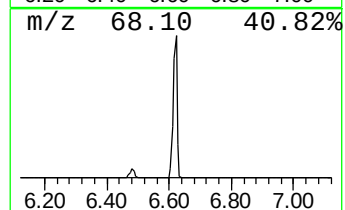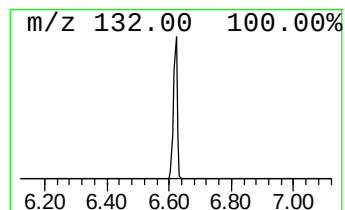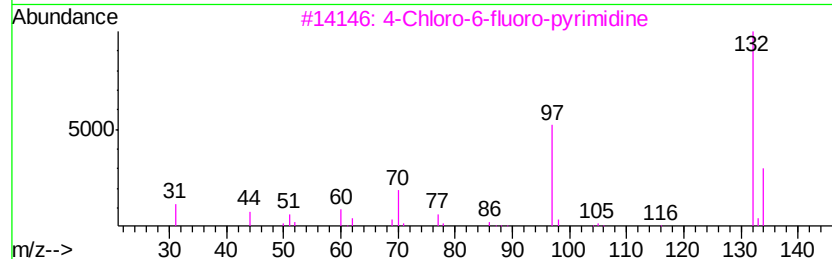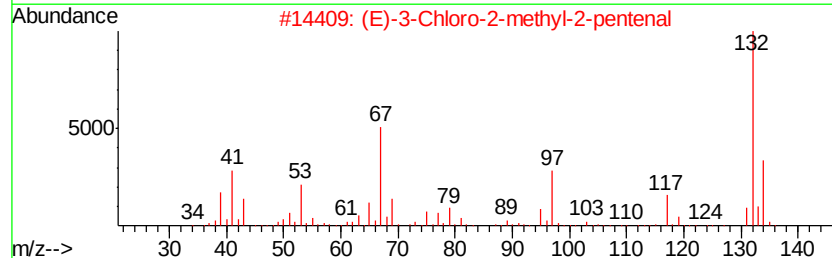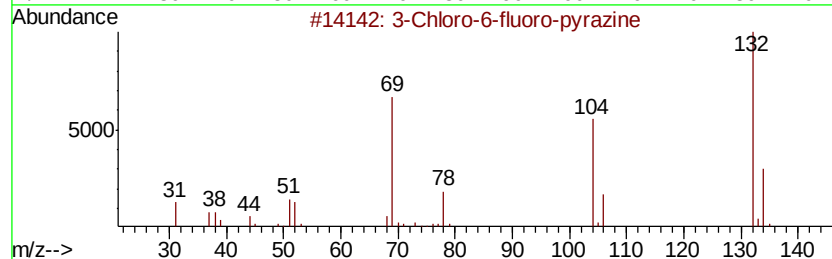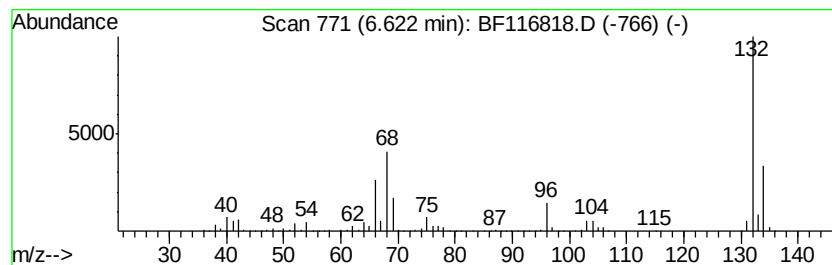

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090419\
Data File : BF116818.D
Acq On : 4 Sep 2019 16:27
Operator : HP/JU
Sample : K4601-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T12-F1-F4-(0-2.7)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.62	6.62	81.6	ng	1775460	1	6.85	435319	20.0