


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090419\
 Data File : BF116804.D
 Acq On : 4 Sep 2019 10:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 20:02:30 2019

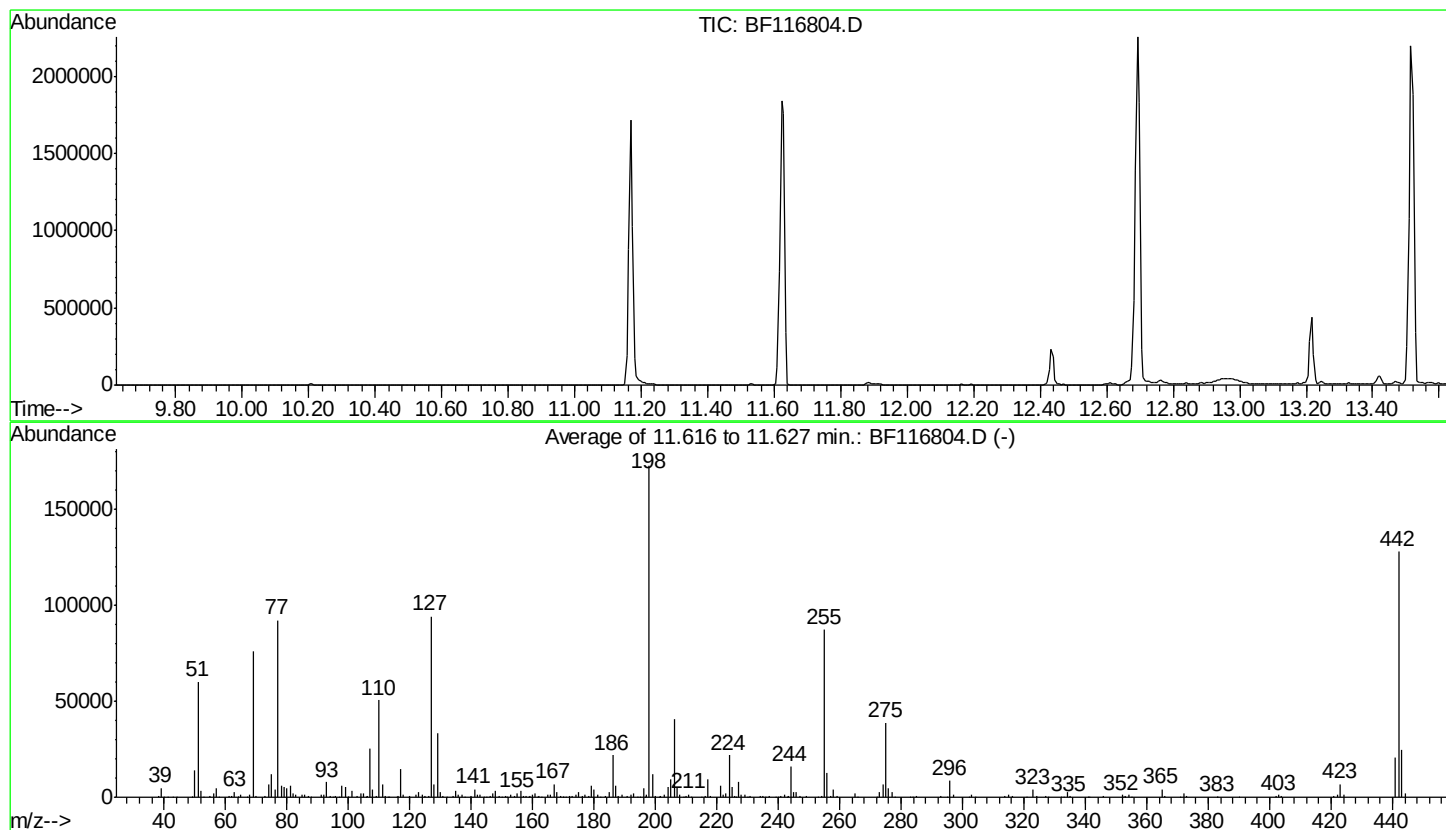

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	60061	PASS
68	69	0.00	2	1.7	1287	PASS
69	198	0.00	100	44.1	76040	PASS
70	69	0.00	2	0.6	470	PASS
127	198	10	80	54.5	94037	PASS
197	198	0.00	2	0.7	1227	PASS
198	198	100	100	100.0	172432	PASS
199	198	5	9	6.9	11907	PASS
275	198	10	60	22.5	38874	PASS
365	198	1	100	2.4	4200	PASS
441	198	0.01	100	11.9	20461	PASS
442	198	50	100	74.1	127728	PASS
443	442	15	24	19.3	24708	PASS