

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090518\
 Data File : BF108821.D
 Acq On : 6 Sep 2018 12:58
 Operator : JU/SJ
 Sample : J4724-14
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 06 14:35:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 05 18:03:31 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	279156	20.00	ng	0.00
21) Naphthalene-d8	8.02	136	1031921	20.00	ng	0.00
38) Acenaphthene-d10	9.77	164	443606	20.00	ng	0.00
63) Phenanthrene-d10	11.24	188	683864	20.00	ng	0.00
75) Chrysene-d12	13.87	240	575040	20.00	ng	0.00
86) Perylene-d12	15.27	264	503411	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	1433167	85.05	ng	0.01
7) Phenol-d6	6.37	99	1822198	84.05	ng	0.00
23) Nitrobenzene-d5	7.30	82	1108610	67.23	ng	0.00
41) 2,4,6-Tribromophenol	10.55	330	341757	80.70	ng	0.00
44) 2-Fluorobiphenyl	9.10	172	1837161	70.65	ng	0.00
78) Terphenyl-d14	12.82	244	1334033	54.10	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.30	70	156414	10.379	ng	# 79
25) Isophorone	7.30	82	1099507	33.429	ng	# 64
32) Benzoic acid	7.68	122	241	4.044	ng	# 60
49) Dimethylphthalate	9.48	163	596428	19.223	ng	100
56) 2,4-Dinitrotoluene	9.77	165	57765	7.640	ng	# 23
64) 4,6-Dinitro-2-methylphenol	10.55	198	734	7.102	ng	# 1
66) 4-Bromophenyl-phenylether	10.55	248	20520	2.657	ng	# 1
83) Bis(2-ethylhexyl)phthalate	13.87	149	143032	5.712	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090518\
Data File : BF108821.D
Acq On : 6 Sep 2018 12:58
Operator : JU/SJ
Sample : J4724-14
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 06 14:35:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 18:03:31 2018
Response via : Initial Calibration

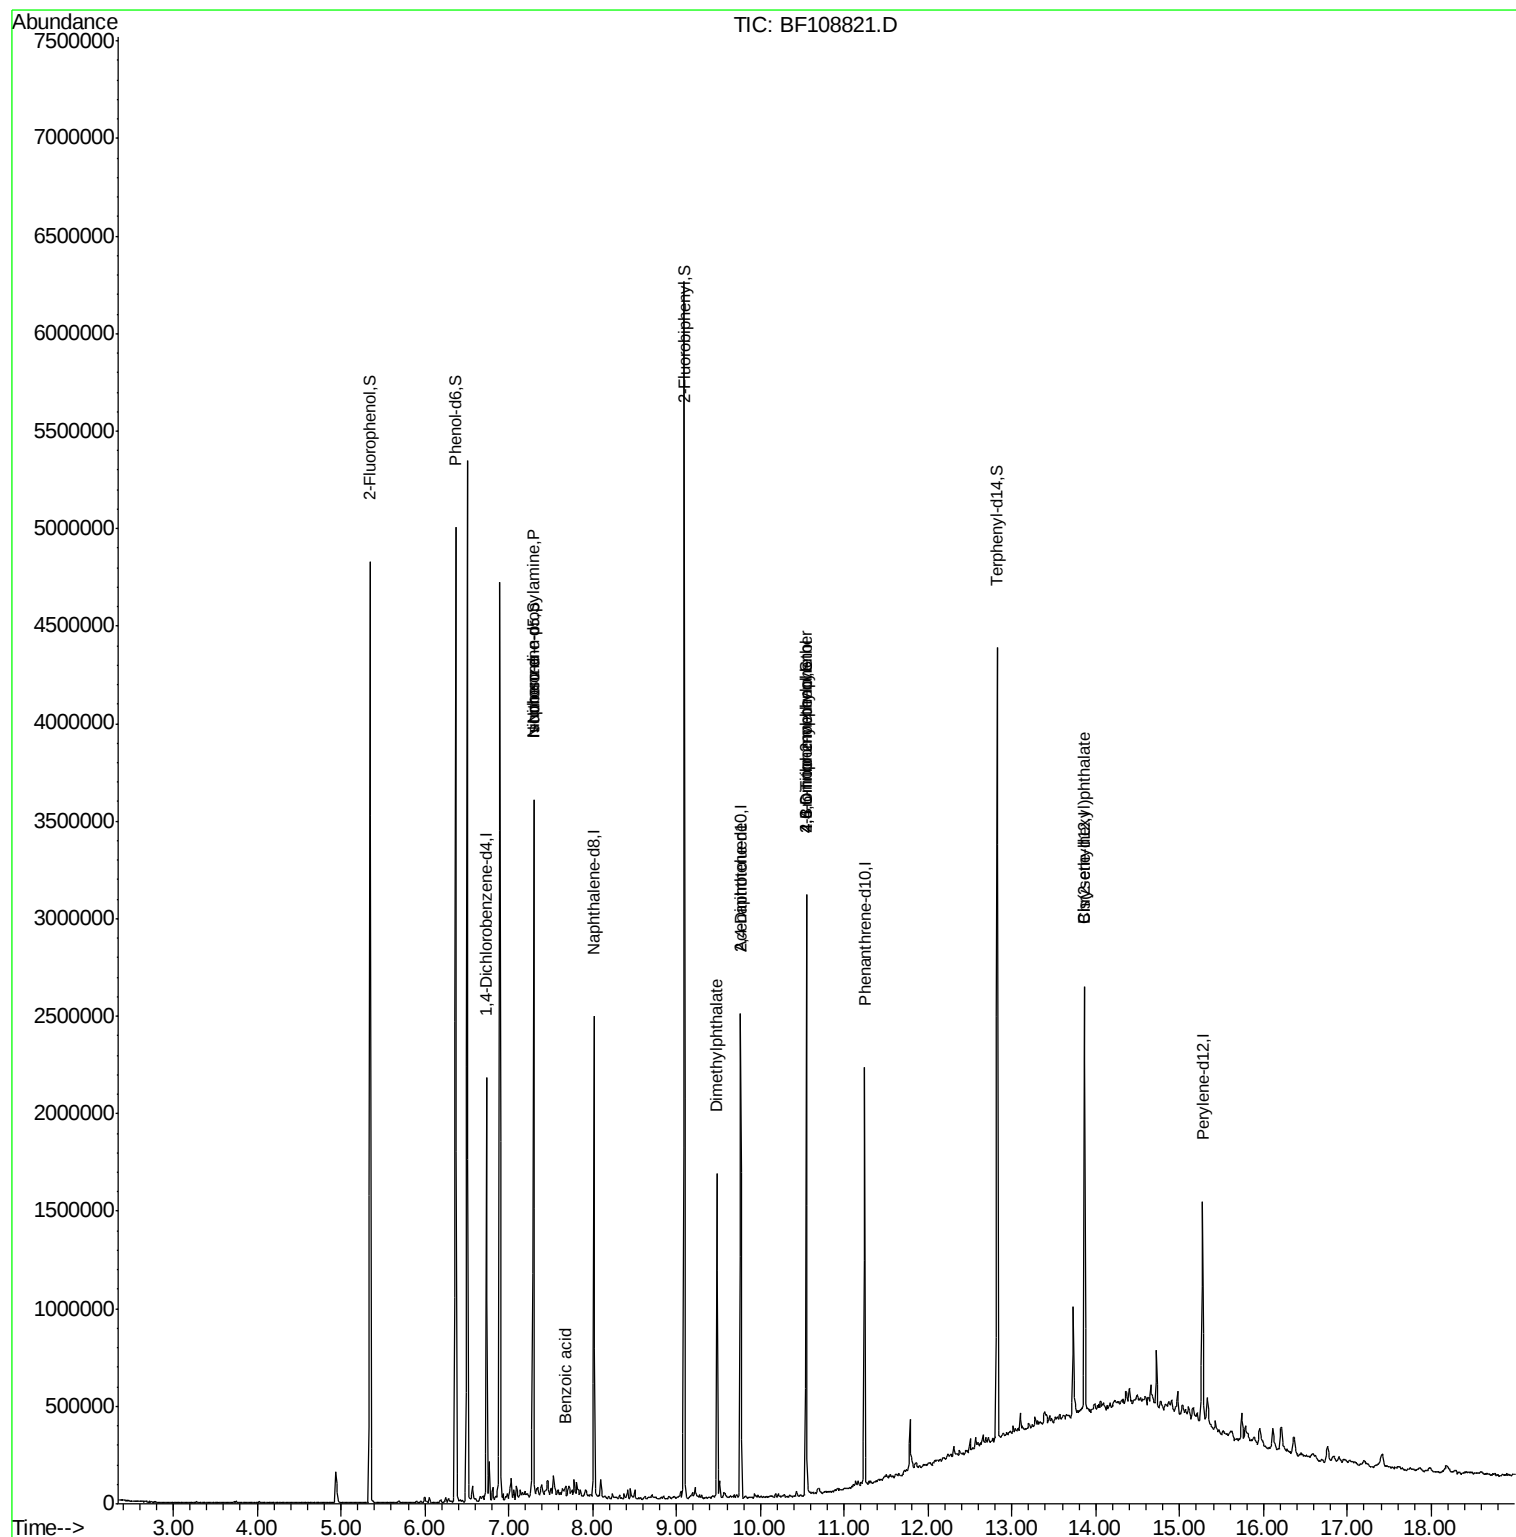

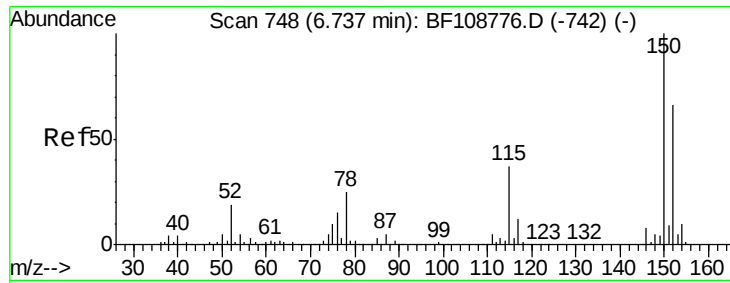


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.74 min Scan# 748
 Delta R.T. -0.00 min
 Lab File: BF108821.D
 Acq: 6 Sep 2018 12:58

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.1	124.6	186.8
115	61.1	50.1	75.1

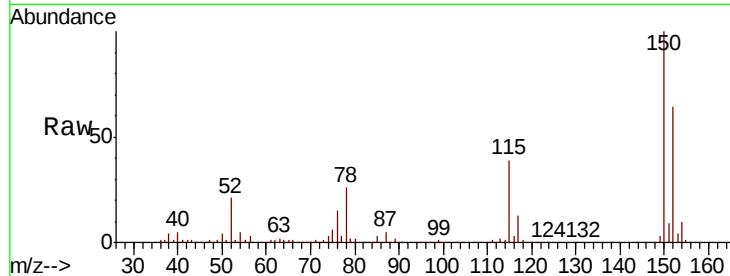


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

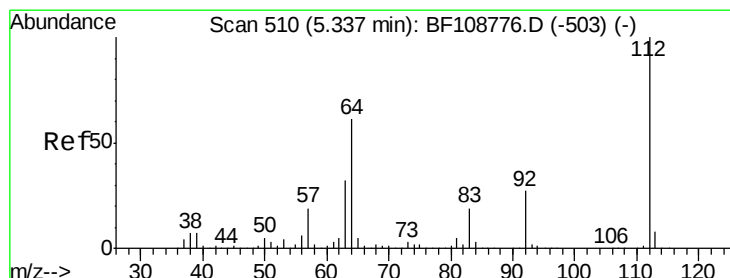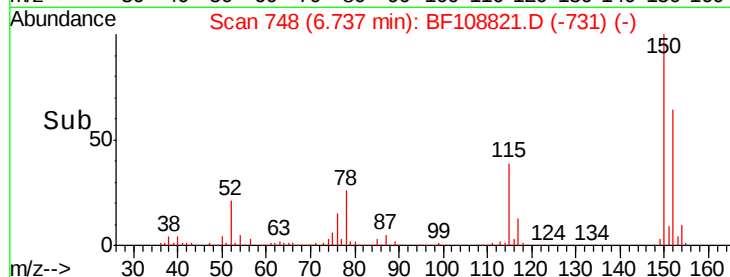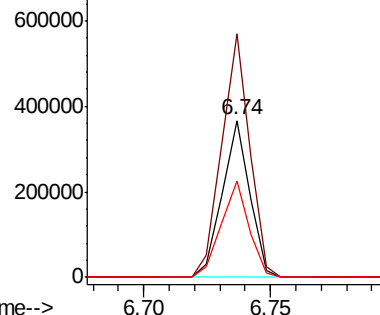



#5


2-Fluorophenol
 Concen: 85.052 ng
 RT: 5.35 min Scan# 512
 Delta R.T. 0.01 min
 Lab File: BF108821.D
 Acq: 6 Sep 2018 12:58

Tgt Ion	Ratio	Lower	Upper
112	100		
64	61.1	47.9	71.9
63	31.4	23.7	35.5

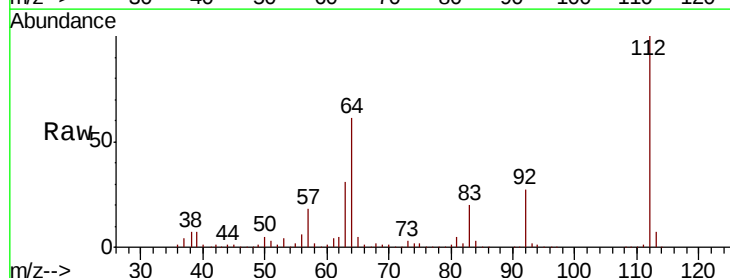

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

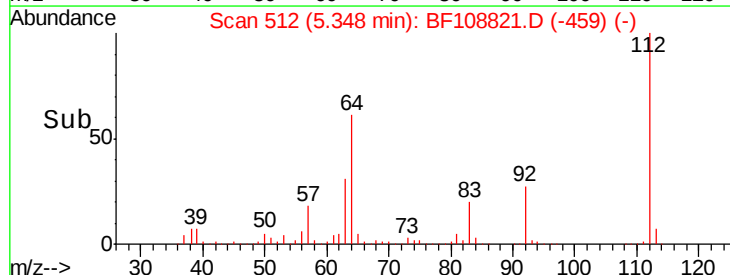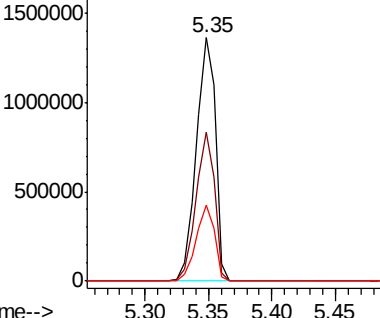

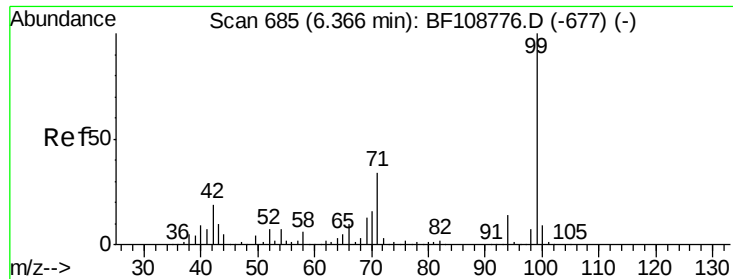

#7

Phenol-d6

Concen: 84.047 ng

RT: 6.37 min Scan# 686

Delta R.T. 0.01 min

Lab File: BF108821.D

Acq: 6 Sep 2018 12:58

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 1822198

Ion Ratio Lower Upper

99 100

42 19.7 14.5 21.7




71 35.1 25.4 38.0

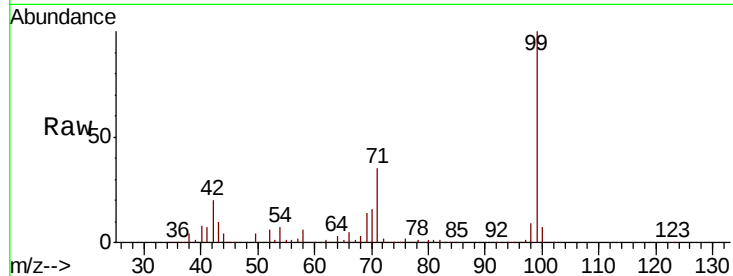

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

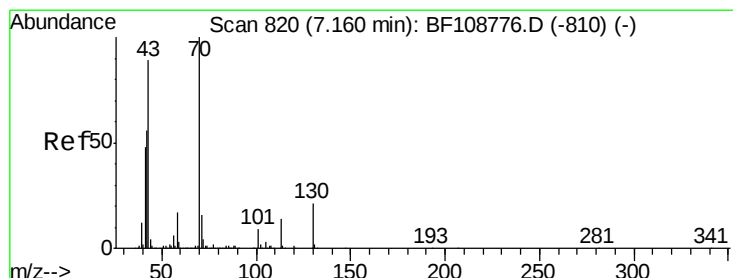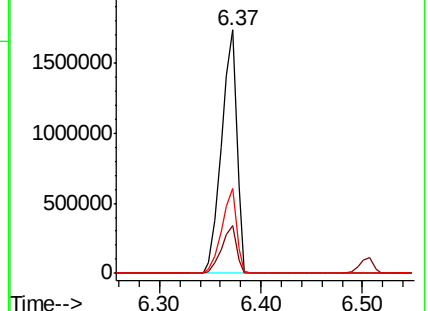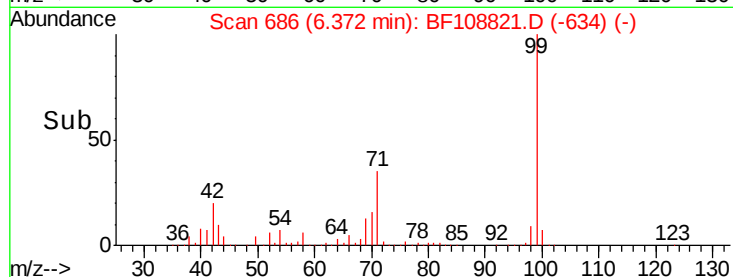

#19

n-Nitroso-di-n-propylamine

Concen: 10.379 ng

RT: 7.30 min Scan# 843

Delta R.T. 0.14 min

Lab File: BF108821.D

Acq: 6 Sep 2018 12:58

Tgt Ion: 70 Resp: 156414


Ion Ratio Lower Upper

70 100

42 48.9 47.5 71.3

101 0.0 7.4 11.2#

130 2.1 16.6 25.0#


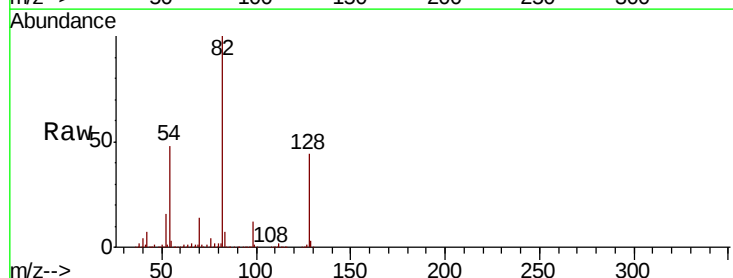


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

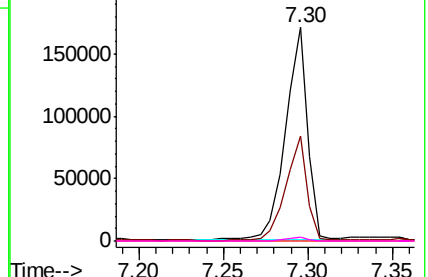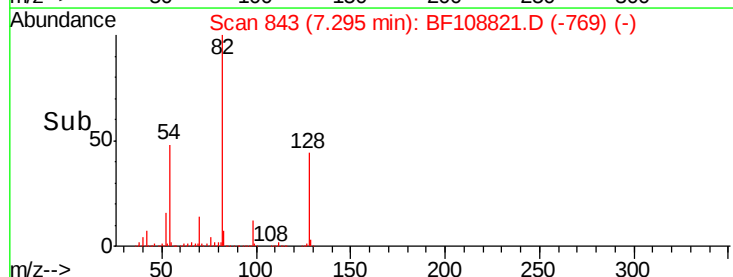



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.02 min Scan# 966

Delta R.T. -0.00 min

Lab File: BF108821.D

Acq: 6 Sep 2018 12:58

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 1031921



Ion Ratio Lower Upper

136 100

137 11.1 8.9 13.3

54 7.5 6.6 9.8

68 6.5 5.0 7.4

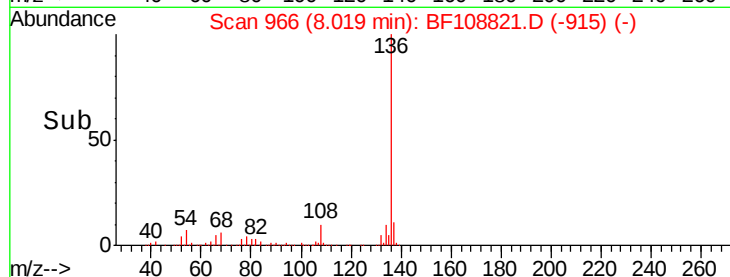
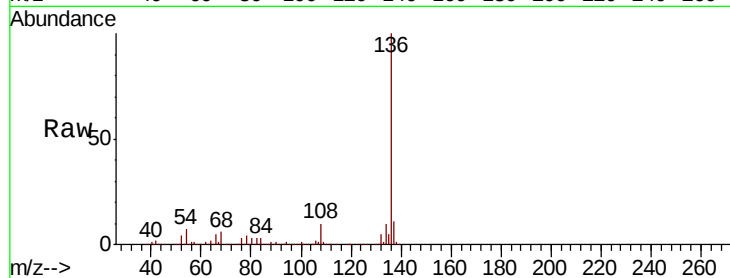


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

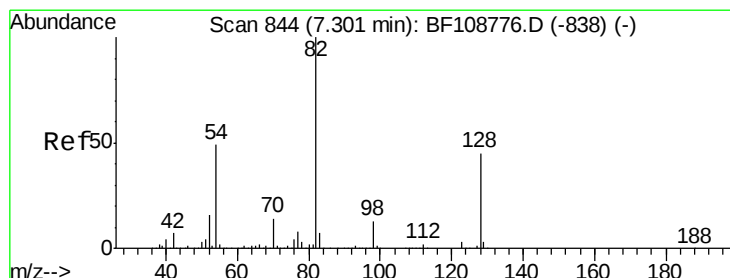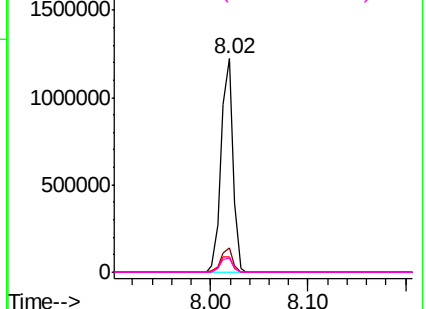

#23

Nitrobenzene-d5

Concen: 67.232 ng

RT: 7.30 min Scan# 843

Delta R.T. -0.01 min

Lab File: BF108821.D

Acq: 6 Sep 2018 12:58



Tgt Ion: 82 Resp: 1108610

Ion Ratio Lower Upper

82 100

128 44.5 36.1 54.1


54 48.4 41.4 62.2

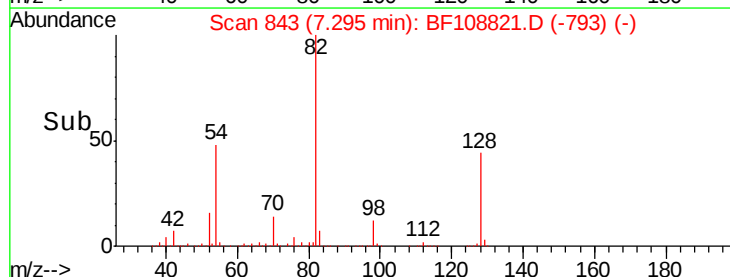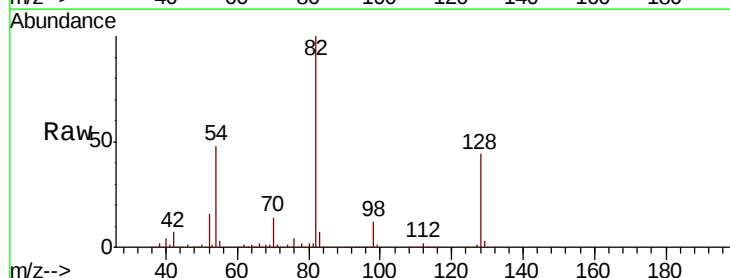


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

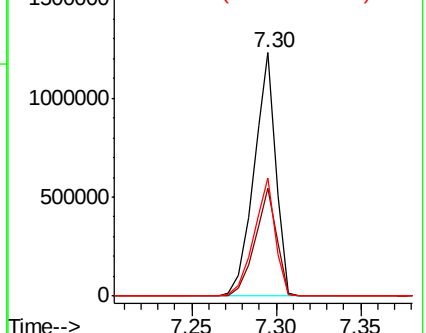

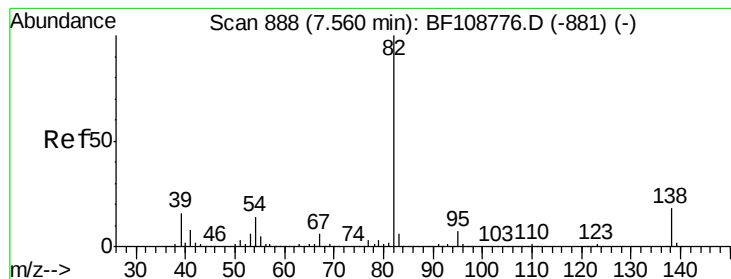

#25

Isophorone

Concen: 33.429 ng

RT: 7.30 min Scan# 843

Delta R.T. -0.26 min

Lab File: BF108821.D

Acq: 6 Sep 2018 12:58

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 1099507

Ion Ratio Lower Upper

82 100

95 0.2 5.2 7.8#




138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

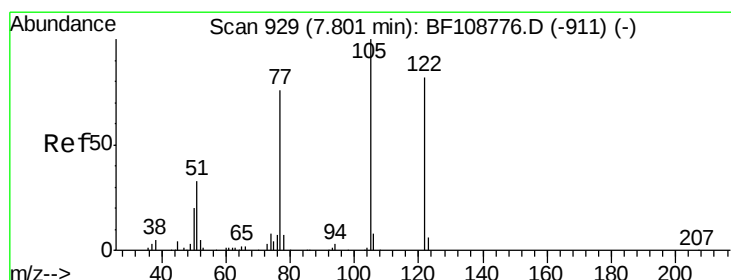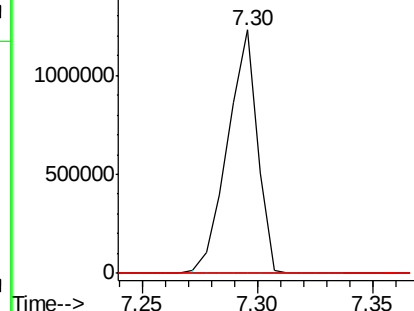

#32

Benzoic acid

Concen: 4.044 ng

RT: 7.68 min Scan# 909

Delta R.T. -0.12 min

Lab File: BF108821.D

Acq: 6 Sep 2018 12:58


Tgt Ion:122 Resp: 241

Ion Ratio Lower Upper

122 100

105 146.3 101.1 141.1#



77 150.6 70.7 110.7#




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF1

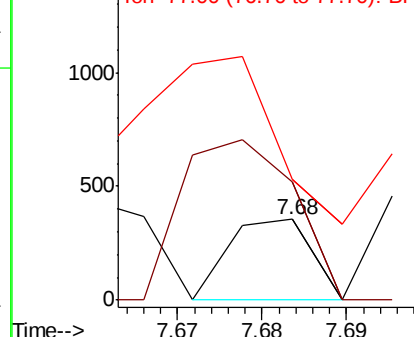


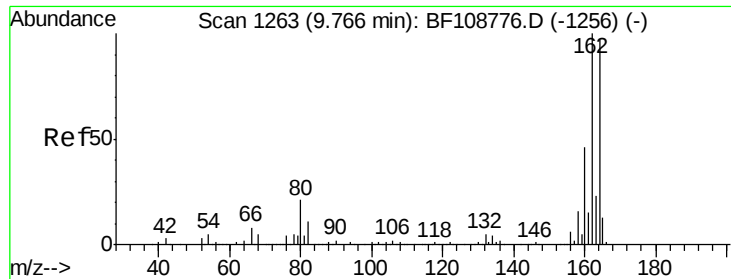




#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.77 min Scan# 1263
 Delta R.T. -0.00 min
 Lab File: BF108821.D
 Acq: 6 Sep 2018 12:58

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
164	100		
162	102.1	86.1	129.1
160	46.7	38.3	57.5

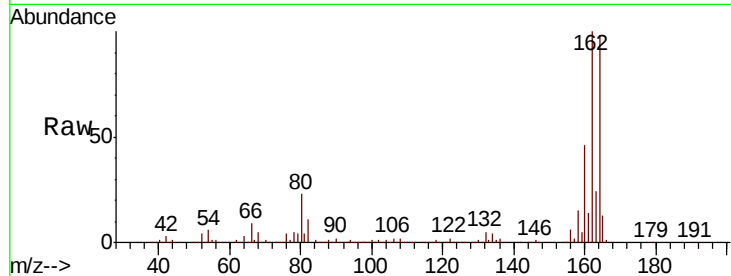


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E


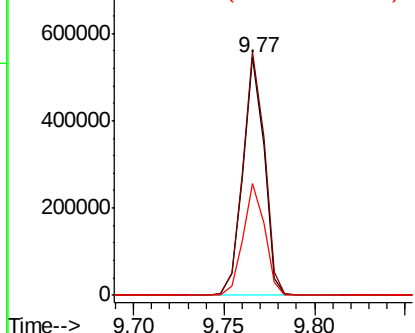



#41
 2,4,6-Tribromophenol
 Concen: 80.701 ng
 RT: 10.55 min Scan# 1396
 Delta R.T. -0.01 min
 Lab File: BF108821.D
 Acq: 6 Sep 2018 12:58

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.1	77.0	115.6
141	32.7	29.9	44.9



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E




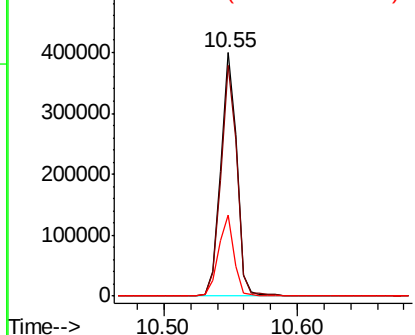


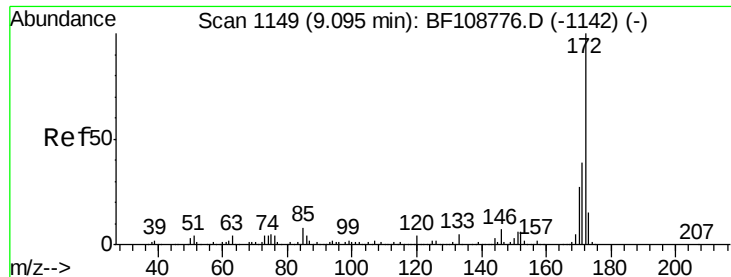

#44
2-Fluorobiphenyl
Concen: 70.652 ng
RT: 9.10 min Scan# 1149
Delta R.T. -0.00 min
Lab File: BF108821.D
Acq: 6 Sep 2018 12:58




Instrument :
BNA_F
ClientSampleId :


Tot Ion:172 Resp: 1837161
Ion Ratio Lower Upper
172 100
171 37.7 29.7 44.5
170 25.4 19.6 29.4

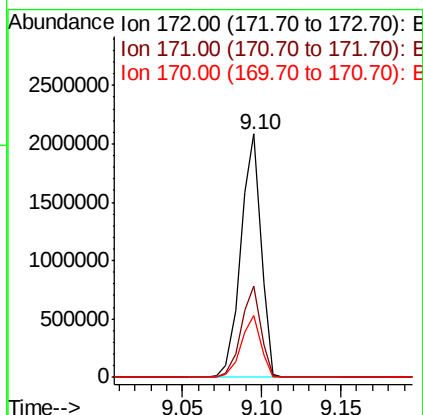

#49
Dimethylphthalate
Concen: 19.223 ng
RT: 9.48 min Scan# 1215
Delta R.T. -0.01 min
Lab File: BF108821.D
Acq: 6 Sep 2018 12:58

Tgt Ion:163 Resp: 596428
Ion Ratio Lower Upper
163 100
194 3.7 2.7 4.1
164 10.3 8.2 12.2



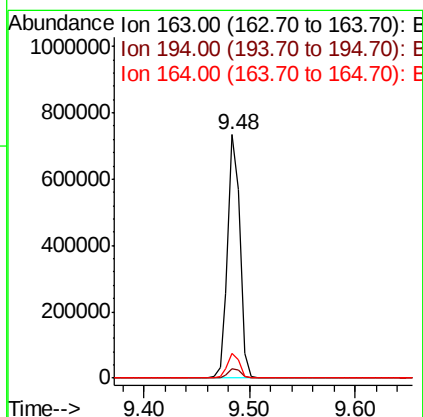





#56
 2,4-Dinitrotoluene
 Concen: 7.640 ng
 RT: 9.77 min Scan# 1263
 Delta R.T. -0.18 min
 Lab File: BF108821.D
 Acq: 6 Sep 2018 12:58




Instrument :
 BNA_F
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.3	36.4	54.6#
89	1.4	57.8	86.6#
182	0.0	1.6	2.4#

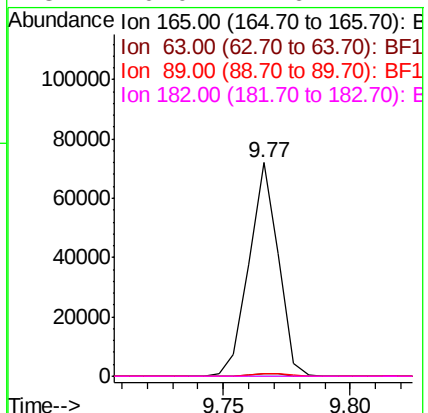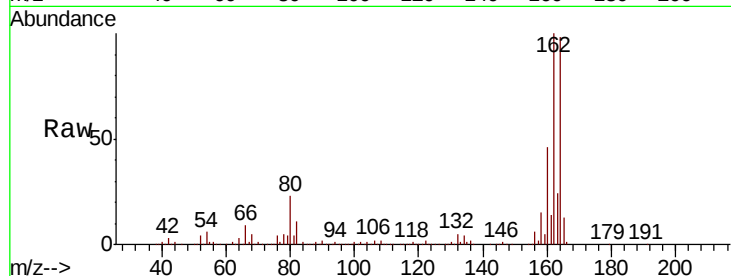

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.24 min Scan# 1514
 Delta R.T. -0.00 min
 Lab File: BF108821.D
 Acq: 6 Sep 2018 12:58

Tgt Ion	Ratio	Lower	Upper
188	100		
94	11.1	8.5	12.7
80	11.5	9.2	13.8

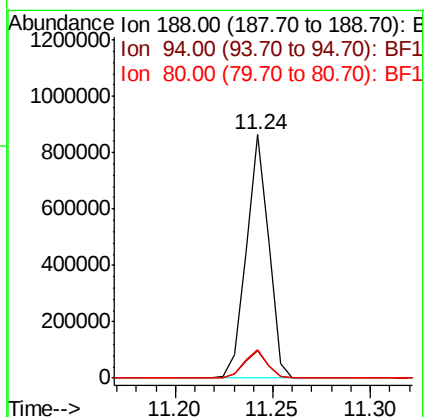

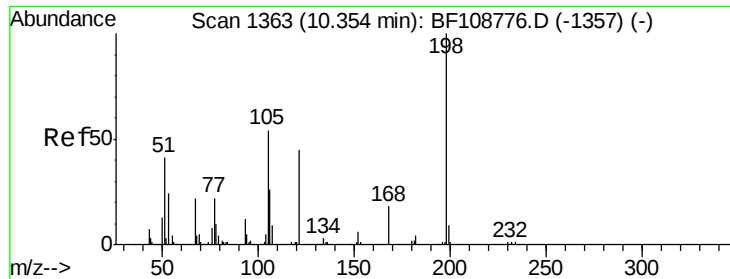

#64

4,6-Dinitro-2-methylphenol

Concen: 7.102 ng

RT: 10.55 min Scan# 1396

Delta R.T. 0.19 min

Lab File: BF108821.D

Acq: 6 Sep 2018 12:58

Instrument :

BNA_F

ClientSampleId :


Tot Ion:198 Resp: 734

Ion Ratio Lower Upper

198 100

51 185.5 37.7 77.7#




105 187.1 36.3 76.3#

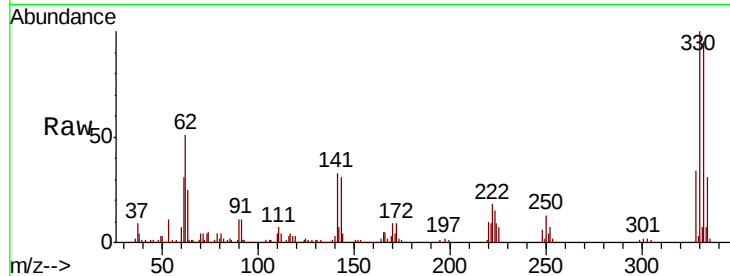

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

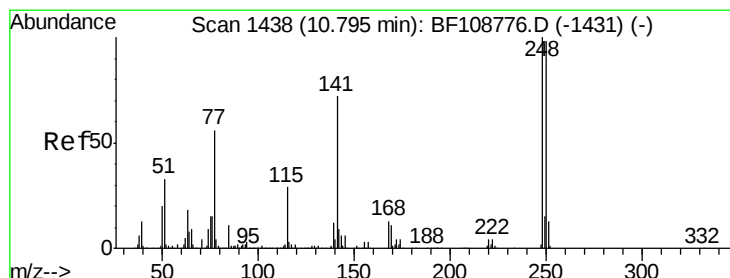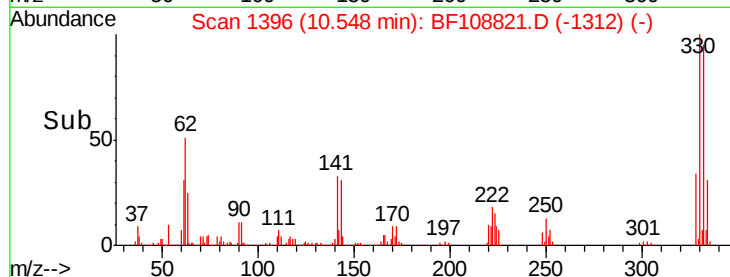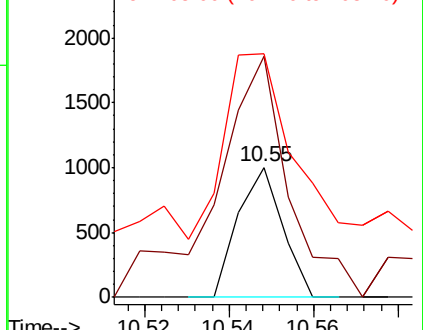

#66

4-Bromophenyl-phenylether

Concen: 2.657 ng

RT: 10.55 min Scan# 1396

Delta R.T. -0.25 min

Lab File: BF108821.D

Acq: 6 Sep 2018 12:58


Tgt Ion:248 Resp: 20520

Ion Ratio Lower Upper

248 100

250 200.7 76.9 115.3#



141 529.6 74.4 111.6#

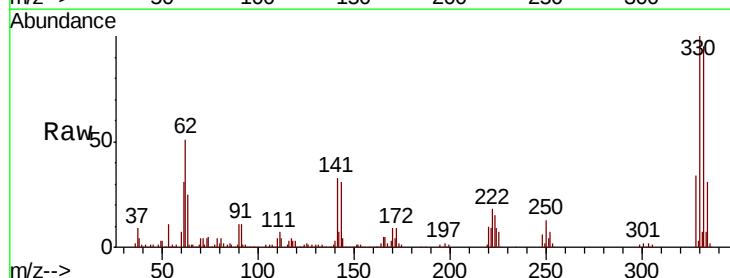


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E



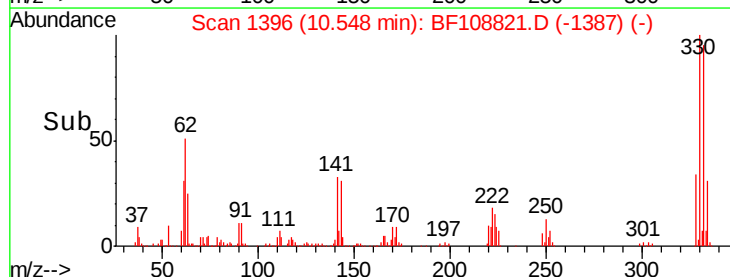
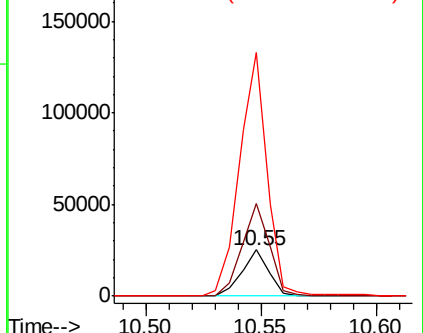




#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.87 min Scan# 1960
Delta R.T. -0.00 min
Lab File: BF108821.D
Acq: 6 Sep 2018 12:58




Instrument :
BNA_F
ClientSampleId :


Tot Ion:240 Resp: 575040
Ion Ratio Lower Upper
240 100
120 13.2 9.5 14.3
236 26.0 20.7 31.1

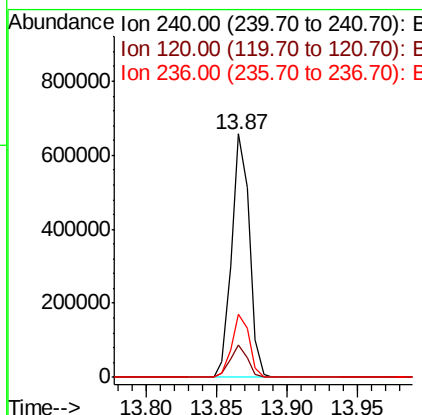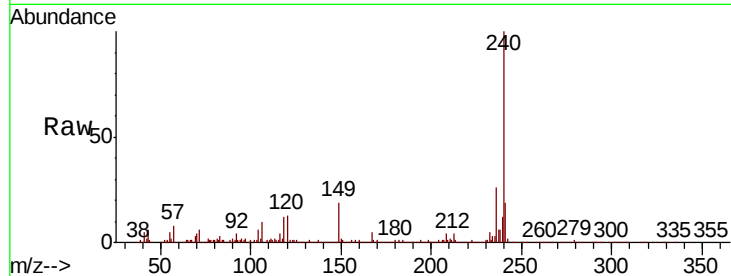

#78
Terphenyl-d14
Concen: 54.098 ng
RT: 12.82 min Scan# 1783
Delta R.T. 0.00 min
Lab File: BF108821.D
Acq: 6 Sep 2018 12:58

Tgt Ion:244 Resp: 1334033
Ion Ratio Lower Upper
244 100
212 7.5 5.4 8.0
122 13.7 11.0 16.4

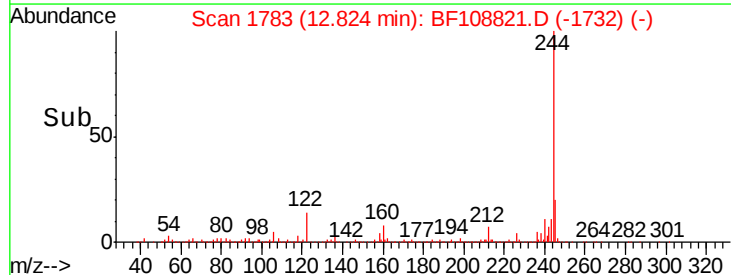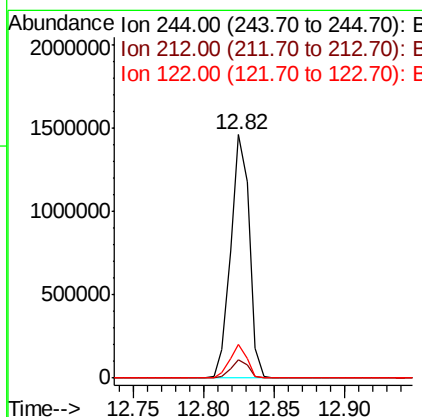




#83
 Bis(2-ethylhexyl)phthalate
 Concen: 5.712 ng
 RT: 13.87 min Scan# 1961
 Delta R.T. 0.01 min
 Lab File: BF108821.D
 Acq: 6 Sep 2018 12:58

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
149	100		
167	25.8	21.3	31.9
279	3.9	3.0	4.4



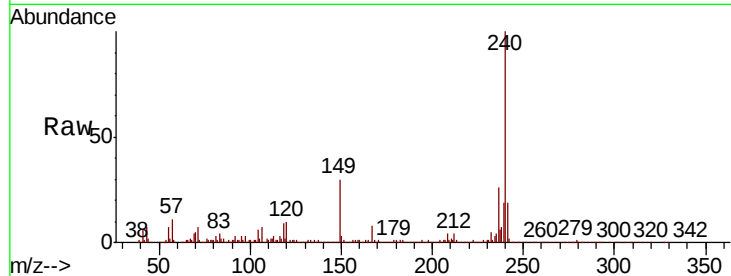


Abundance

Ion 149.00 (148.70 to 149.70): E


Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

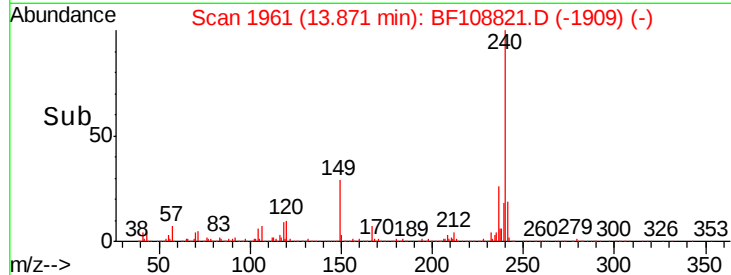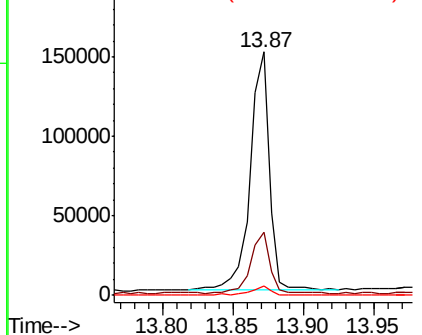

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.27 min Scan# 2199
 Delta R.T. 0.01 min
 Lab File: BF108821.D
 Acq: 6 Sep 2018 12:58

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.2	28.8
265	21.7	17.5	26.3

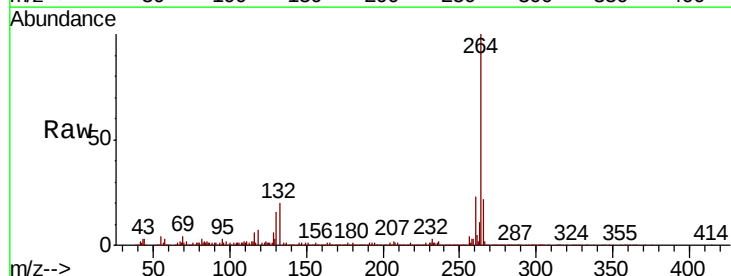

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

