
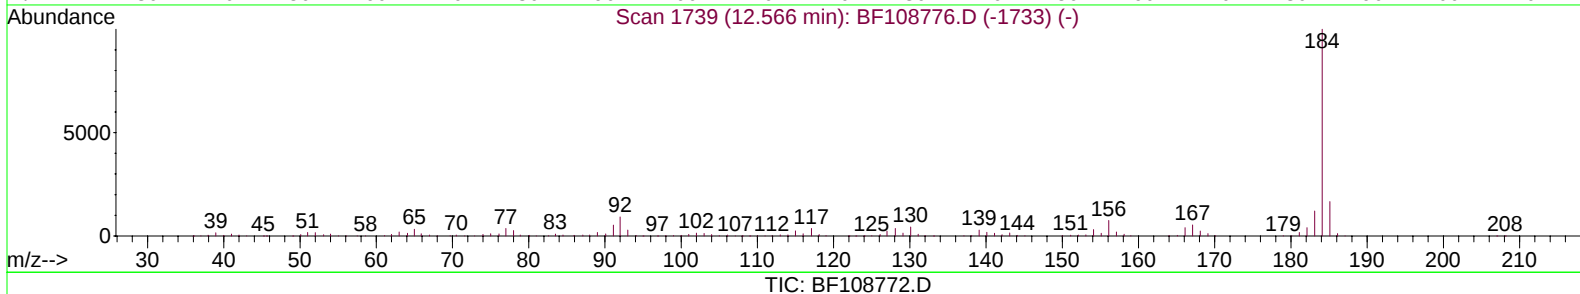
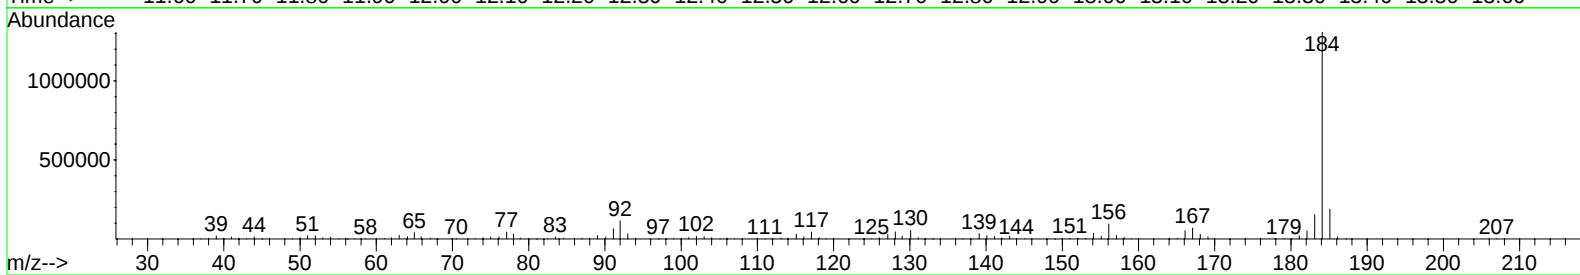


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090518\
Data File : BF108772.D
Acq On : 5 Sep 2018 14:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 19:22:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 18:03:31 2018
Response via : Initial Calibration

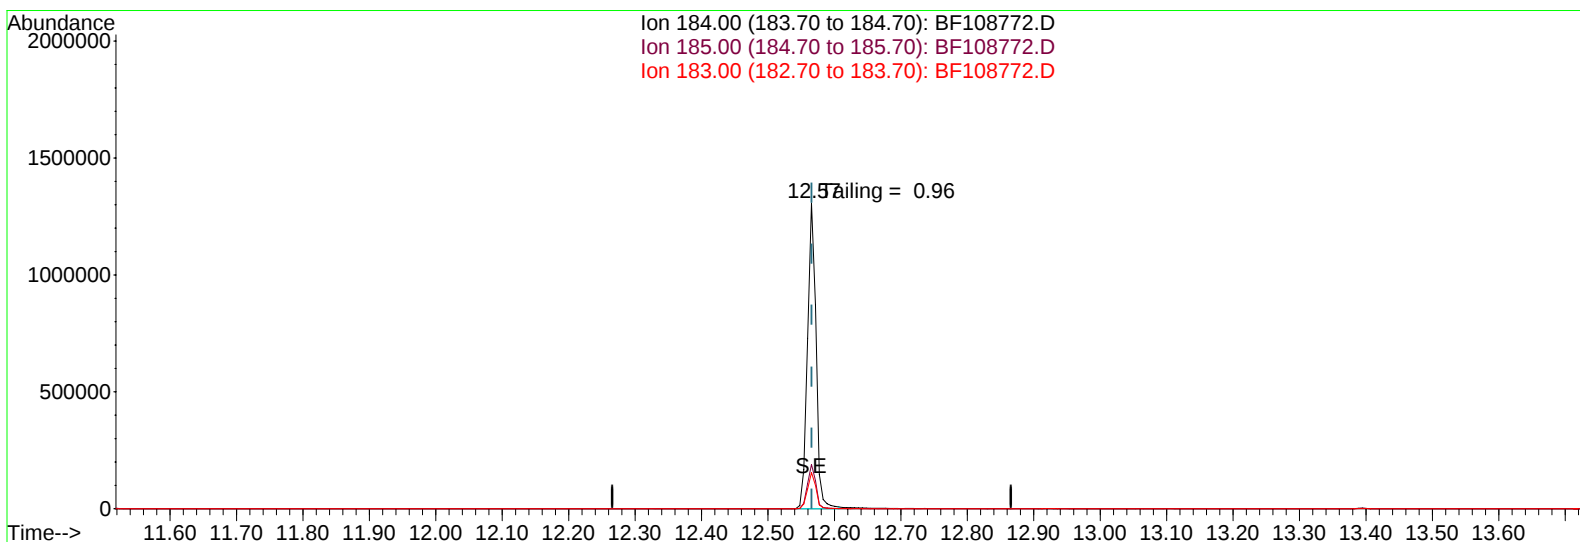

(76) Benzidine




12.566min (-0.000) 0.00ng

response 1191689

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.48
183.00	11.60	11.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090518\
Data File : BF108772.D
Acq On : 5 Sep 2018 14:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 05 19:22:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 18:03:31 2018
Response via : Initial Calibration

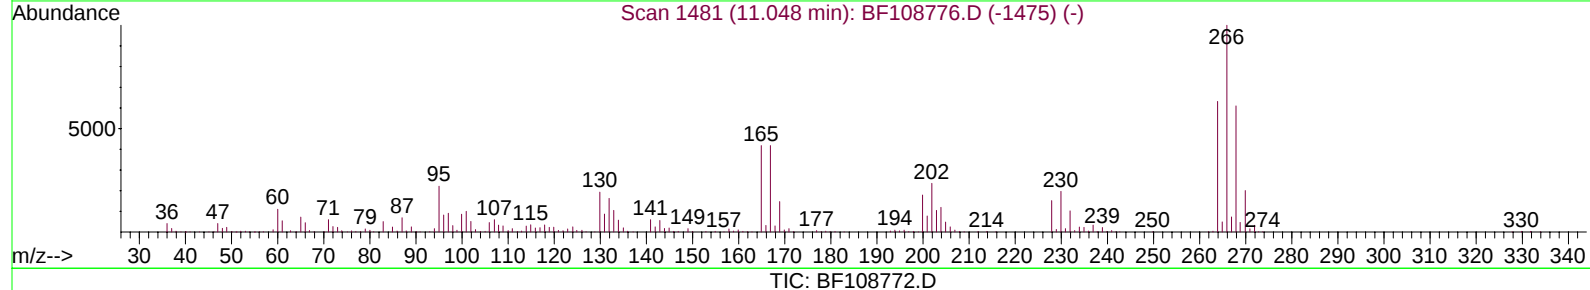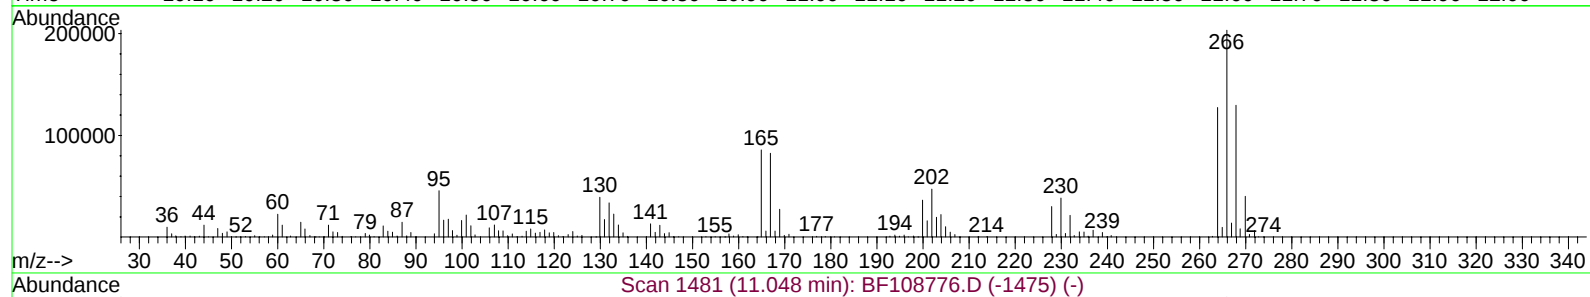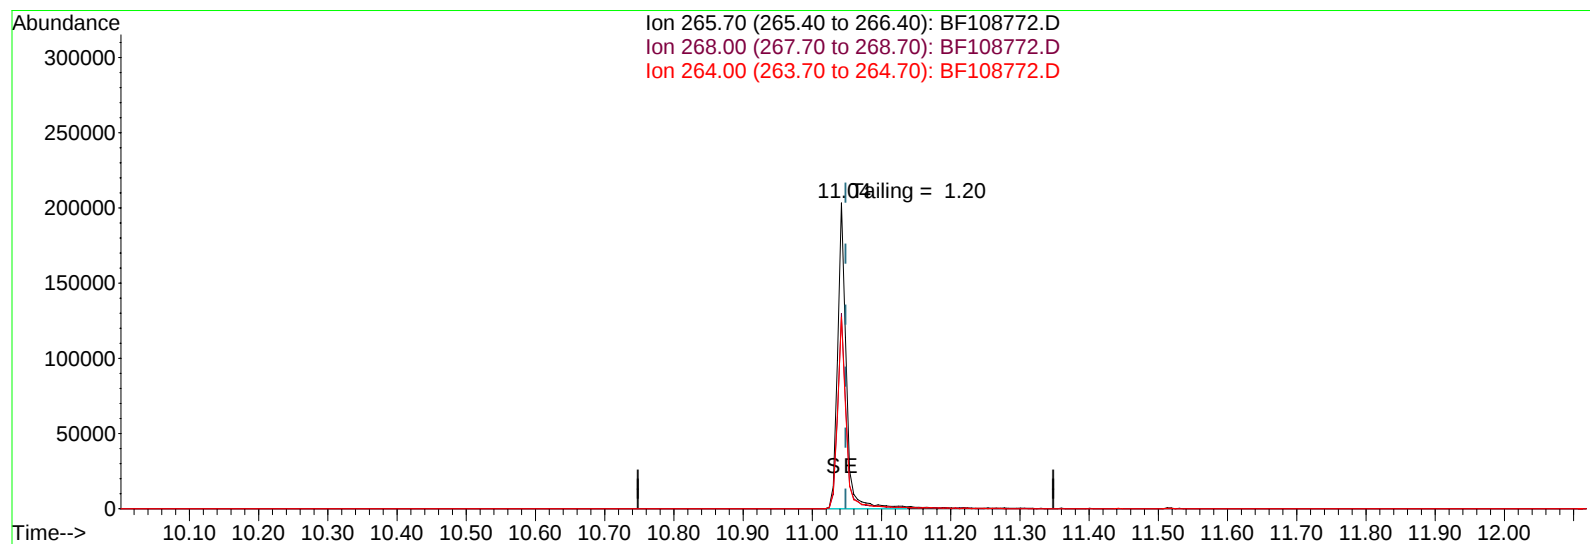

(69) Pentachlorophenol (C)

11.042min (-0.006) 29129.28ng

response 175213

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.79
264.00	61.90	62.65
0.00	0.00	0.00