

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090518\
 Data File : BF108817.D
 Acq On : 6 Sep 2018 11:11
 Operator : JU/SJ
 Sample : J4791-03DL 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DOCUMENTATION-#12DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.337	506	510	513	rVB	457957	430492	5.28%	1.943%
2	6.354	680	683	690	rBV	564753	471683	5.79%	2.129%
3	6.495	704	707	711	rBV	538409	476411	5.84%	2.150%
4	6.736	744	748	751	rBV	2155764	1718979	21.09%	7.758%
5	6.889	770	774	778	rBV	485127	378738	4.65%	1.709%
6	7.289	838	842	845	rBV	322007	264159	3.24%	1.192%
7	8.019	961	966	969	rBV	2654590	2207144	27.07%	9.961%
8	9.089	1144	1148	1151	rBV	734950	548025	6.72%	2.473%
9	9.483	1212	1215	1218	rBV	199928	148522	1.82%	0.670%
10	9.766	1259	1263	1267	rBV2	2607916	2169219	26.61%	9.790%
11	10.542	1392	1395	1399	rBV	231563	199861	2.45%	0.902%
12	11.242	1510	1514	1517	rBV	2206921	1857095	22.78%	8.381%
13	11.266	1517	1518	1521	rVB	216720	109950	1.35%	0.496%
14	12.448	1716	1719	1723	rVB	357918	283748	3.48%	1.281%
15	12.671	1752	1757	1761	rBV	318798	335681	4.12%	1.515%
16	12.818	1779	1782	1788	rVB	451179	421355	5.17%	1.902%
17	13.301	1861	1864	1867	rBV	252658	201139	2.47%	0.908%
18	13.871	1953	1961	1970	rBV2	7628555	8152280	100.00%	36.792%
19	14.036	1984	1989	1991	rBV	117654	154182	1.89%	0.696%
20	14.877	2129	2132	2134	rBV	110705	137649	1.69%	0.621%
21	14.977	2146	2149	2153	rBV3	107984	134052	1.64%	0.605%
22	15.271	2195	2199	2207	rVB	1123728	1357673	16.65%	6.127%


Sum of corrected areas: 22158037

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090518\
Data File : BF108817.D
Acq On : 6 Sep 2018 11:11
Operator : JU/SJ
Sample : J4791-03DL 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DOCUMENTATION-#12DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

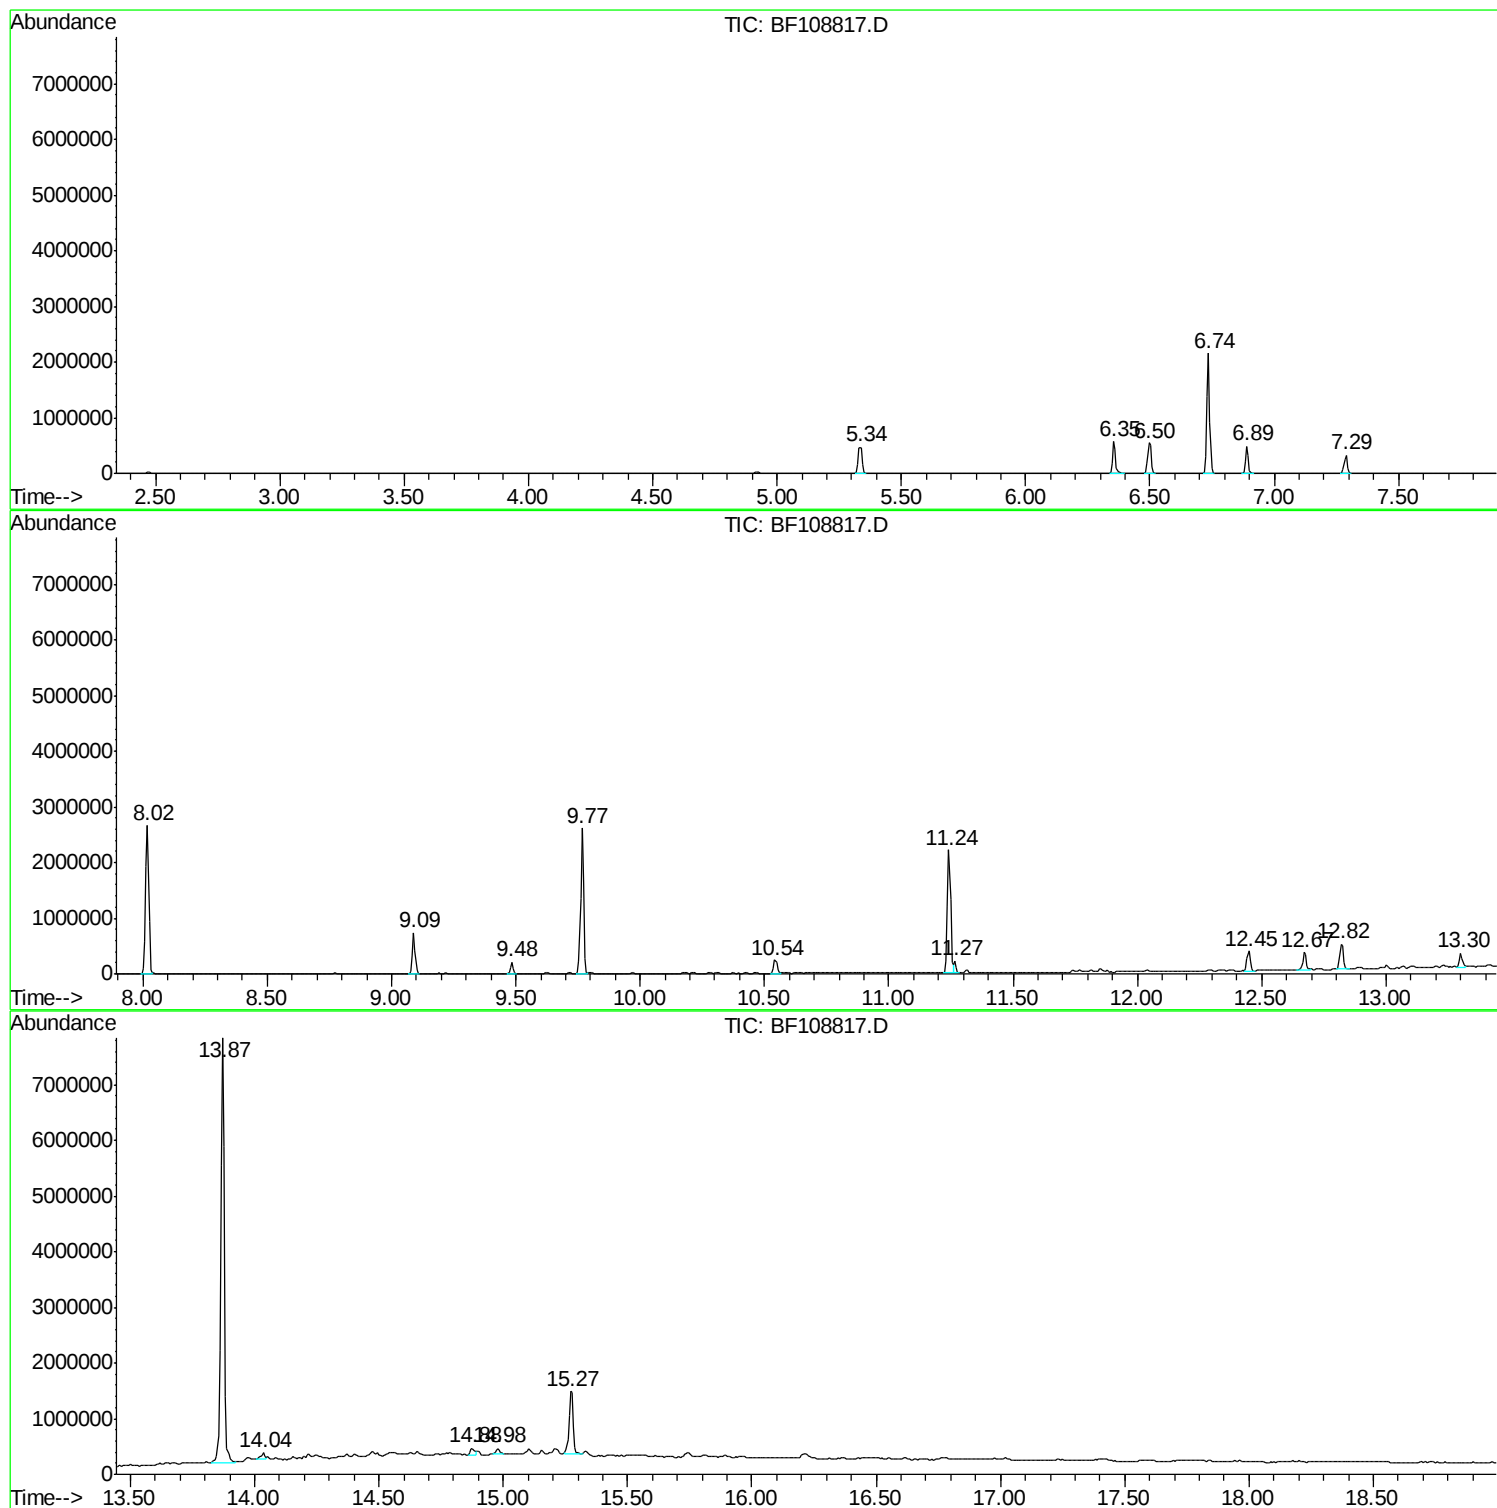

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090518\
Data_File : BF108817.D
Acq_On : 6-Sep-2018 11:111
Operator : JU/SJJ
Sample : J4791-03DL_10XX
Misc :
ALS_Vial : 35 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
DOCUMENTATION-#12DL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
