


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090518\
 Data File : BF108781.D
 Acq On : 5 Sep 2018 18:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 05 18:03:31 2018

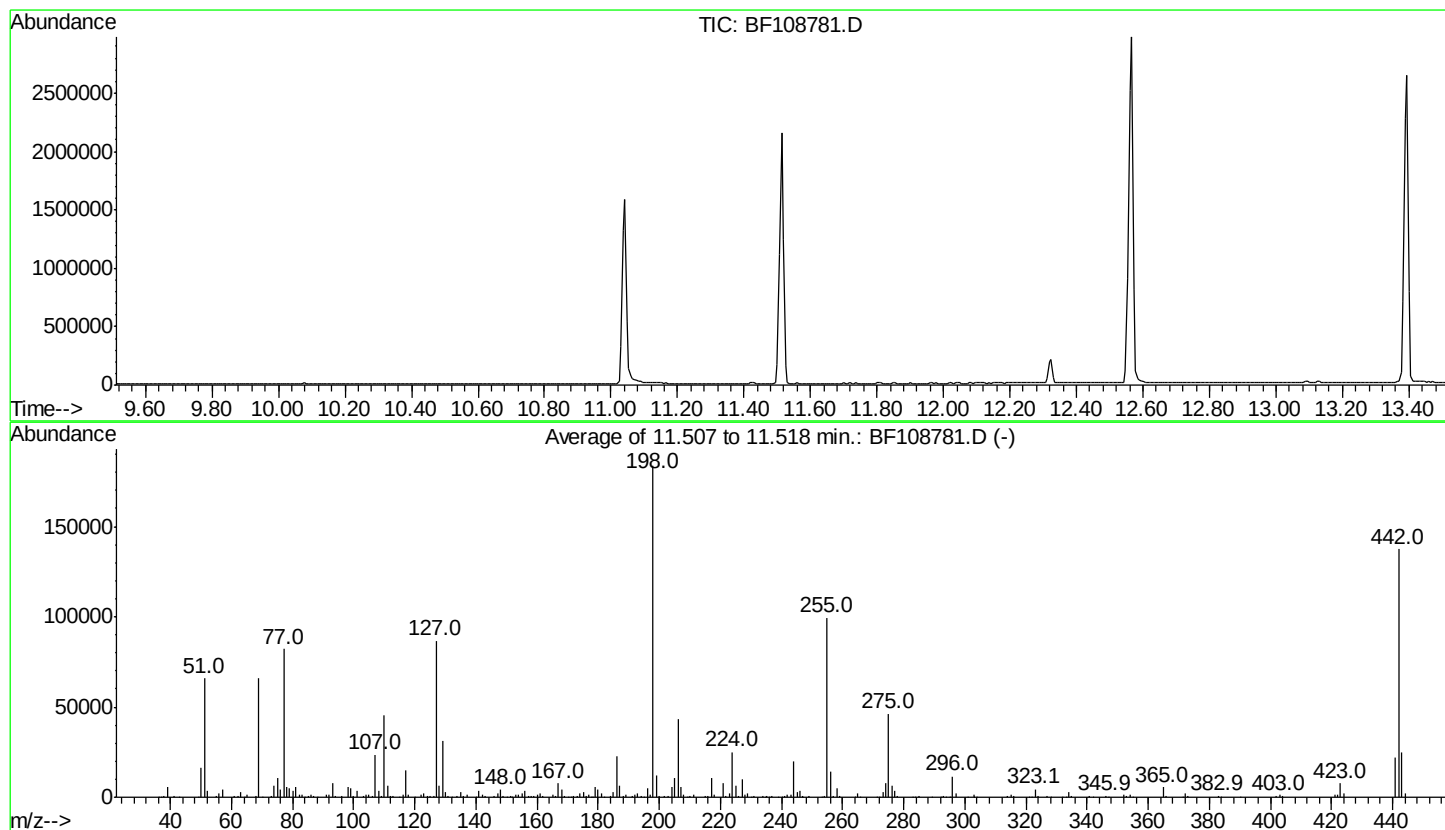

AutoFind: Scans 1559, 1560, 1561; Background Corrected with Scan 1554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	65717	PASS
68	69	0.00	2	1.6	1078	PASS
69	198	0.00	100	35.9	65922	PASS
70	69	0.00	2	0.5	312	PASS
127	198	10	80	47.2	86808	PASS
197	198	0.00	2	0.7	1227	PASS
198	198	100	100	100.0	183765	PASS
199	198	5	9	6.6	12051	PASS
275	198	10	60	25.2	46400	PASS
365	198	1	100	2.9	5393	PASS
441	198	0.01	100	11.9	21912	PASS
442	198	50	100	74.8	137410	PASS
443	442	15	24	18.0	24793	PASS