


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090518\
 Data File : BF108808.D
 Acq On : 6 Sep 2018 7:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 05 18:03:31 2018

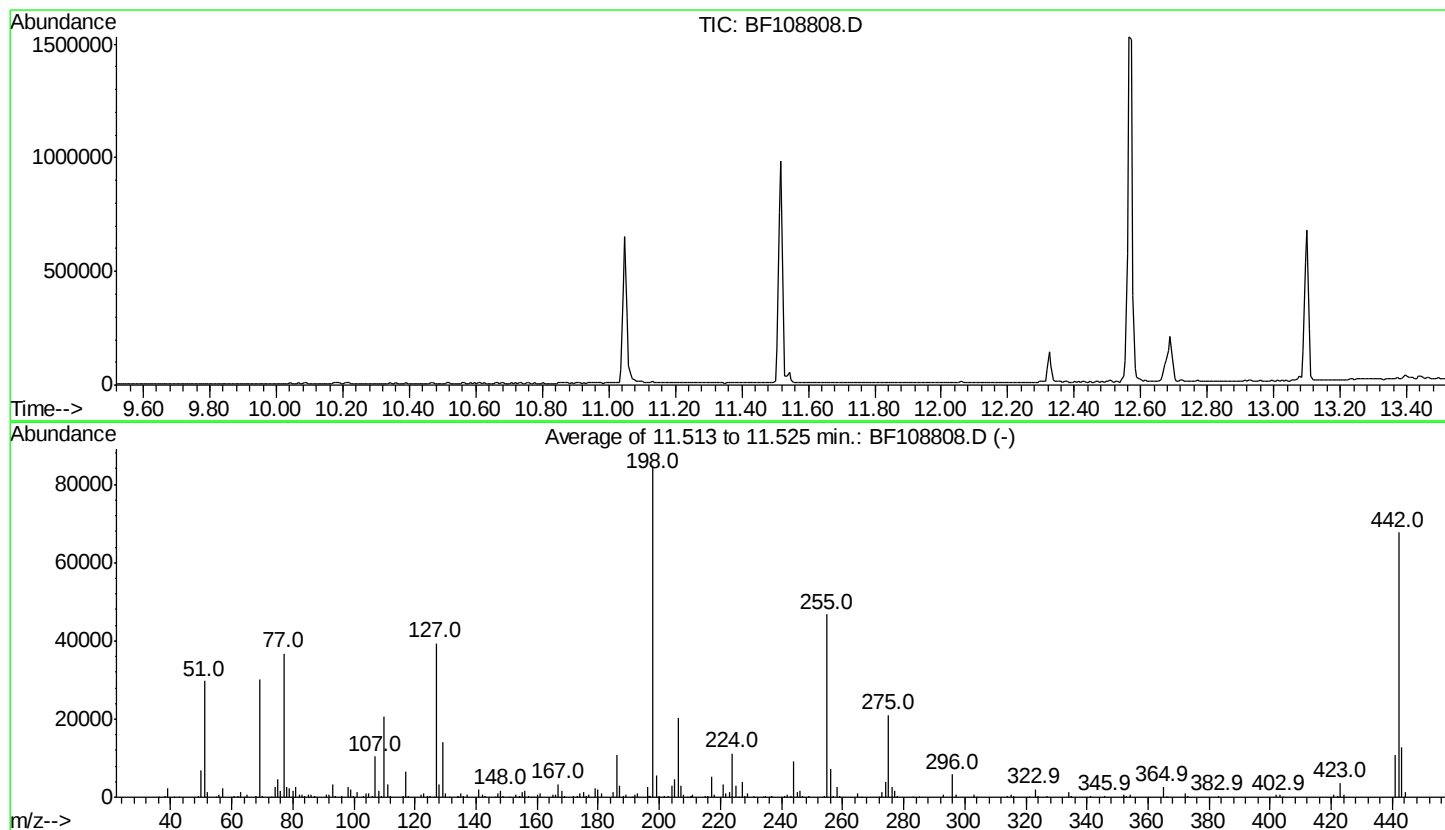

AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	29670	PASS
68	69	0.00	2	1.6	470	PASS
69	198	0.00	100	35.5	30139	PASS
70	69	0.00	2	0.8	244	PASS
127	198	10	80	46.4	39396	PASS
197	198	0.00	2	0.3	267	PASS
198	198	100	100	100.0	84816	PASS
199	198	5	9	6.5	5552	PASS
275	198	10	60	24.8	21056	PASS
365	198	1	100	3.1	2651	PASS
441	198	0.01	100	12.9	10979	PASS
442	198	50	100	79.8	67690	PASS
443	442	15	24	18.9	12769	PASS