
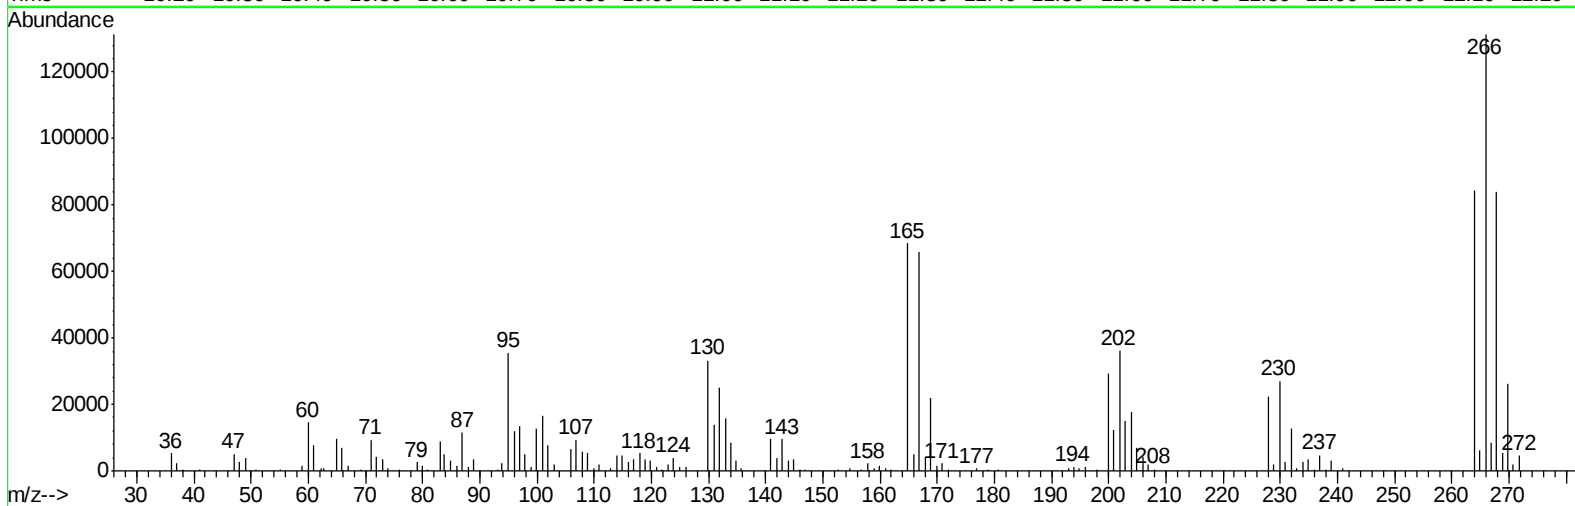


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090519\
Data File : BF116827.D
Acq On : 5 Sep 2019 10:23
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:07:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

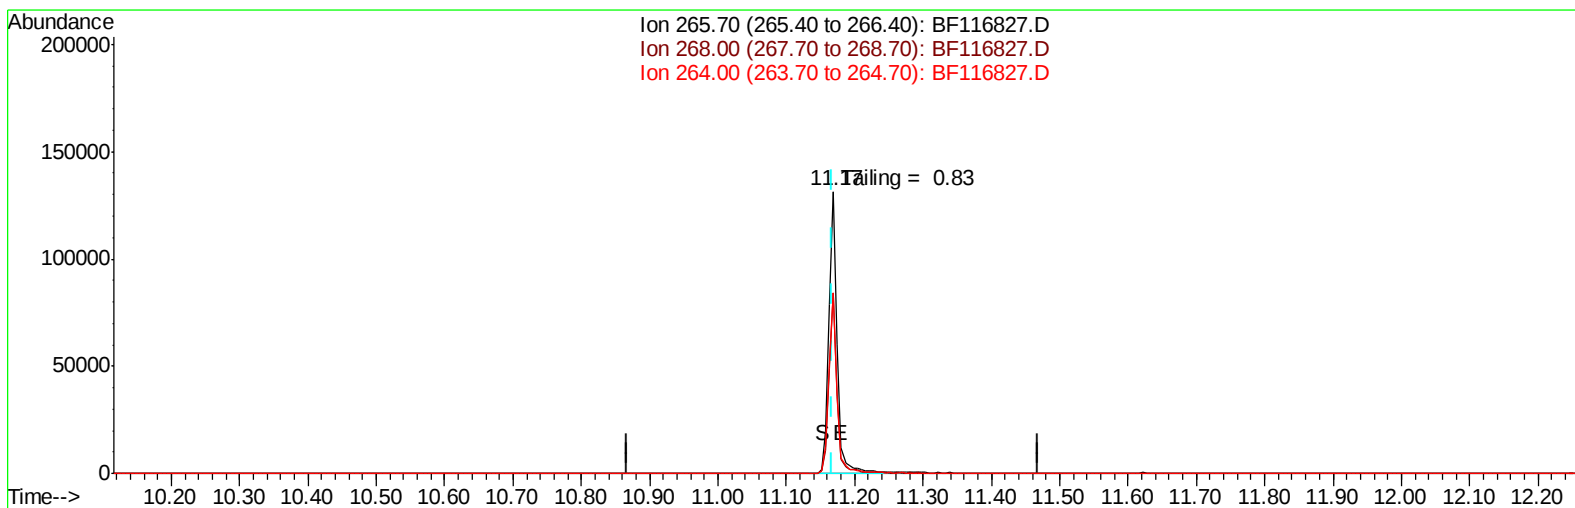

TIC: BF116827.D

(70) Pentachlorophenol (C)



11.169min (+0.000) 101962.73ng

response 114810

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.96
264.00	64.90	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090519\
Data File : BF116827.D
Acq On : 5 Sep 2019 10:23
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 09:07:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

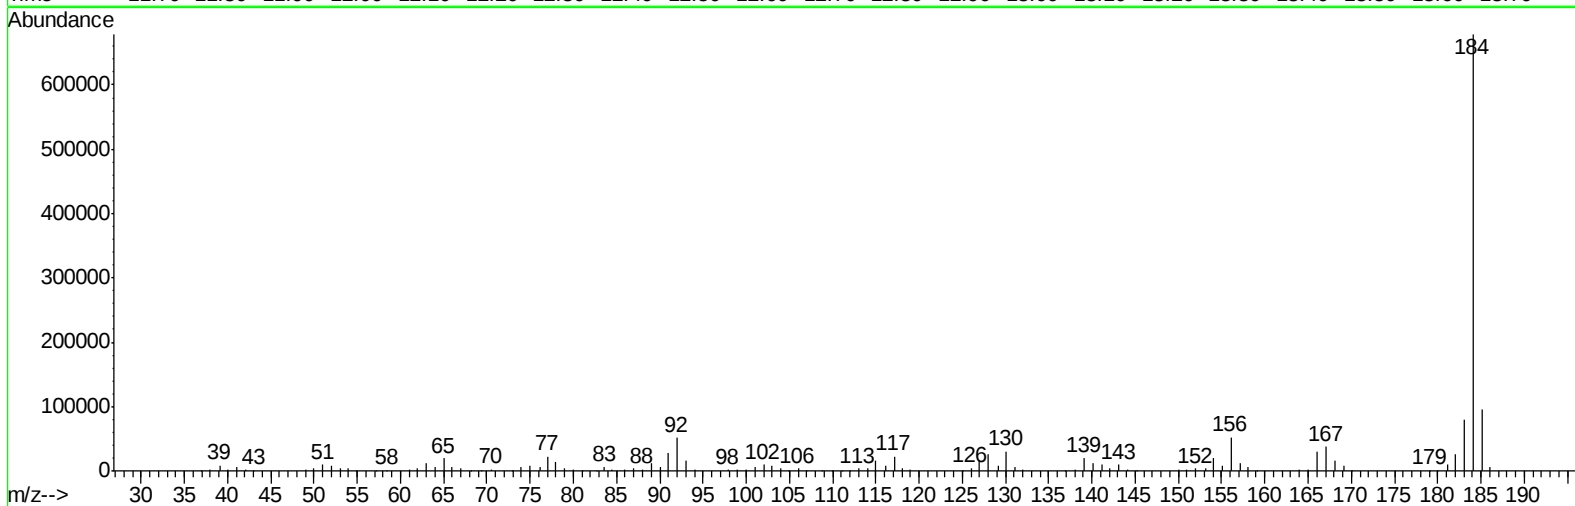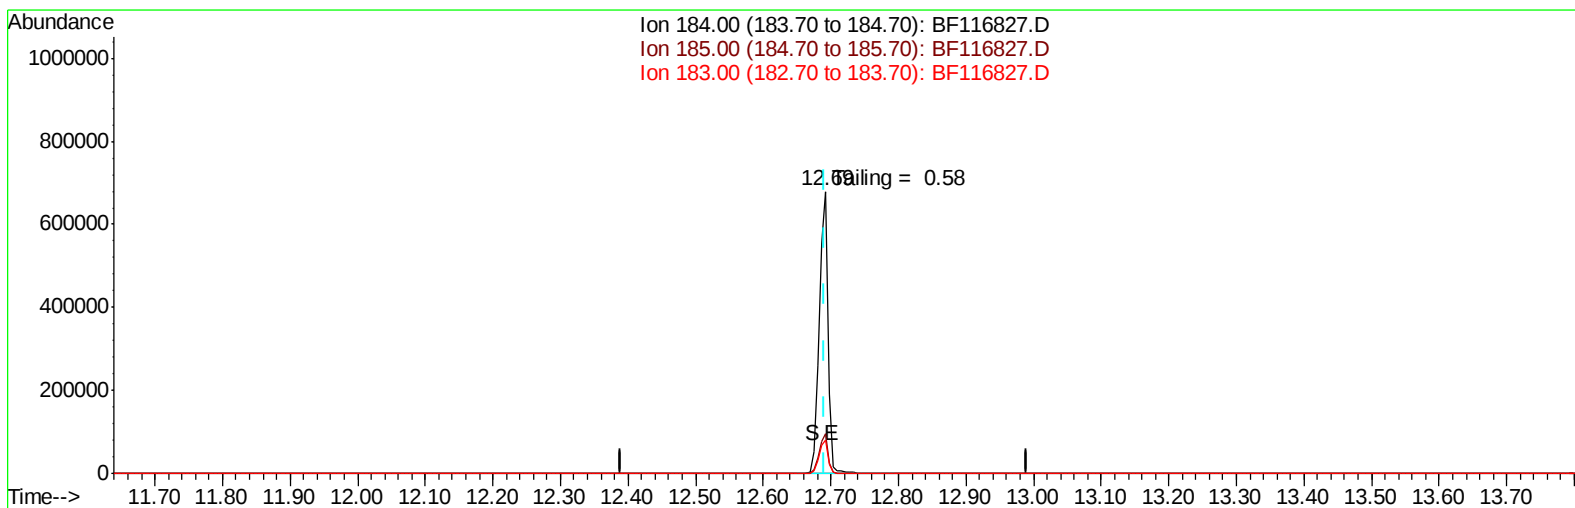

TIC: BF116827.D

(77) Benzidine

12.692min (+0.001) 35684.21ng

response 629830

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.95
183.00	11.50	11.81
0.00	0.00	0.00