


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090519\
 Data File : BF116827.D
 Acq On : 5 Sep 2019 10:23
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 20:02:30 2019

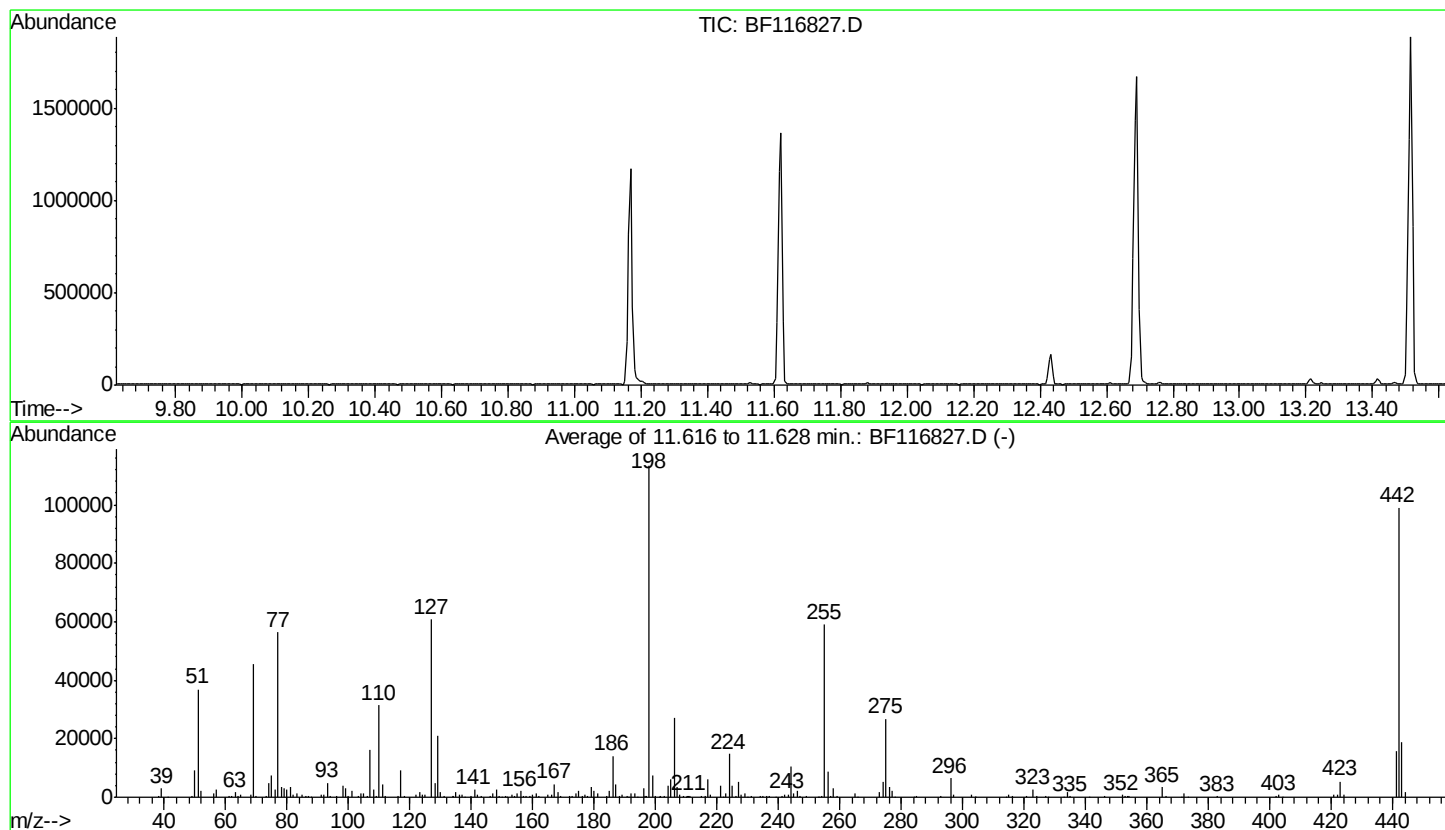

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	36885	PASS
68	69	0.00	2	1.8	813	PASS
69	198	0.00	100	40.2	45589	PASS
70	69	0.00	2	0.6	291	PASS
127	198	10	80	53.5	60662	PASS
197	198	0.00	2	0.4	472	PASS
198	198	100	100	100.0	113405	PASS
199	198	5	9	6.7	7566	PASS
275	198	10	60	23.7	26933	PASS
365	198	1	100	2.9	3313	PASS
441	198	0.01	100	14.0	15826	PASS
442	198	50	100	87.4	99144	PASS
443	442	15	24	18.8	18674	PASS