

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090523\
 Data File : BF135114.D
 Acq On : 06 Sep 2023 02:16
 Operator : CG\JU
 Sample : 04203-01RE
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-1(12-12.5)

Quant Time: Sep 06 03:47:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 31 03:48:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.775	152	106688	20.000	ng	0.00
21) Naphthalene-d8	8.051	136	409559	20.000	ng	0.00
39) Acenaphthene-d10	9.810	164	186732	20.000	ng	0.00
64) Phenanthrene-d10	11.298	188	282574	20.000	ng	-0.01
76) Chrysene-d12	13.957	240	207656	20.000	ng	0.00
86) Perylene-d12	15.427	264	179838	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.404	112	562118	81.383	ng	0.00
7) Phenol-d6	6.416	99	693455	80.548	ng	0.00
23) Nitrobenzene-d5	7.334	82	427825	58.686	ng	-0.01
42) 2,4,6-Tribromophenol	10.598	330	132978	67.132	ng	-0.01
45) 2-Fluorobiphenyl	9.128	172	705489	61.511	ng	-0.01
79) Terphenyl-d14	12.898	244	524631	41.229	ng	0.00
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	7.334	70	57446	11.233	ng	# 76
25) Isophorone	7.334	82	427817	30.952	ng	# 65
50) Dimethylphthalate	9.810	163	36969	2.827	ng	# 1
51) 2,6-Dinitrotoluene	9.810	165	23281	8.115	ng	# 21
57) 2,4-Dinitrotoluene	9.810	165	23281	6.511	ng	# 20
67) 4-Bromophenyl-phenylether	10.598	248	8642	2.883	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090523\
Data File : BF135114.D
Acq On : 06 Sep 2023 02:16
Operator : CG\JU
Sample : 04203-01RE
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-1(12-12.5)

Quant Time: Sep 06 03:47:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration




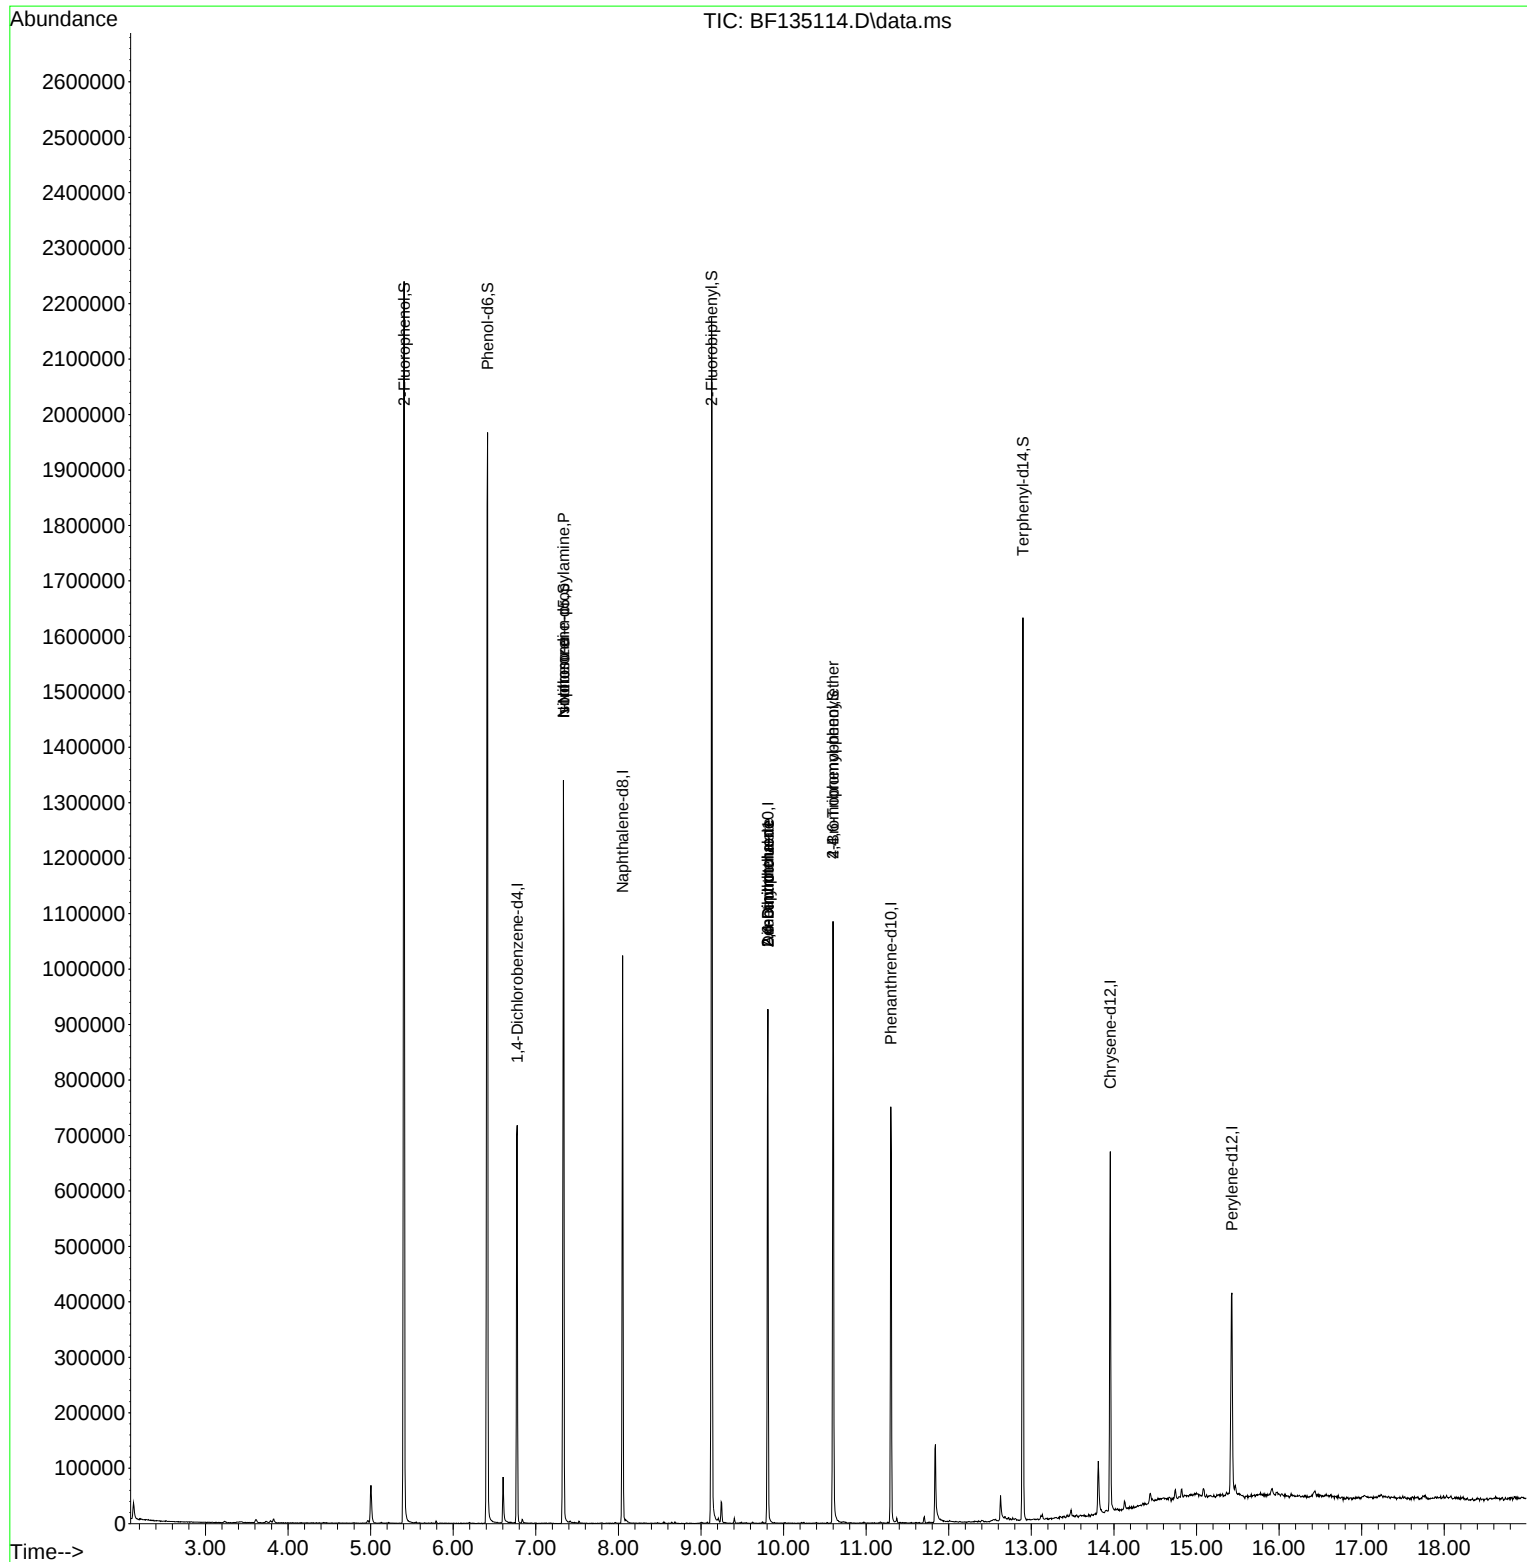




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.775 min Scan# 79
Delta R.T. -0.000 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16




Instrument :
BNA_F
ClientSampleId :
SB-1(12-12.5)


Tgt Ion:152 Resp: 106688
Ion Ratio Lower Upper
152 100
150 150.4 126.2 189.4
115 59.1 51.2 76.8

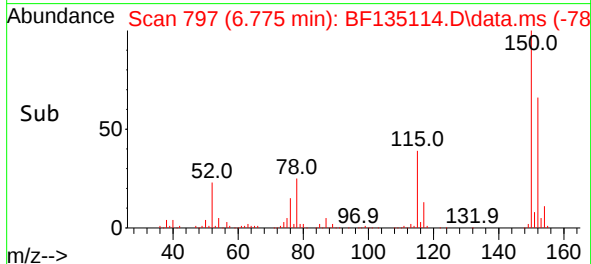

#5
2-Fluorophenol
Concen: 81.383 ng
RT: 5.404 min Scan# 564
Delta R.T. 0.006 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16

Tgt Ion:112 Resp: 562118
Ion Ratio Lower Upper
112 100
64 63.8 50.5 75.7
63 32.7 25.9 38.9


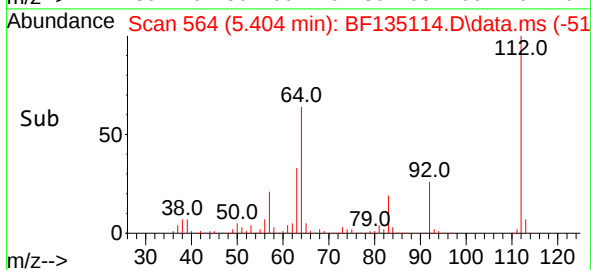

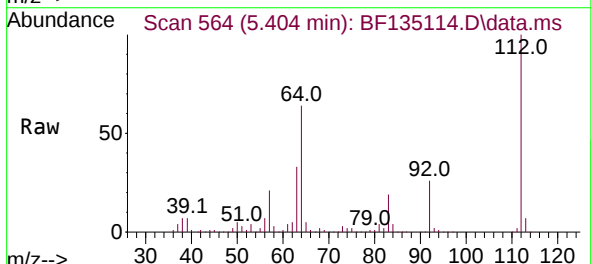




#7
Phenol-d6
Concen: 80.548 ng
RT: 6.416 min Scan# 736
Delta R.T. 0.000 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16




Instrument :
BNA_F
ClientSampleId :
SB-1(12-12.5)


Tgt Ion: 99 Resp: 693455
Ion Ratio Lower Upper
99 100
42 19.6 16.6 25.0
71 34.7 27.0 40.6

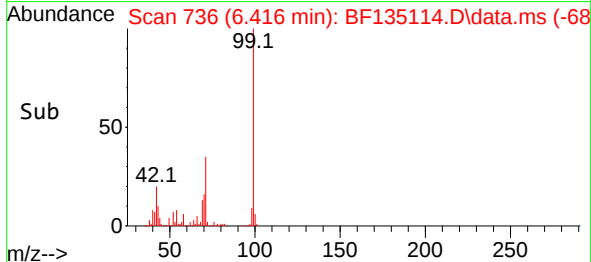

#19
n-Nitroso-di-n-propylamine
Concen: 11.233 ng
RT: 7.334 min Scan# 892
Delta R.T. 0.135 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16

Tgt Ion: 70 Resp: 57446
Ion Ratio Lower Upper
70 100
42 50.9 50.2 75.4
101 0.0 8.1 12.1#
130 1.8 19.3 28.9#


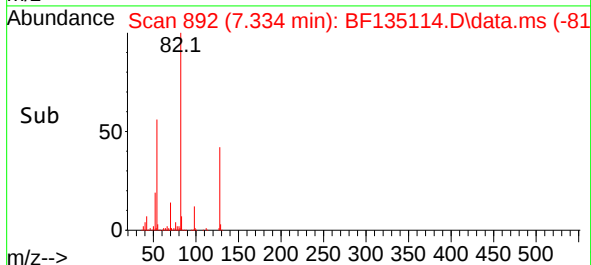
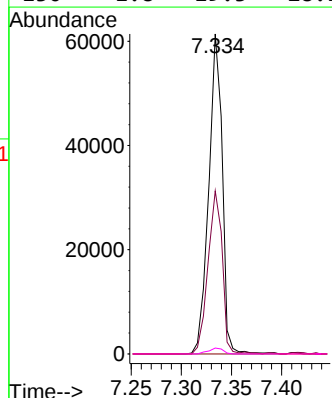
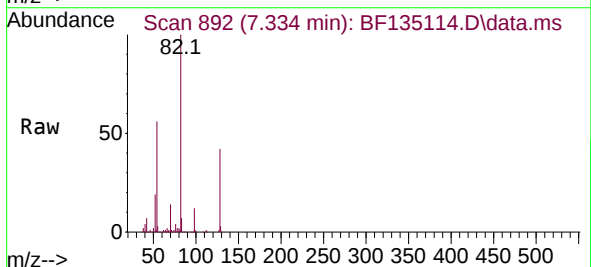




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.051 min Scan# 1015
Delta R.T. -0.006 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16




Instrument :
BNA_F
ClientSampleId :
SB-1(12-12.5)


Tgt Ion:136 Resp: 409559
Ion Ratio Lower Upper
136 100
137 11.3 8.8 13.2
54 8.3 7.0 10.4
68 5.5 4.6 6.8

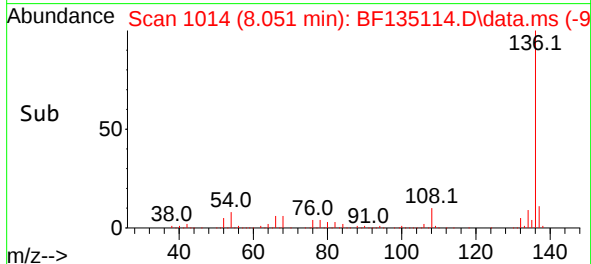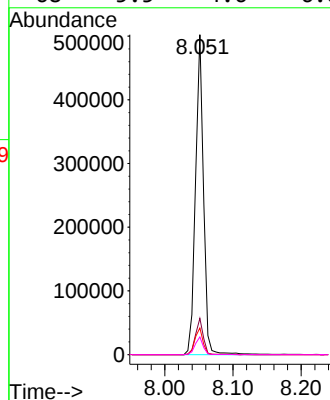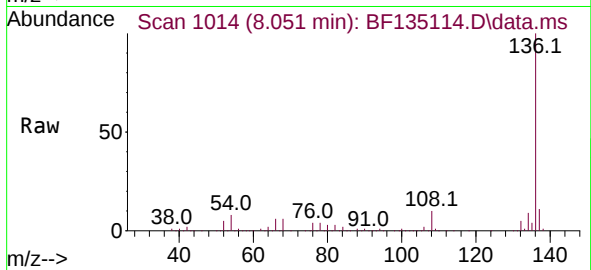

#23
Nitrobenzene-d5
Concen: 58.686 ng
RT: 7.334 min Scan# 892
Delta R.T. -0.012 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16

Tgt Ion: 82 Resp: 427825
Ion Ratio Lower Upper
82 100
128 42.2 37.8 56.8
54 56.3 45.0 67.6


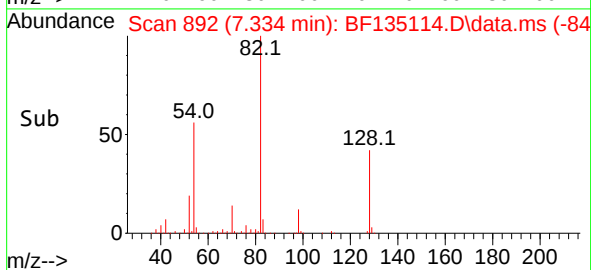
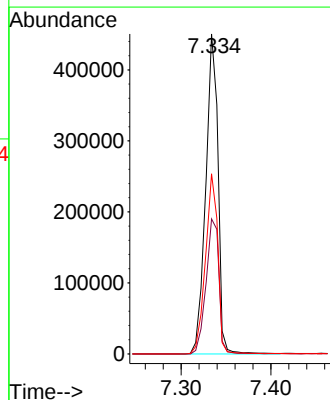
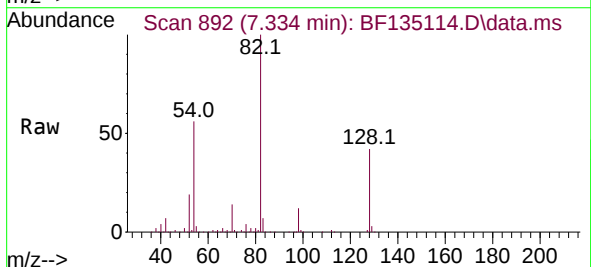




#25
Isophorone
Concen: 30.952 ng
RT: 7.334 min Scan# 89
Delta R.T. -0.264 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16




Instrument :
BNA_F
ClientSampleId :
SB-1(12-12.5)


Tgt Ion: 82 Resp: 427817
Ion Ratio Lower Upper
82 100
95 0.0 5.6 8.4#
138 0.0 14.7 22.1#

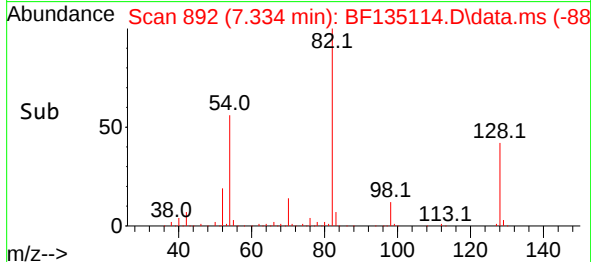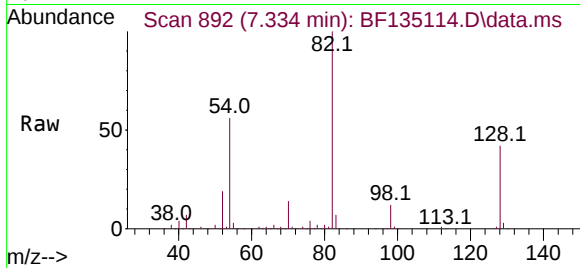

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.810 min Scan# 1313
Delta R.T. -0.006 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16

Tgt Ion:164 Resp: 186732
Ion Ratio Lower Upper
164 100
162 103.9 79.5 119.3
160 46.5 36.0 54.0

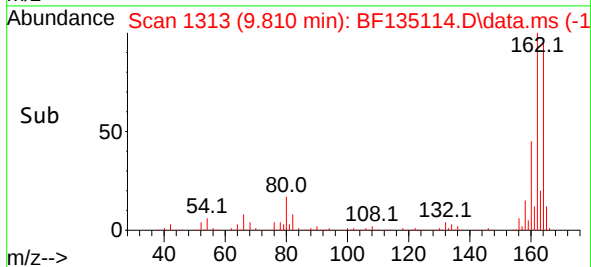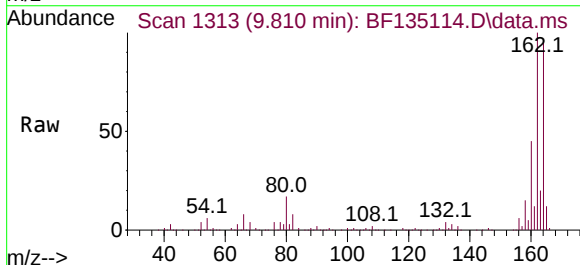



#42

2,4,6-Tribromophenol

Concen: 67.132 ng

RT: 10.598 min Scan# 1447

Delta R.T. -0.012 min

Lab File: BF135114.D

Acq: 06 Sep 2023 02:16

Instrument :

BNA_F

ClientSampleId :

SB-1(12-12.5)





Tgt Ion:330 Resp: 132978

Ion Ratio Lower Upper

330 100

332 96.2 77.6 116.4

141 32.3 26.3 39.5



#45

2-Fluorobiphenyl

Concen: 61.511 ng

RT: 9.128 min Scan# 1197

Delta R.T. -0.012 min

Lab File: BF135114.D

Acq: 06 Sep 2023 02:16




Tgt Ion:172 Resp: 705489


Ion Ratio Lower Upper

172 100

171 35.7 28.2 42.2

170 23.2 19.0 28.4


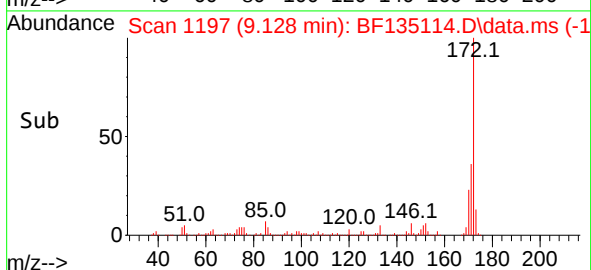






#50
Dimethylphthalate
Concen: 2.827 ng
RT: 9.810 min Scan# 1313
Delta R.T. 0.265 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16




Instrument :
BNA_F
ClientSampleId :
SB-1(12-12.5)


Tgt Ion:163 Resp: 36969
Ion Ratio Lower Upper
163 100
194 0.0 3.0 4.6#
164 470.2 8.1 12.1#

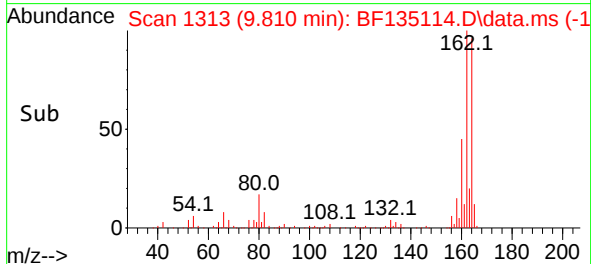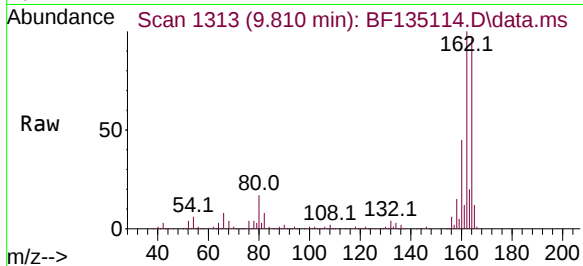

#51
2,6-Dinitrotoluene
Concen: 8.115 ng
RT: 9.810 min Scan# 1313
Delta R.T. 0.206 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16

Tgt Ion:165 Resp: 23281
Ion Ratio Lower Upper
165 100
63 1.3 50.4 75.6#
89 0.9 47.1 70.7#


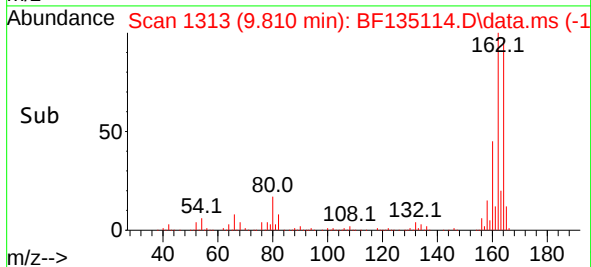

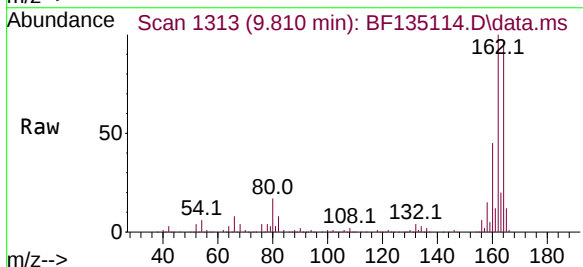




#57
2,4-Dinitrotoluene
Concen: 6.511 ng
RT: 9.810 min Scan# 1347
Delta R.T. -0.200 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16




Instrument :
BNA_F
ClientSampleId :
SB-1(12-12.5)


Tgt Ion:165 Resp: 23281
Ion Ratio Lower Upper
165 100
63 1.3 43.2 64.8#
89 0.9 60.8 91.2#
182 0.0 2.0 3.0#

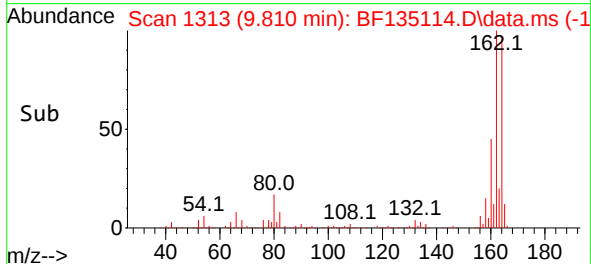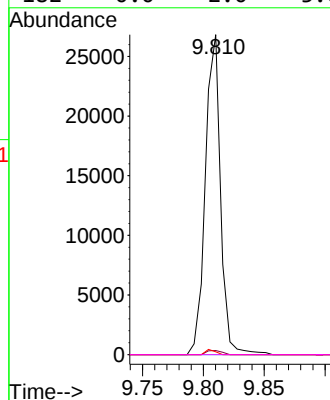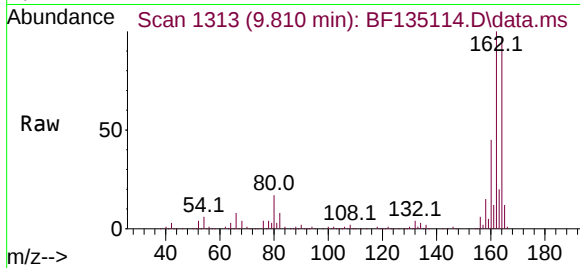

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.298 min Scan# 1566
Delta R.T. -0.012 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16

Tgt Ion:188 Resp: 282574
Ion Ratio Lower Upper
188 100
94 9.8 7.0 10.4
80 10.7 7.4 11.2


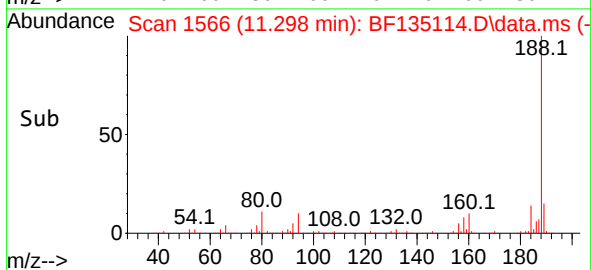
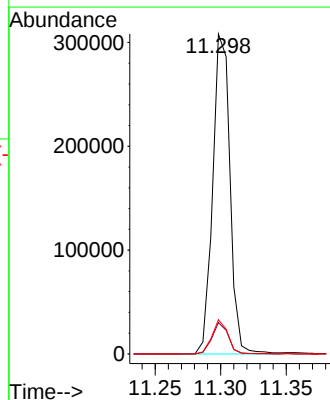
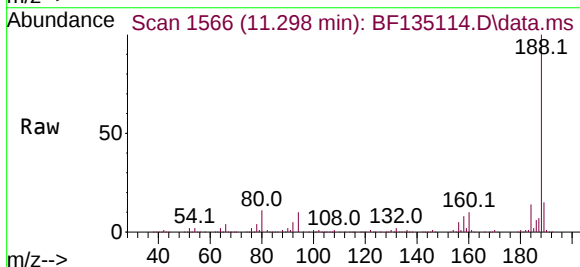




#67
4-Bromophenyl-phenylether
Concen: 2.883 ng
RT: 10.598 min Scan# 1490
Delta R.T. -0.253 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16




Instrument :
BNA_F
ClientSampleId :
SB-1(12-12.5)


Tgt Ion:248 Resp: 8642
Ion Ratio Lower Upper
248 100
250 185.4 77.9 116.9#
141 504.1 59.8 89.8#

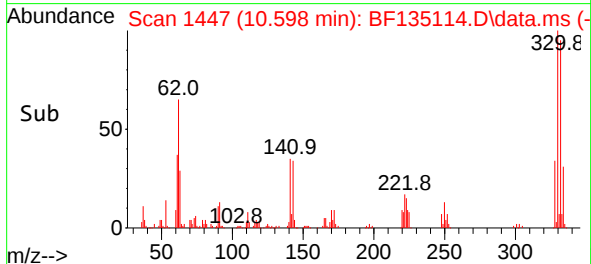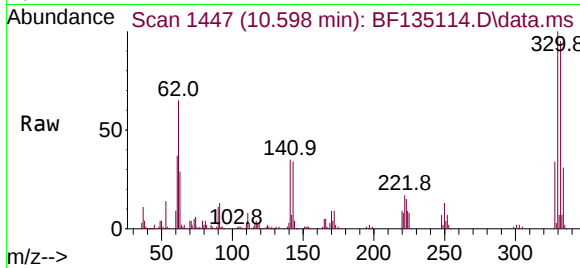

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.957 min Scan# 2018
Delta R.T. -0.006 min
Lab File: BF135114.D
Acq: 06 Sep 2023 02:16


Tgt Ion:240 Resp: 207656
Ion Ratio Lower Upper
240 100
120 10.8 10.2 15.2
236 25.0 21.3 31.9

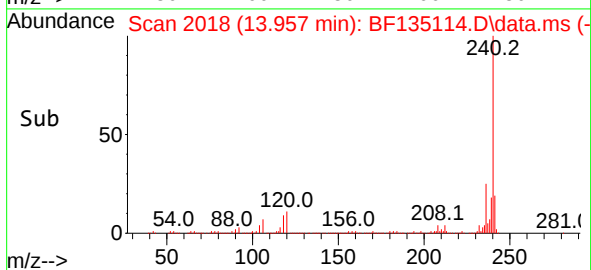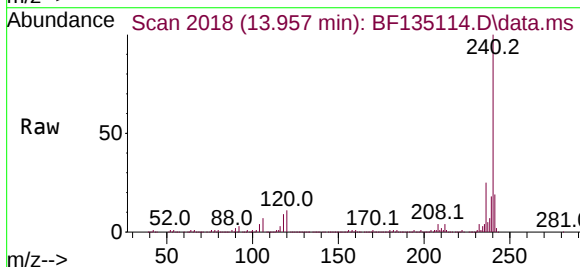






#79
 Terphenyl-d14
 Concen: 41.229 ng
 RT: 12.898 min Scan# 1839
 Delta R.T. -0.006 min
 Lab File: BF135114.D
 Acq: 06 Sep 2023 02:16

Instrument :
 BNA_F
 ClientSampleId :
 SB-1(12-12.5)

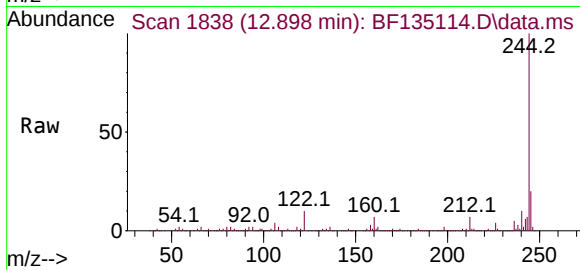

Tgt Ion:244 Resp: 524631
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.6 8.4
 122 10.3 9.8 14.6

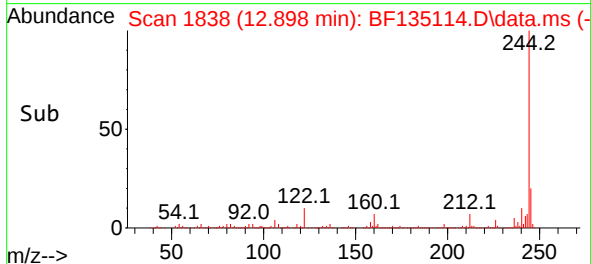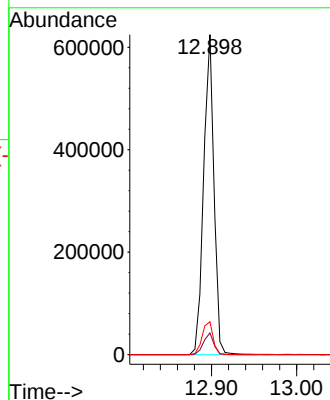

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.427 min Scan# 2268
 Delta R.T. 0.000 min
 Lab File: BF135114.D
 Acq: 06 Sep 2023 02:16

Tgt Ion:264 Resp: 179838
 Ion Ratio Lower Upper
 264 100
 260 25.3 19.0 28.6
 265 20.8 18.2 27.2

