
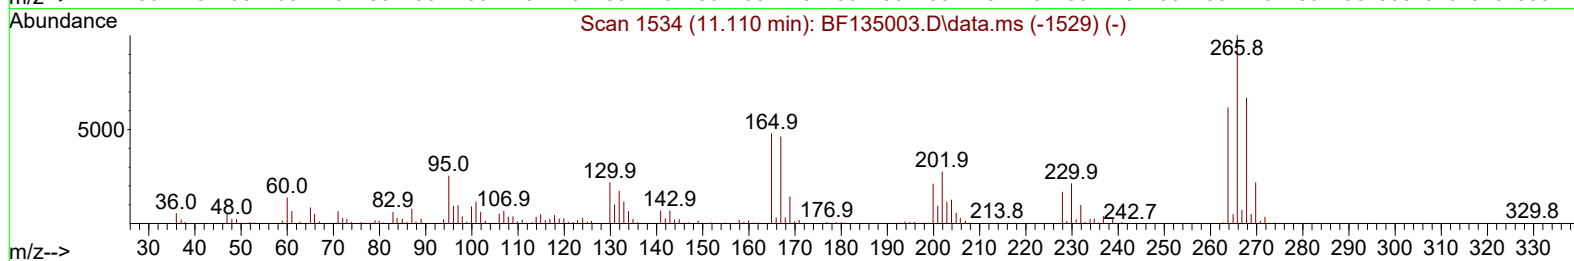
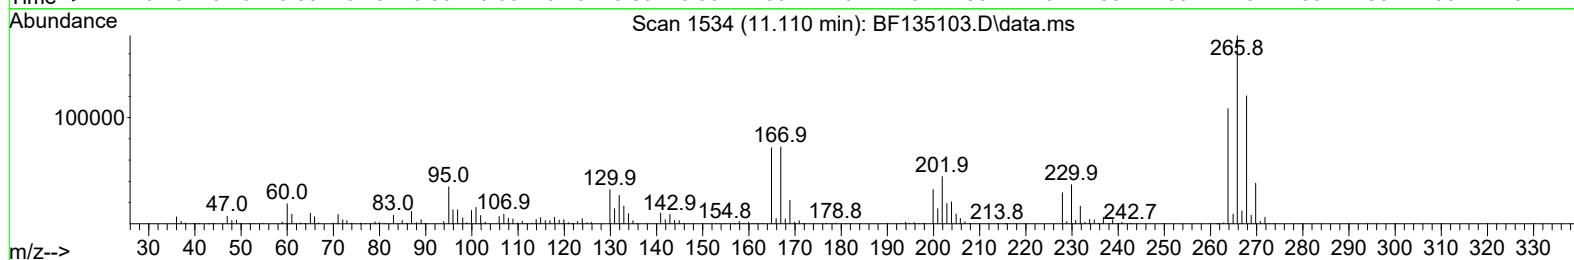


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090523\
Data File : BF135103.D
Acq On : 05 Sep 2023 19:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 08:09:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

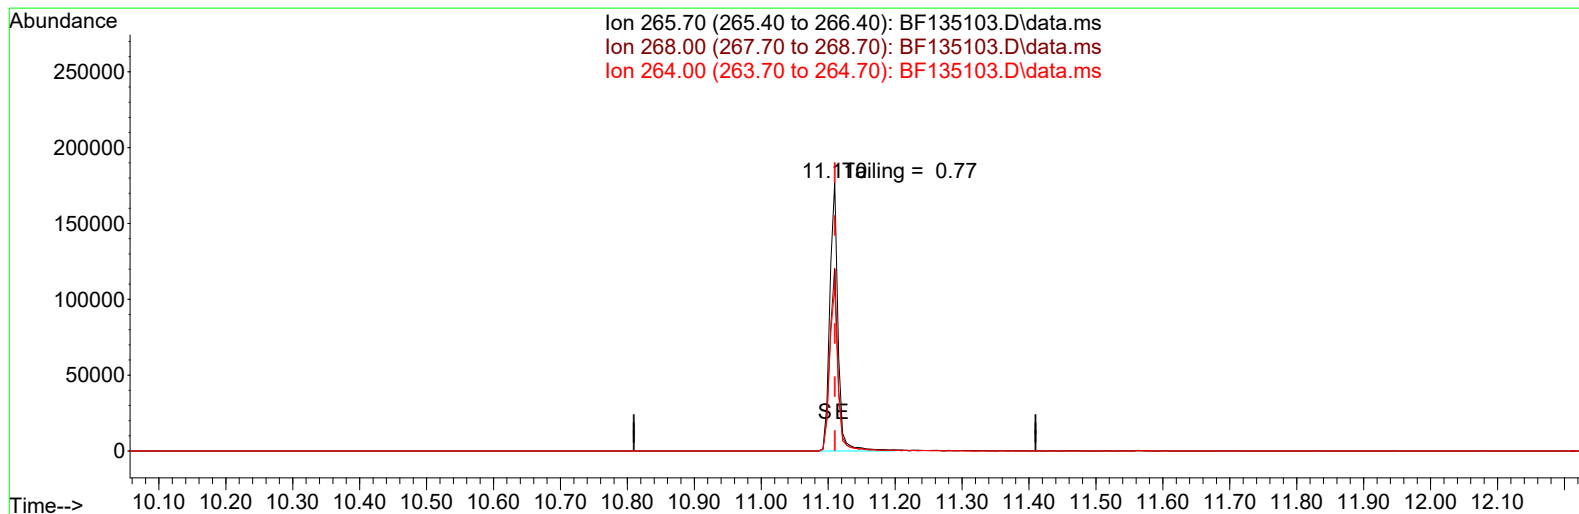

TIC: BF135103.D\data.ms

(70) Pentachlorophenol (C)




11.110min (+ 0.000) 410942.86 ng

response 152693

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	68.06
264.00	61.60	61.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090523\
Data File : BF135103.D
Acq On : 05 Sep 2023 19:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 06 08:09:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

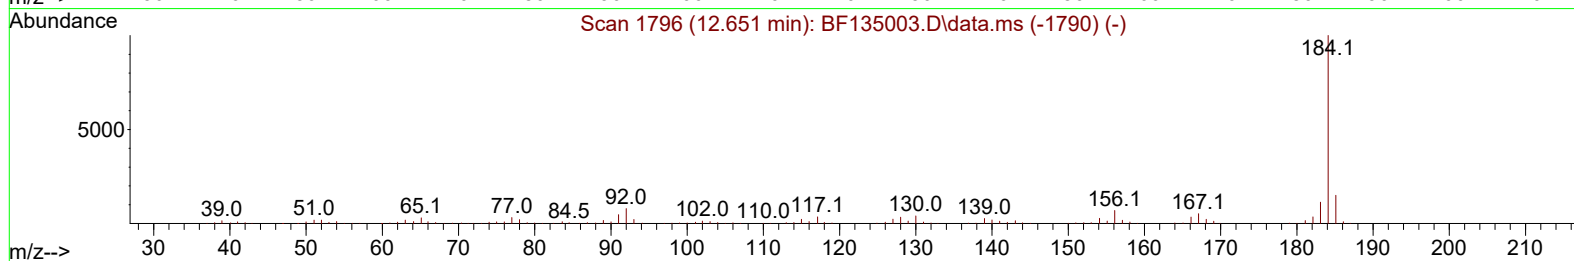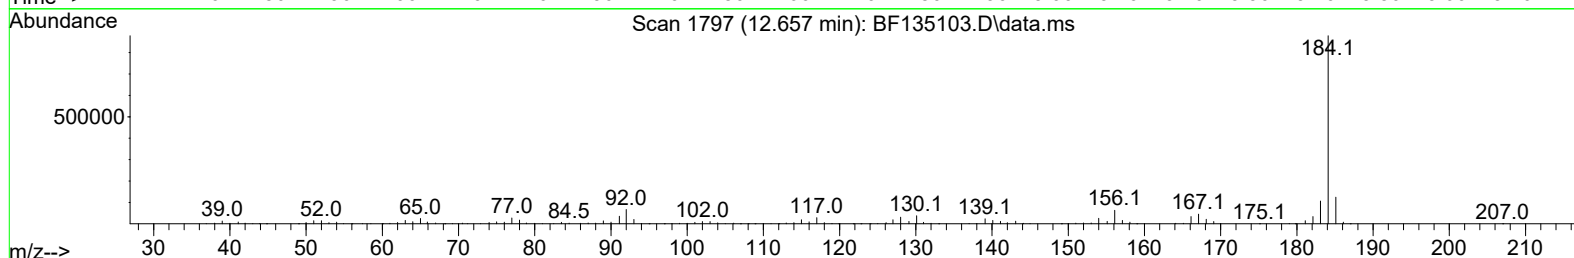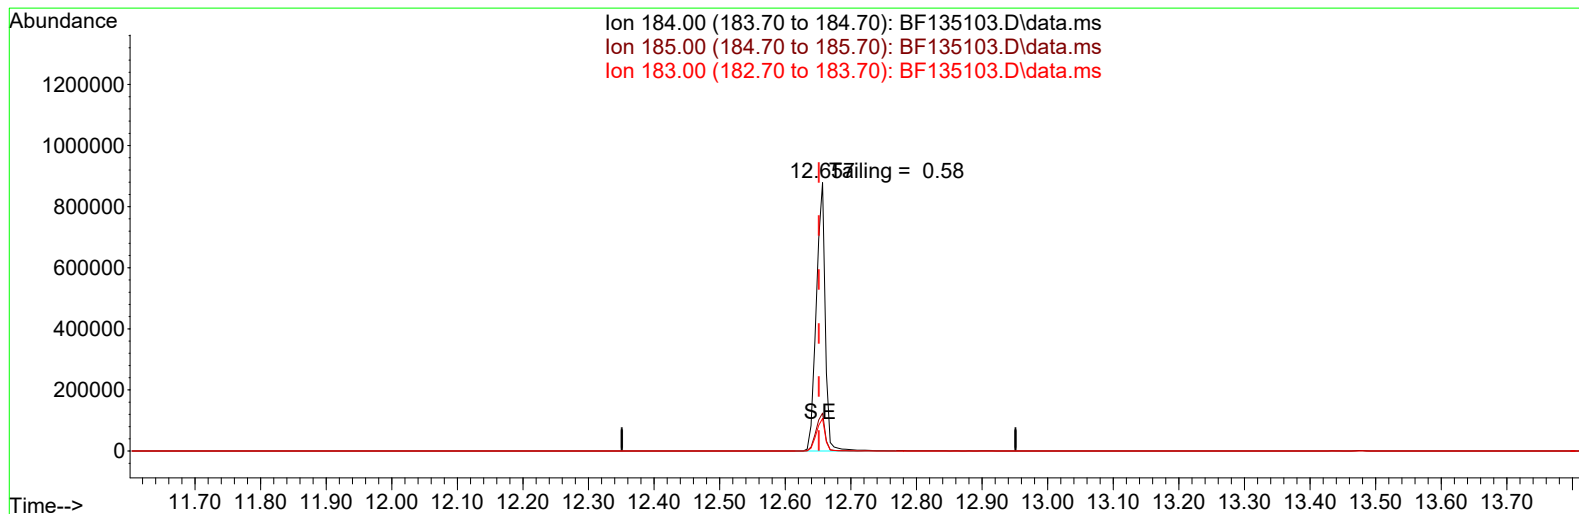

TIC: BF135103.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 325476.47 ng

response 839008

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.14
183.00	11.30	12.10
0.00	0.00	0.00