
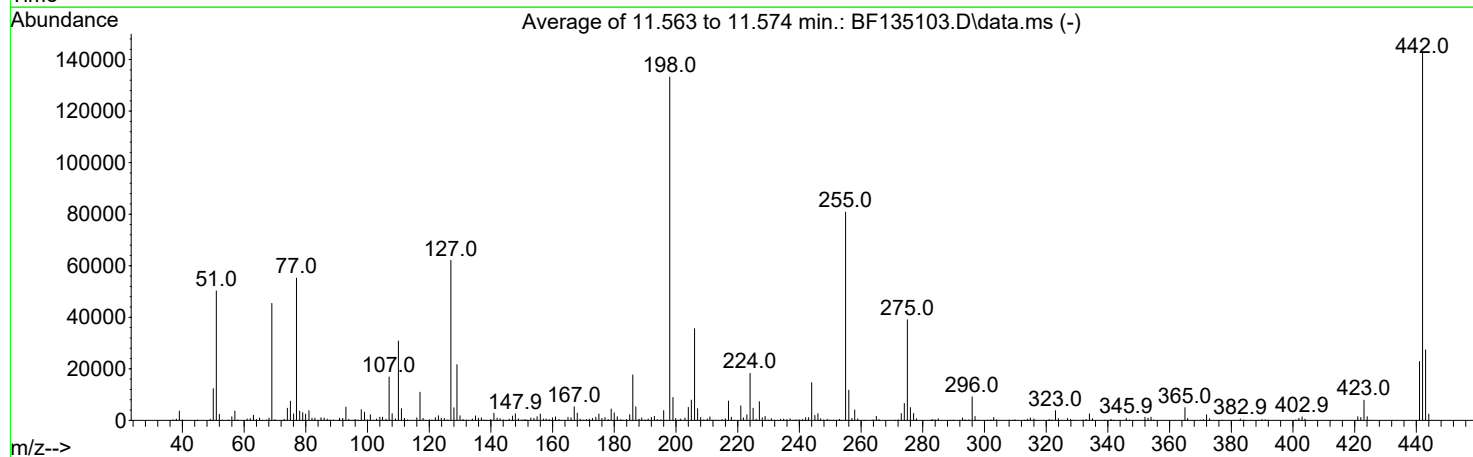


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090523\
Data File : BF135103.D
Acq On : 05 Sep 2023 19:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 31 03:48:08 2023

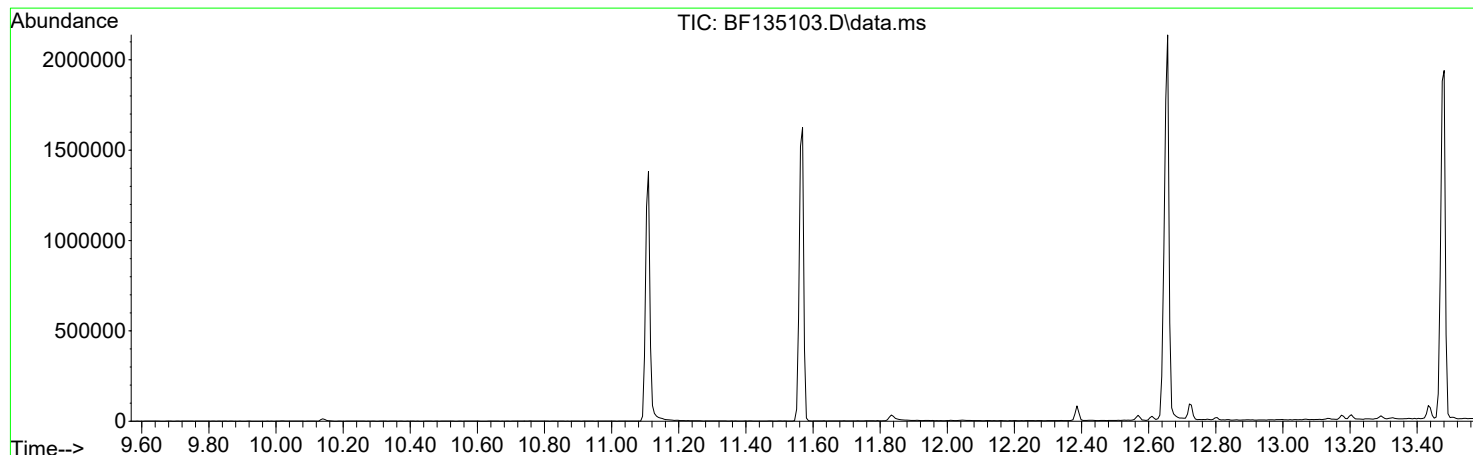




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	50229	PASS
68	69	0.00	2	1.9	853	PASS
69	198	0.00	100	34.0	45363	PASS
70	69	0.00	2	0.5	243	PASS
127	198	10	80	46.6	62065	PASS
197	198	0.00	2	0.1	93	PASS
198	198	100	100	100.0	133232	PASS
199	198	5	9	6.7	8874	PASS
275	198	10	60	29.3	39053	PASS
365	198	1	100	3.8	5001	PASS
441	198	0.01	100	17.1	22832	PASS
442	442	50	100	100.0	142757	PASS
443	442	15	24	19.2	27384	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090523\
Data File : BF135103.D
Acq On : 05 Sep 2023 19:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 06 08:09:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

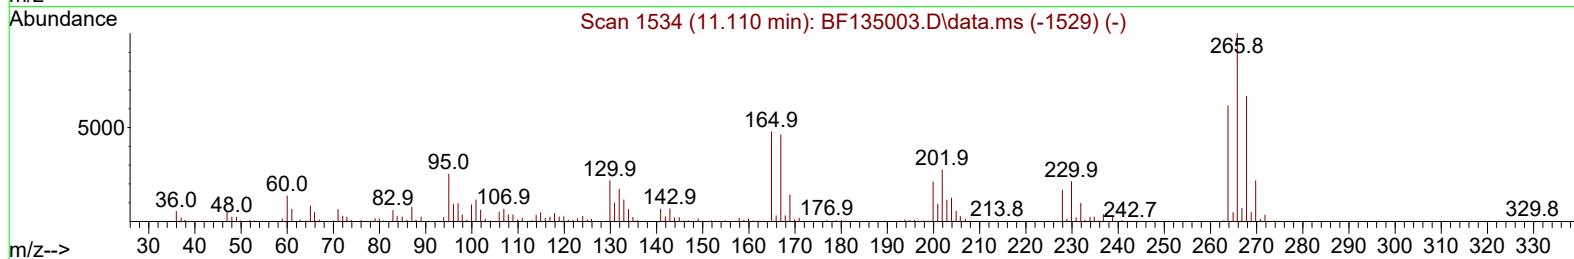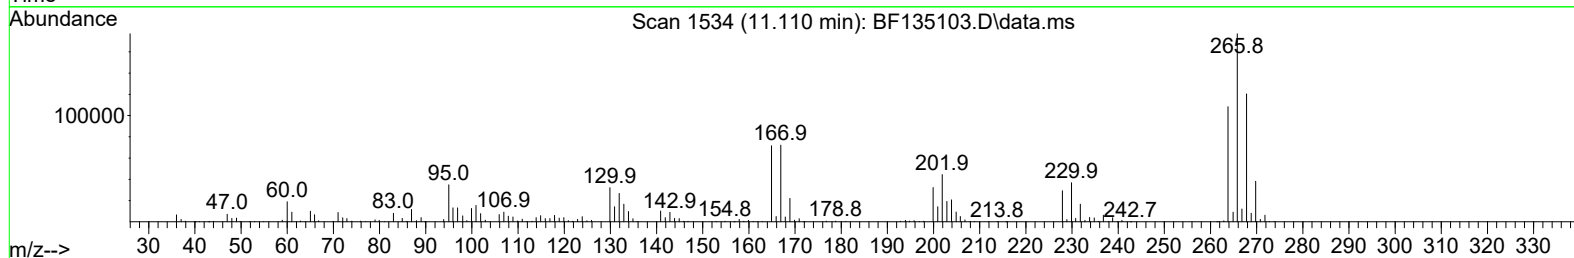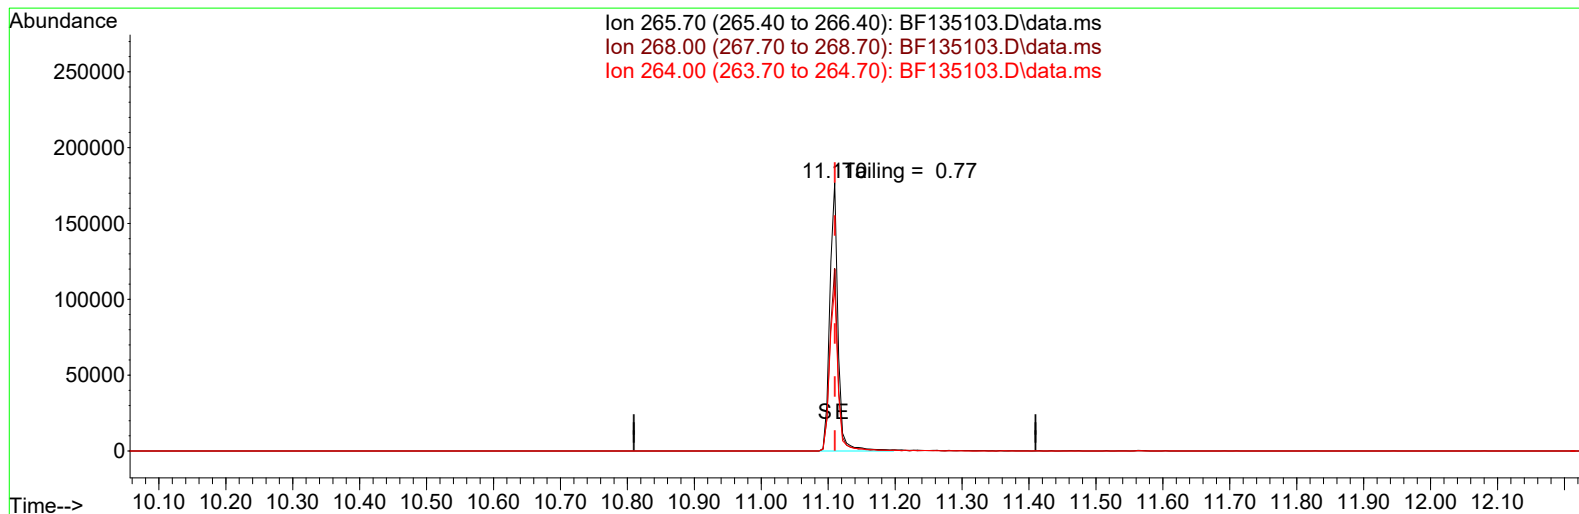

TIC: BF135103.D\data.ms

(70) Pentachlorophenol (C)

11.110min (+ 0.000) 410942.86 ng




response 152693

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	68.06
264.00	61.60	61.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090523\
Data File : BF135103.D
Acq On : 05 Sep 2023 19:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 06 08:09:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

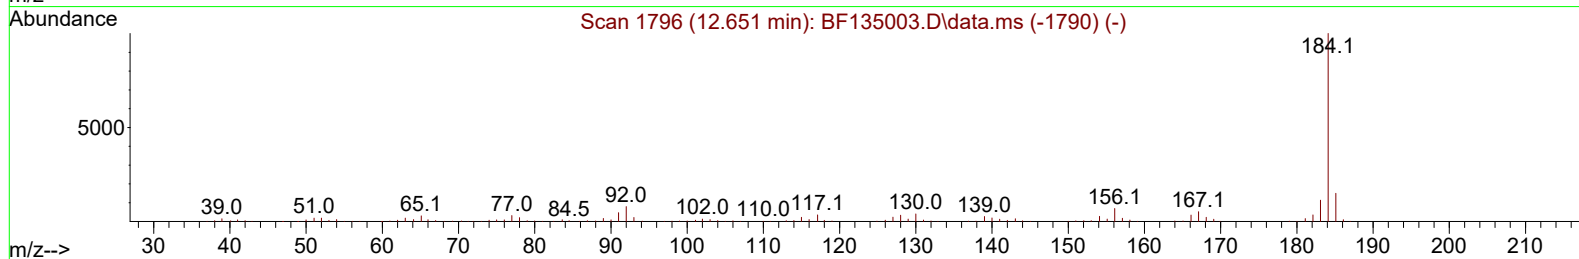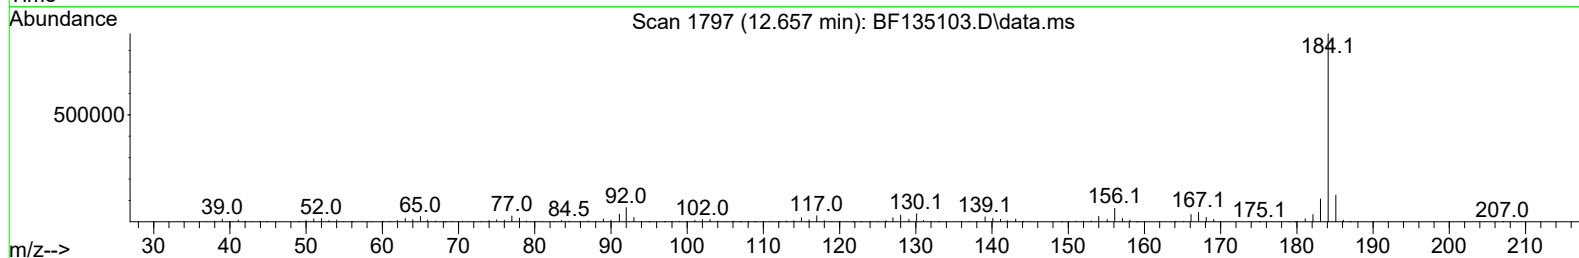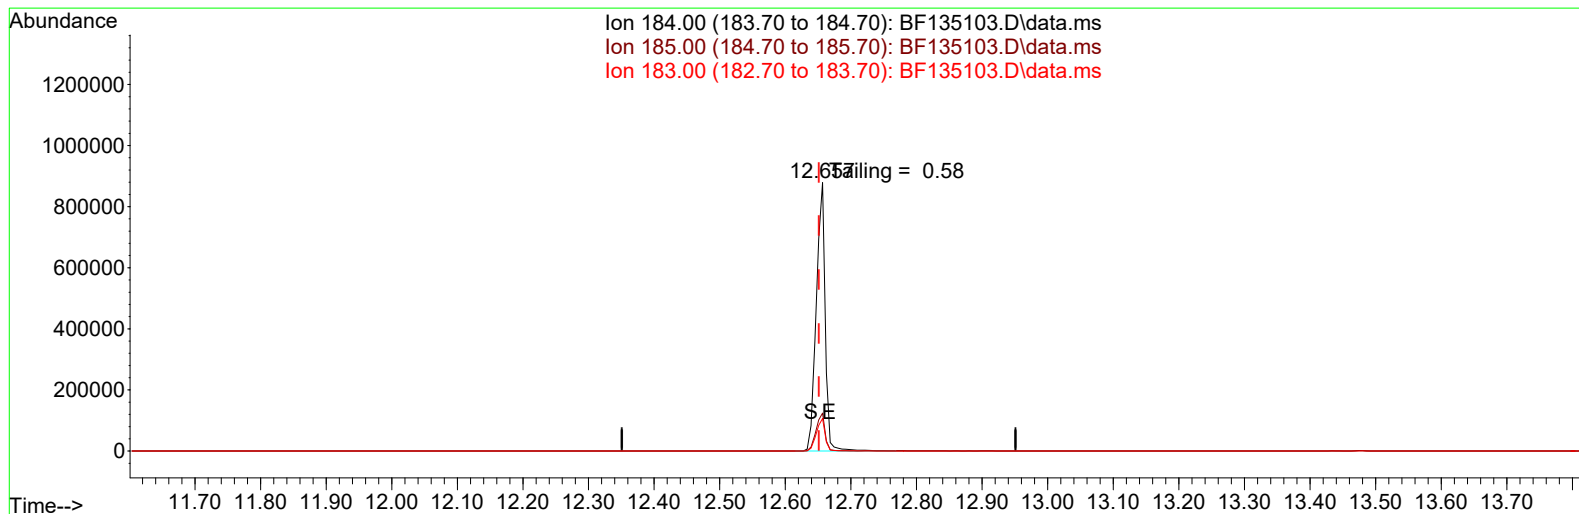

TIC: BF135103.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 325476.47 ng

response 839008

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.14
183.00	11.30	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/5/2023	BNA_F	<u>BF135103.D</u>
Compound Name	Response	Retention Time
DDT	365250	13.48
DDD	8616	13.204
DDE	205	12.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8821	374071	2.36

Instrument :
BNA_F
ClientSampleId :
DFTPP