

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090618\
 Data File : BF108833.D
 Acq On : 6 Sep 2018 19:47
 Operator : JU/SJ
 Sample : J4803-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EP1-Q2-F7

Quant Time: Sep 07 02:02:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 05 18:03:31 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	287339	20.00	ng	0.00
21) Naphthalene-d8	8.02	136	1122985	20.00	ng	0.00
38) Acenaphthene-d10	9.77	164	531501	20.00	ng	0.00
63) Phenanthrene-d10	11.24	188	896756	20.00	ng	0.00
75) Chrysene-d12	13.87	240	644952	20.00	ng	0.00
86) Perylene-d12	15.27	264	731449	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	1201249	69.26	ng	0.01
7) Phenol-d6	6.37	99	1563456	70.06	ng	0.00
23) Nitrobenzene-d5	7.30	82	973940	54.28	ng	0.00
41) 2,4,6-Tribromophenol	10.55	330	356026	70.17	ng	0.00
44) 2-Fluorobiphenyl	9.10	172	1718288	55.15	ng	0.00
78) Terphenyl-d14	12.82	244	1351058	48.85	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.48	163	563378	15.155	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090618\
Data File : BF108833.D
Acq On : 6 Sep 2018 19:47
Operator : JU/SJ
Sample : J4803-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EP1-Q2-F7

Quant Time: Sep 07 02:02:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 05 18:03:31 2018
Response via : Initial Calibration

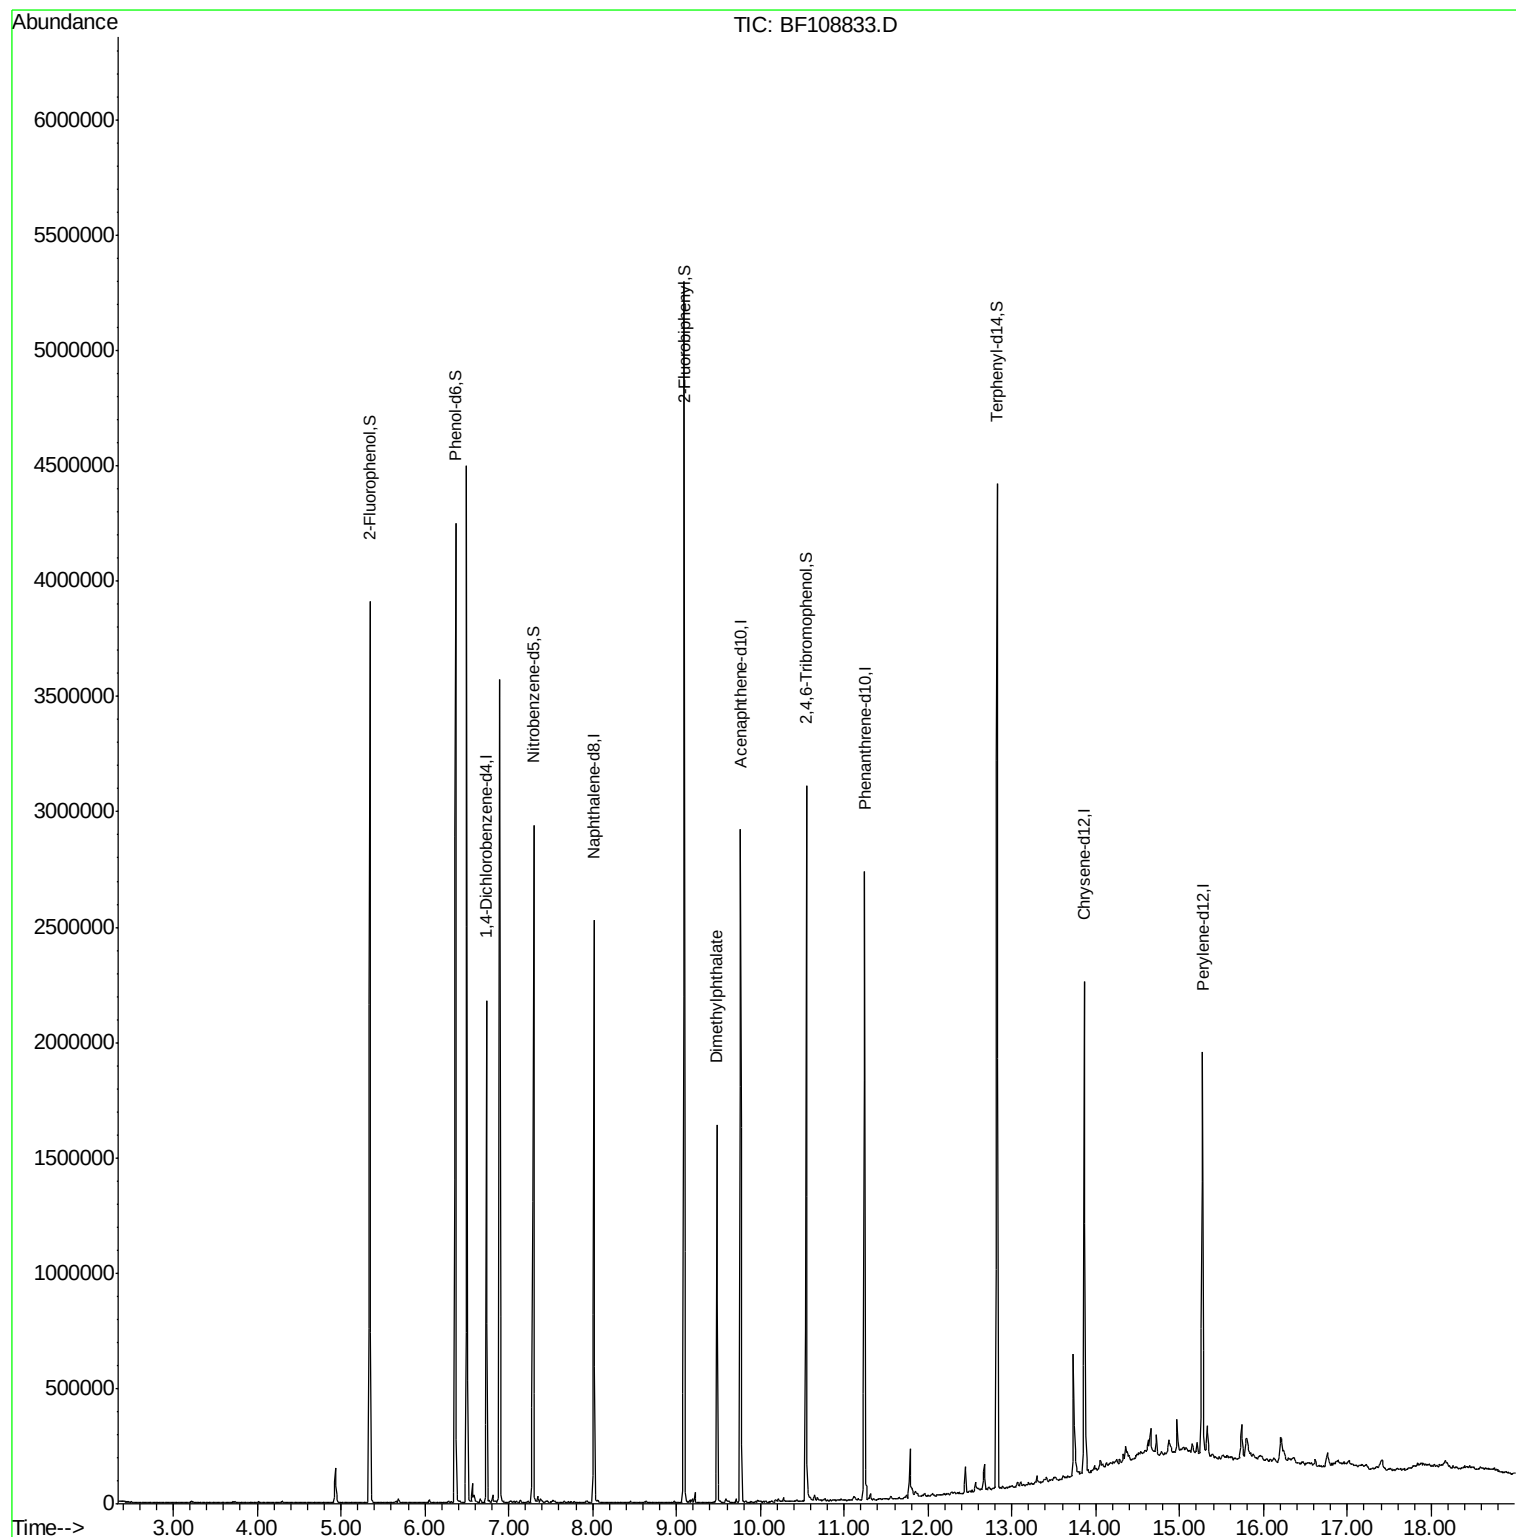

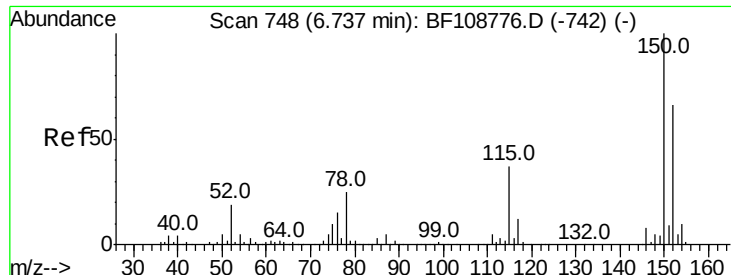


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.74 min Scan# 748
Delta R.T. 0.00 min
Lab File: BF108833.D
Acq: 6 Sep 2018 19:47

Instrument :
BNA_F
ClientSampleId :
EP1-Q2-F7

Tot Ion:152 Resp: 287339
Ion Ratio Lower Upper
152 100
150 158.5 124.6 186.8
115 61.3 50.1 75.1

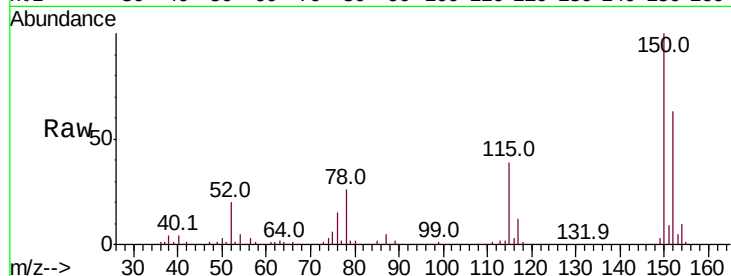


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

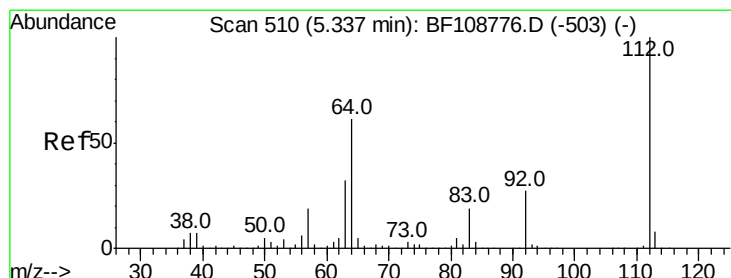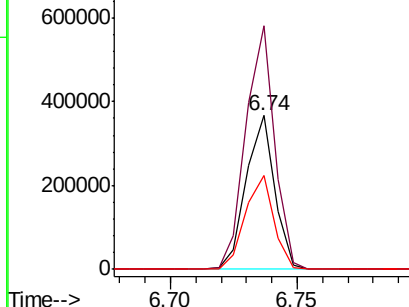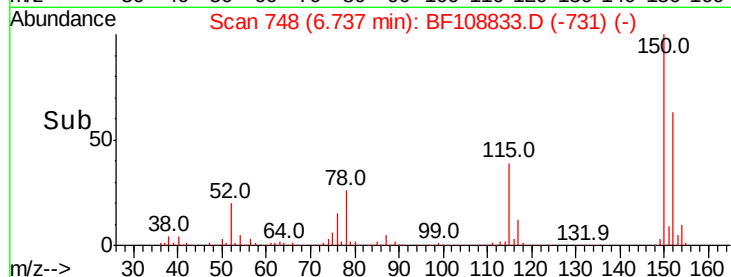



#5


2-Fluorophenol
Concen: 69.259 ng
RT: 5.35 min Scan# 512
Delta R.T. 0.01 min
Lab File: BF108833.D
Acq: 6 Sep 2018 19:47

Tgt Ion:112 Resp: 1201249
Ion Ratio Lower Upper
112 100
64 55.7 47.9 71.9
63 28.6 23.7 35.5

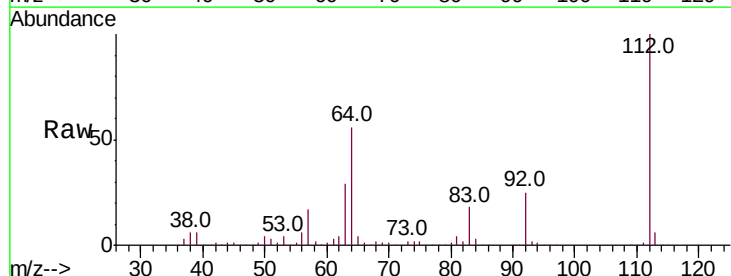

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

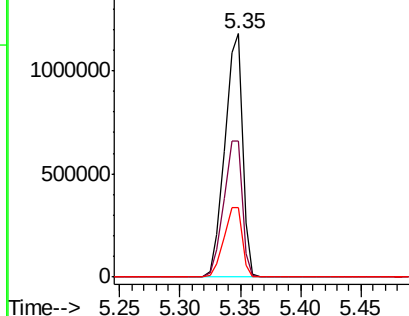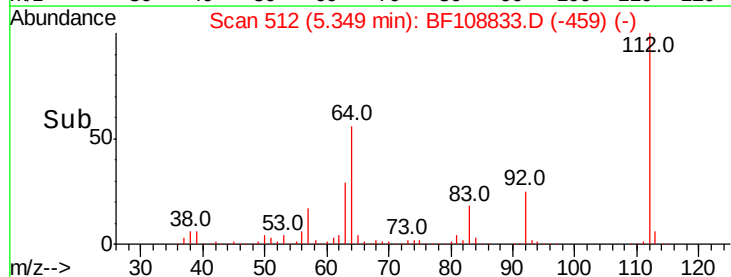

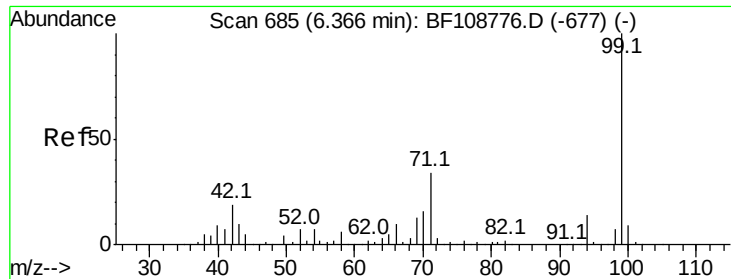

#7

Phenol-d6

Concen: 70.059 ng

RT: 6.37 min Scan# 685

Delta R.T. 0.00 min

Lab File: BF108833.D

Acq: 6 Sep 2018 19:47

Instrument :

BNA_F

ClientSampleId :

EP1-Q2-F7


Tot Ion: 99 Resp: 1563456

Ion Ratio Lower Upper




99 100

42 19.4 14.5 21.7

71 34.3 25.4 38.0

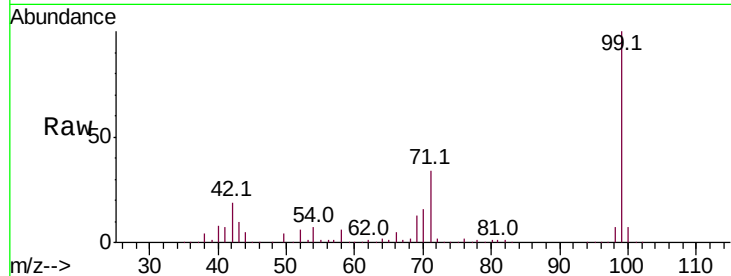

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

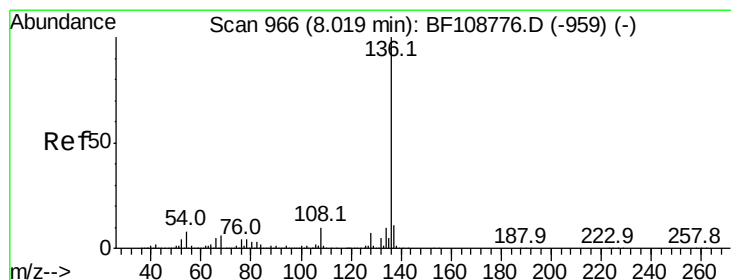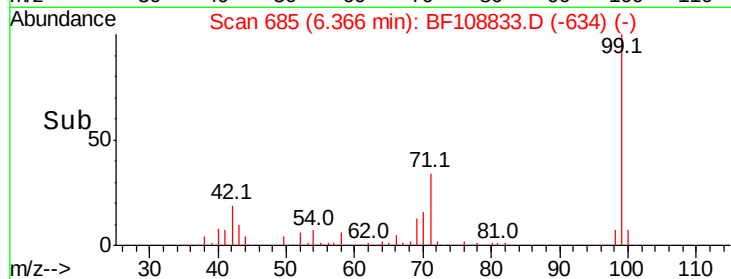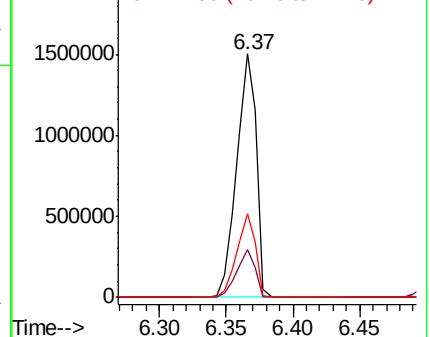

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.02 min Scan# 966

Delta R.T. 0.00 min

Lab File: BF108833.D

Acq: 6 Sep 2018 19:47

Tgt Ion: 136 Resp: 1122985


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3


54 7.4 6.6 9.8

68 6.4 5.0 7.4

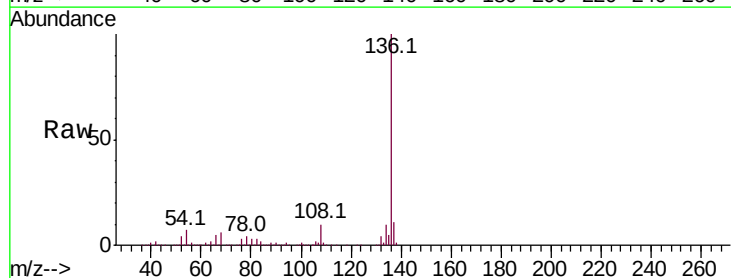

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

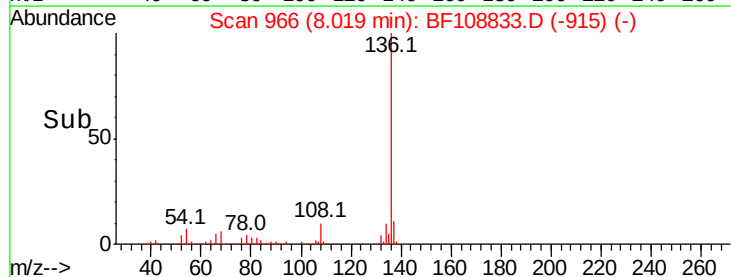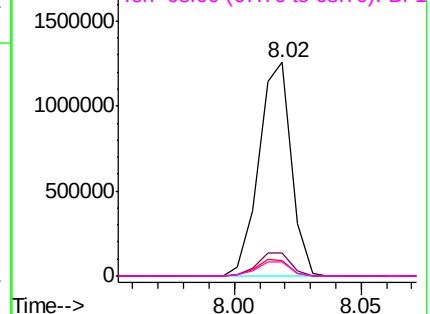


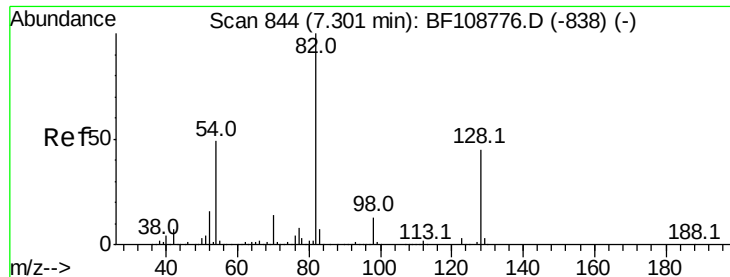




#23
 Nitrobenzene-d5
 Concen: 54.275 ng
 RT: 7.30 min Scan# 843
 Delta R.T. -0.01 min
 Lab File: BF108833.D
 Acq: 6 Sep 2018 19:47

Instrument :
 BNA_F
 ClientSampleId :
 EP1-Q2-F7

Tot Ion: 82 Resp: 973940
 Ion Ratio Lower Upper
 82 100
 128 46.5 36.1 54.1
 54 46.0 41.4 62.2

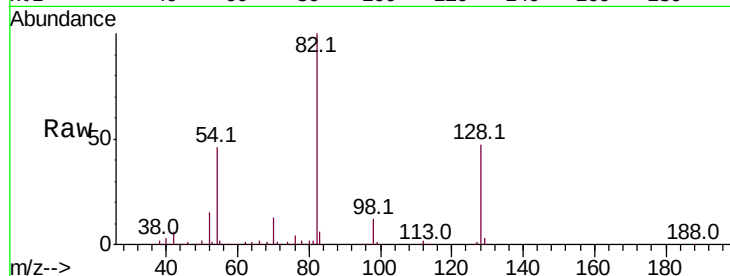


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

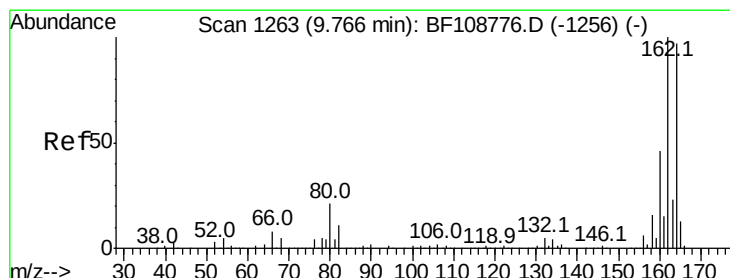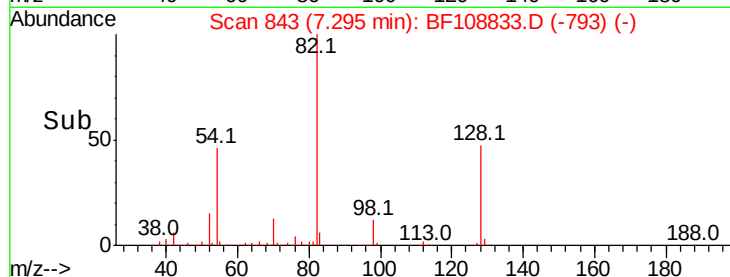
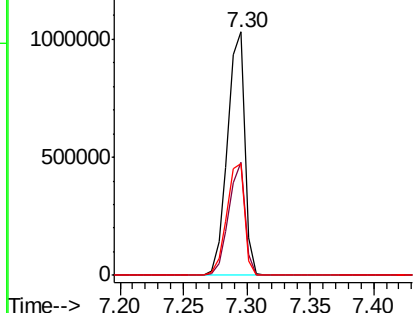



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.77 min Scan# 1263
 Delta R.T. 0.00 min
 Lab File: BF108833.D
 Acq: 6 Sep 2018 19:47

Tgt Ion:164 Resp: 531501
 Ion Ratio Lower Upper
 164 100
 162 101.7 86.1 129.1
 160 46.7 38.3 57.5

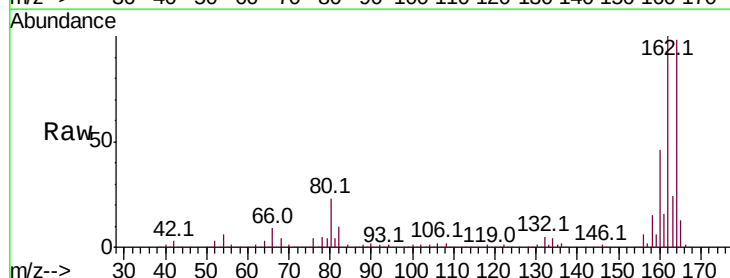

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



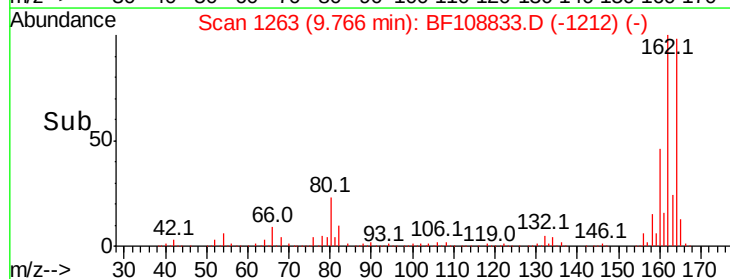
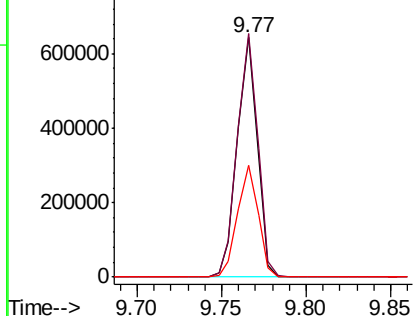


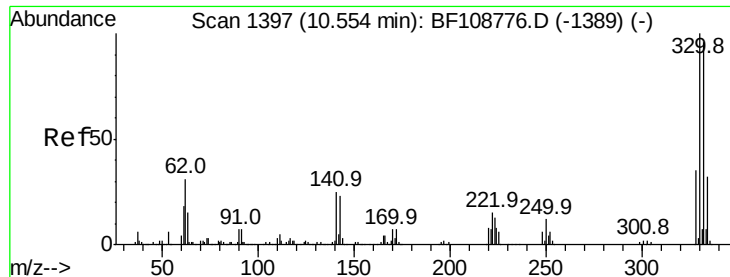

#41
 2,4,6-Tribromophenol
 Concen: 70.167 ng
 RT: 10.55 min Scan# 1396
 Delta R.T. -0.01 min
 Lab File: BF108833.D
 Acq: 6 Sep 2018 19:47




Instrument :
 BNA_F
 ClientSampled :
 EP1-Q2-F7


Tot Ion:330 Resp: 356026
 Ion Ratio Lower Upper
 330 100
 332 96.1 77.0 115.6
 141 32.4 29.9 44.9

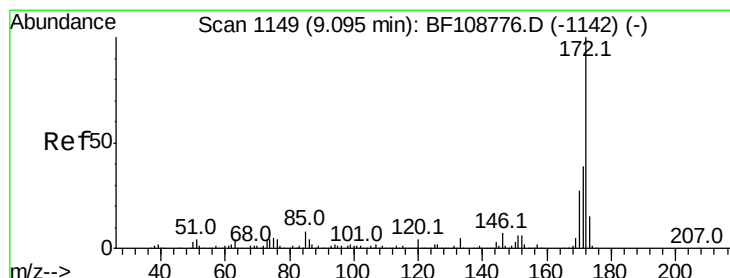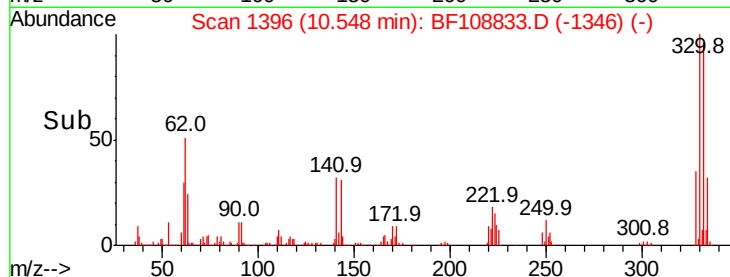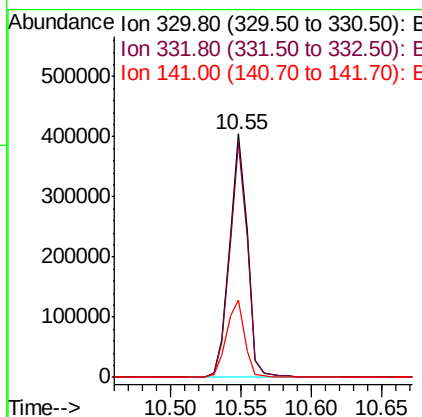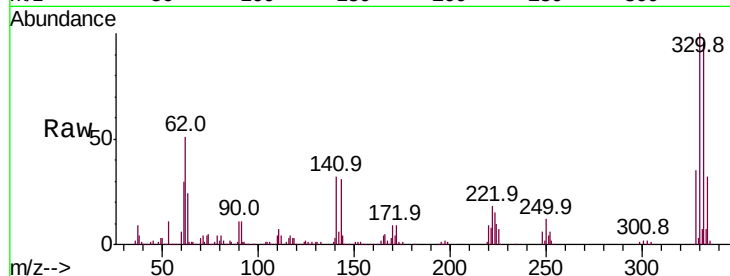

#44
 2-Fluorobiphenyl
 Concen: 55.153 ng
 RT: 9.10 min Scan# 1149
 Delta R.T. 0.00 min
 Lab File: BF108833.D
 Acq: 6 Sep 2018 19:47

Tgt Ion:172 Resp: 1718288
 Ion Ratio Lower Upper
 172 100
 171 36.5 29.7 44.5
 170 25.0 19.6 29.4

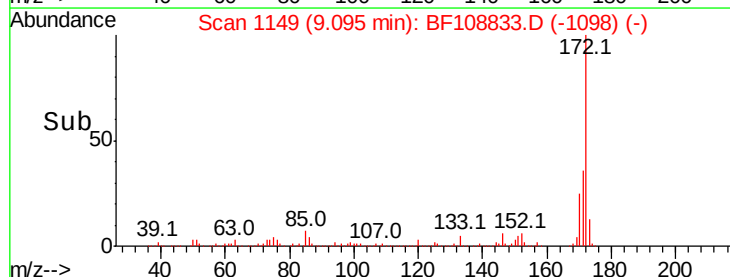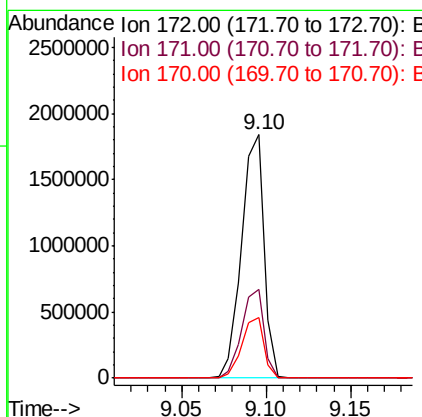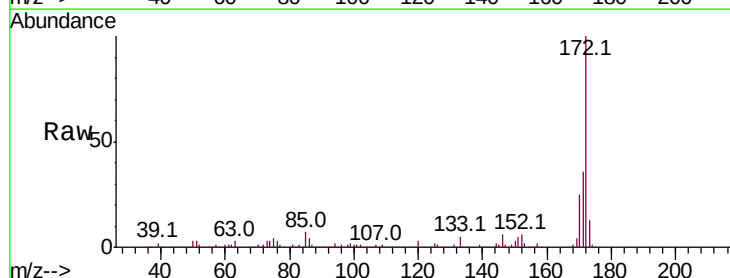


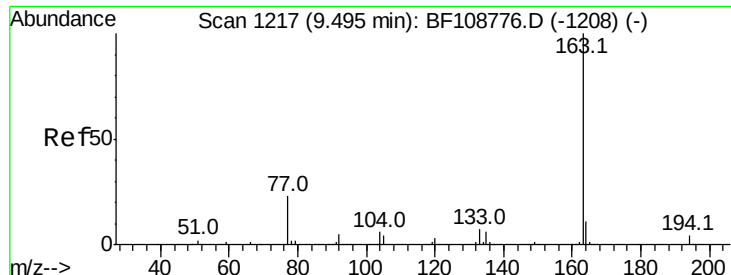




#49
Dimethylphthalate
Concen: 15.155 ng
RT: 9.48 min Scan# 1215
Delta R.T. -0.01 min
Lab File: BF108833.D
Acq: 6 Sep 2018 19:47

Instrument :
BNA_F
ClientSampleId :
EP1-Q2-F7

Tot Ion:163 Resp: 563378
Ion Ratio Lower Upper
163 100
194 3.8 2.7 4.1
164 10.6 8.2 12.2

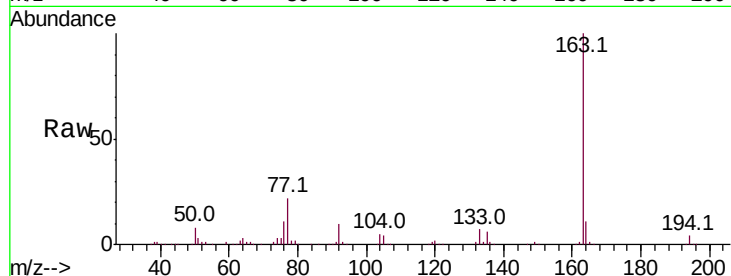


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

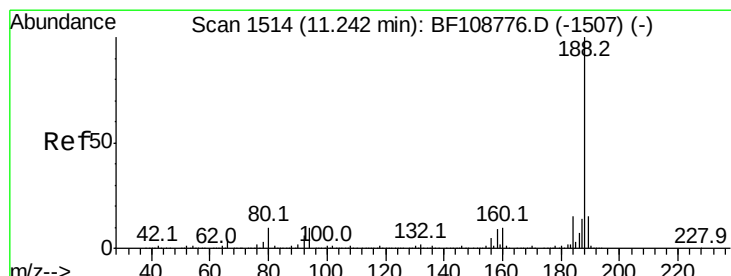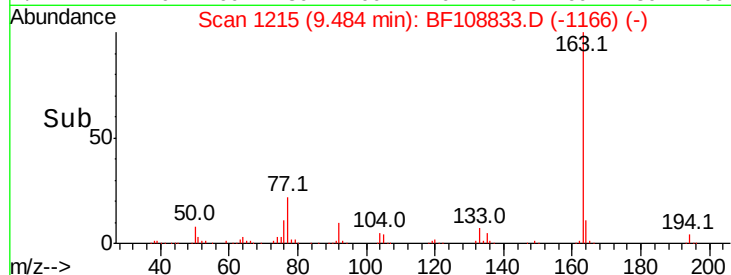
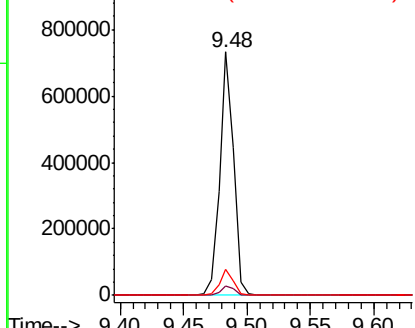



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.24 min Scan# 1514
Delta R.T. 0.00 min
Lab File: BF108833.D
Acq: 6 Sep 2018 19:47

Tgt Ion:188 Resp: 896756
Ion Ratio Lower Upper
188 100
94 11.0 8.5 12.7
80 11.7 9.2 13.8

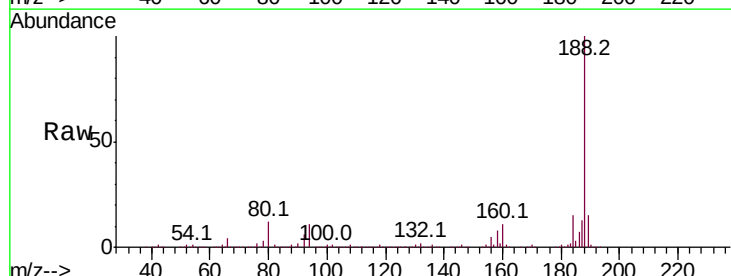

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

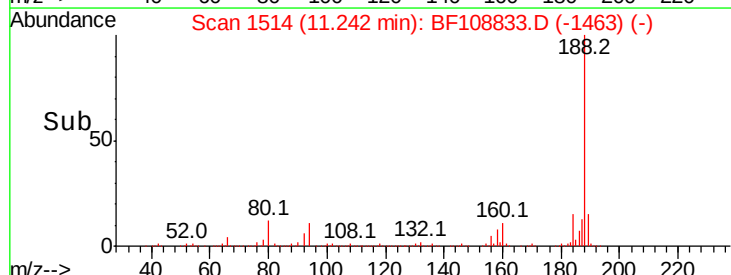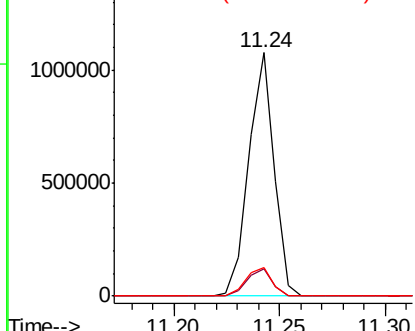

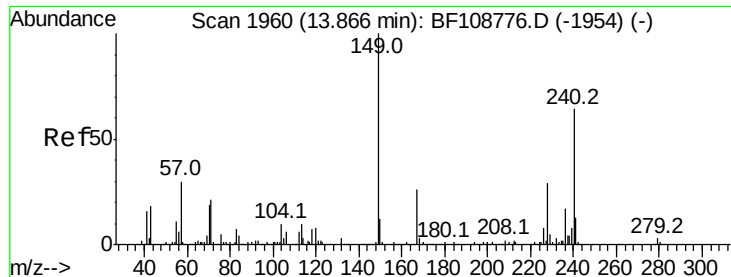

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.87 min Scan# 1960

Delta R.T. 0.00 min

Lab File: BF108833.D

Acq: 6 Sep 2018 19:47

Instrument :

BNA_F

ClientSampleId :

EP1-Q2-F7


Tot Ion:240 Resp: 644952

Ion Ratio Lower Upper

240 100

120 12.5 9.5 14.3




236 26.8 20.7 31.1

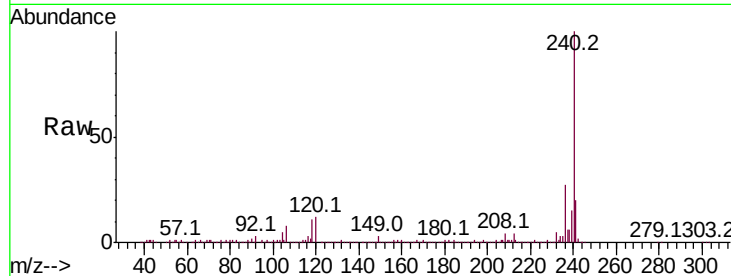

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

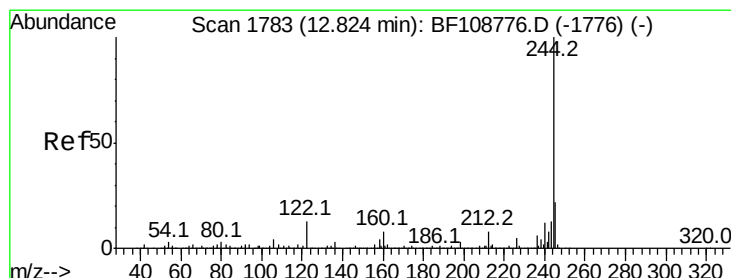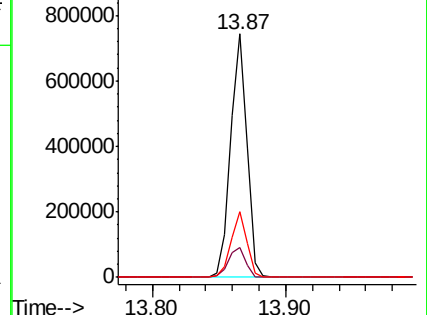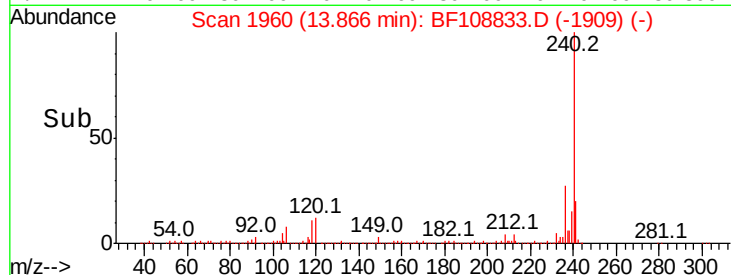

#78

Terphenyl-d14

Concen: 48.849 ng

RT: 12.82 min Scan# 1783

Delta R.T. 0.00 min

Lab File: BF108833.D

Acq: 6 Sep 2018 19:47


Tgt Ion:244 Resp: 1351058

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0



122 12.3 11.0 16.4

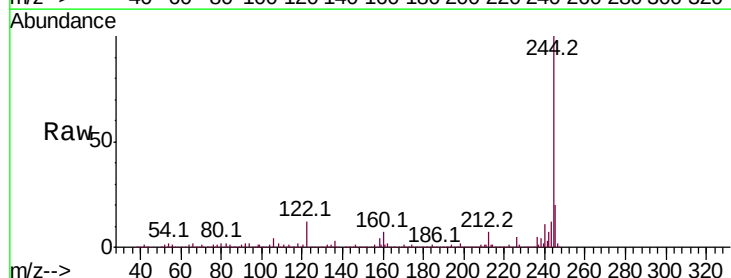


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

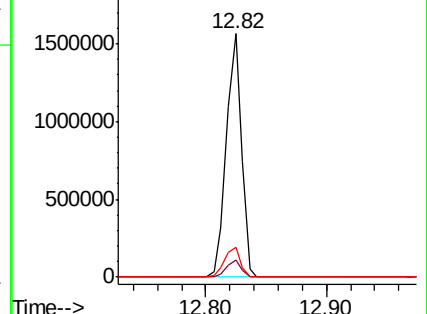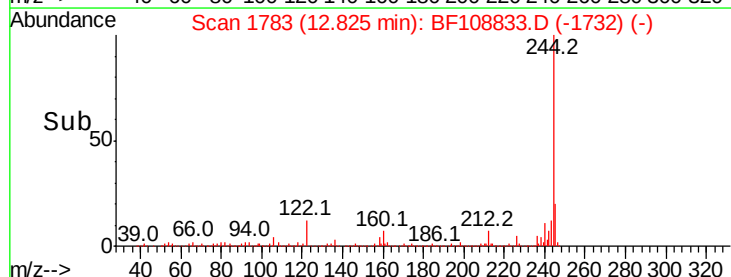

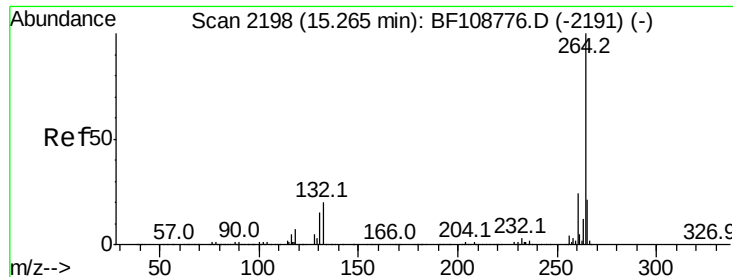

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.27 min Scan# 2199
Delta R.T. 0.01 min
Lab File: BF108833.D
Acq: 6 Sep 2018 19:47

Instrument :
BNA_F
ClientSampleId :
EP1-Q2-F7

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.2	28.8
265	21.3	17.5	26.3

