


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090619\
Data File : BF116852.D
Acq On : 6 Sep 2019 9:28
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 09 16:37:52 2019

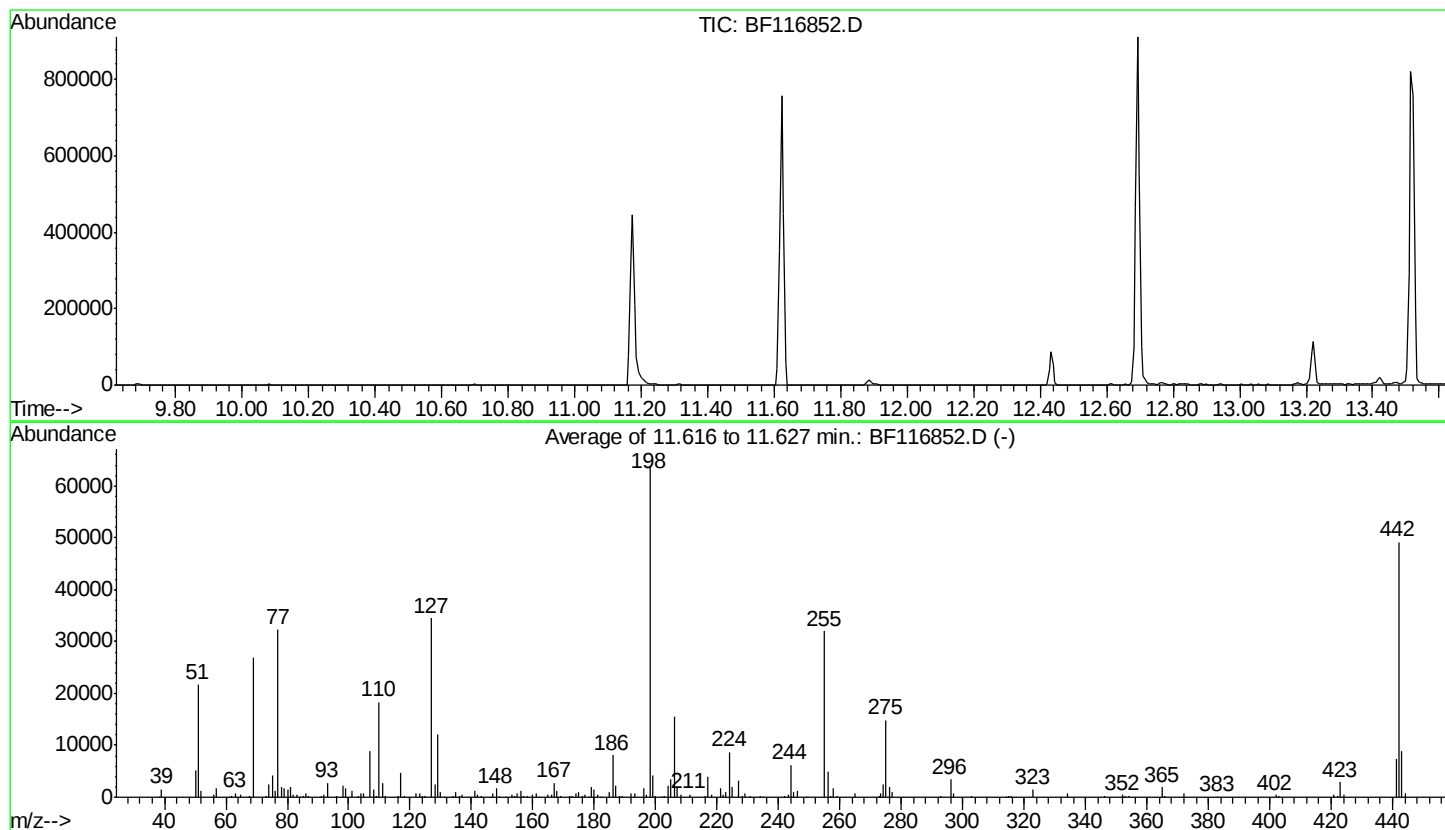

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	21692	PASS
68	69	0.00	2	1.4	376	PASS
69	198	0.00	100	42.0	26808	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.9	34424	PASS
197	198	0.00	2	0.6	394	PASS
198	198	100	100	100.0	63898	PASS
199	198	5	9	6.7	4311	PASS
275	198	10	60	23.2	14841	PASS
365	198	1	100	2.9	1863	PASS
441	198	0.01	100	11.7	7491	PASS
442	198	50	100	76.9	49152	PASS
443	442	15	24	18.3	8991	PASS