


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090619\
 Data File : BF116872.D
 Acq On : 6 Sep 2019 22:17
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 09 16:37:52 2019

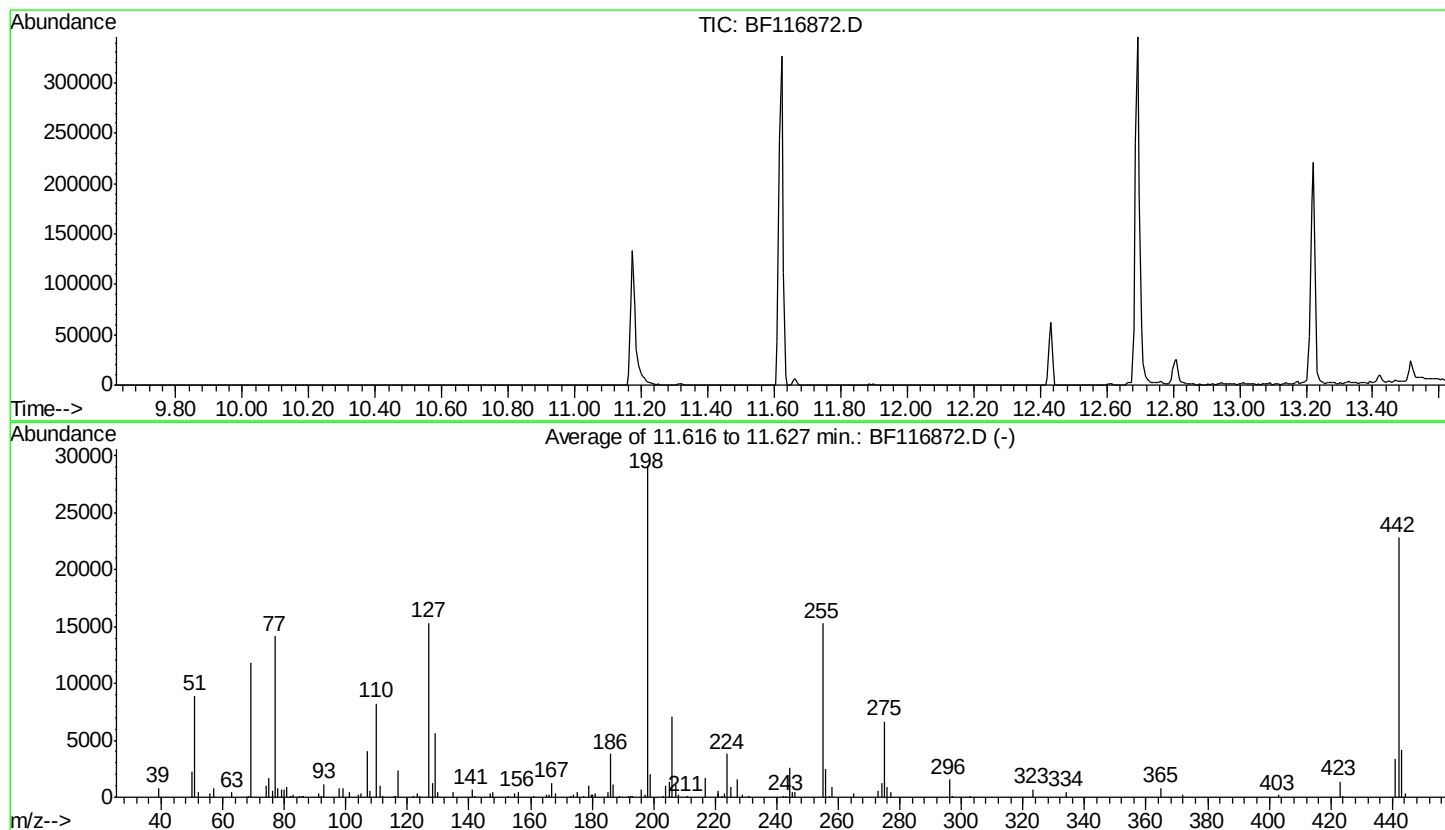

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	8925	PASS
68	69	0.00	2	1.0	113	PASS
69	198	0.00	100	40.5	11797	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	15340	PASS
197	198	0.00	2	1.0	281	PASS
198	198	100	100	100.0	29144	PASS
199	198	5	9	7.1	2071	PASS
275	198	10	60	22.9	6671	PASS
365	198	1	100	2.8	803	PASS
441	198	0.01	100	11.6	3378	PASS
442	198	50	100	78.3	22806	PASS
443	442	15	24	18.4	4197	PASS