

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090723\
 Data File : BF135133.D
 Acq On : 07 Sep 2023 14:26
 Operator : CG\JU
 Sample : 04283-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-3

Quant Time: Sep 07 17:17:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 31 03:48:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.769	152	104286	20.000	ng	0.00
21) Naphthalene-d8	8.051	136	422441	20.000	ng	0.00
39) Acenaphthene-d10	9.810	164	213552	20.000	ng	0.00
64) Phenanthrene-d10	11.298	188	369525	20.000	ng	-0.01
76) Chrysene-d12	13.957	240	189758	20.000	ng	0.00
86) Perylene-d12	15.427	264	208239	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.404	112	509856	75.517	ng	0.00
7) Phenol-d6	6.410	99	611964	72.720	ng	0.00
23) Nitrobenzene-d5	7.334	82	384046	51.075	ng	-0.01
42) 2,4,6-Tribromophenol	10.598	330	162200	71.601	ng	-0.01
45) 2-Fluorobiphenyl	9.128	172	704285	53.694	ng	-0.01
79) Terphenyl-d14	12.898	244	636883	54.771	ng	0.00
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	7.334	70	50874	10.177	ng	# 78
25) Isophorone	7.334	82	384040	26.938	ng	# 65
50) Dimethylphthalate	9.810	163	43296	2.895	ng	# 1
51) 2,6-Dinitrotoluene	9.810	165	27427	8.359	ng	# 22
57) 2,4-Dinitrotoluene	9.810	165	27427	6.708	ng	# 20
67) 4-Bromophenyl-phenylether	10.598	248	10586	2.701	ng	# 1
77) Benzidine	12.898	184	8441	2.468	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090723\
Data File : BF135133.D
Acq On : 07 Sep 2023 14:26
Operator : CG\JU
Sample : 04283-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Time: Sep 07 17:17:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration




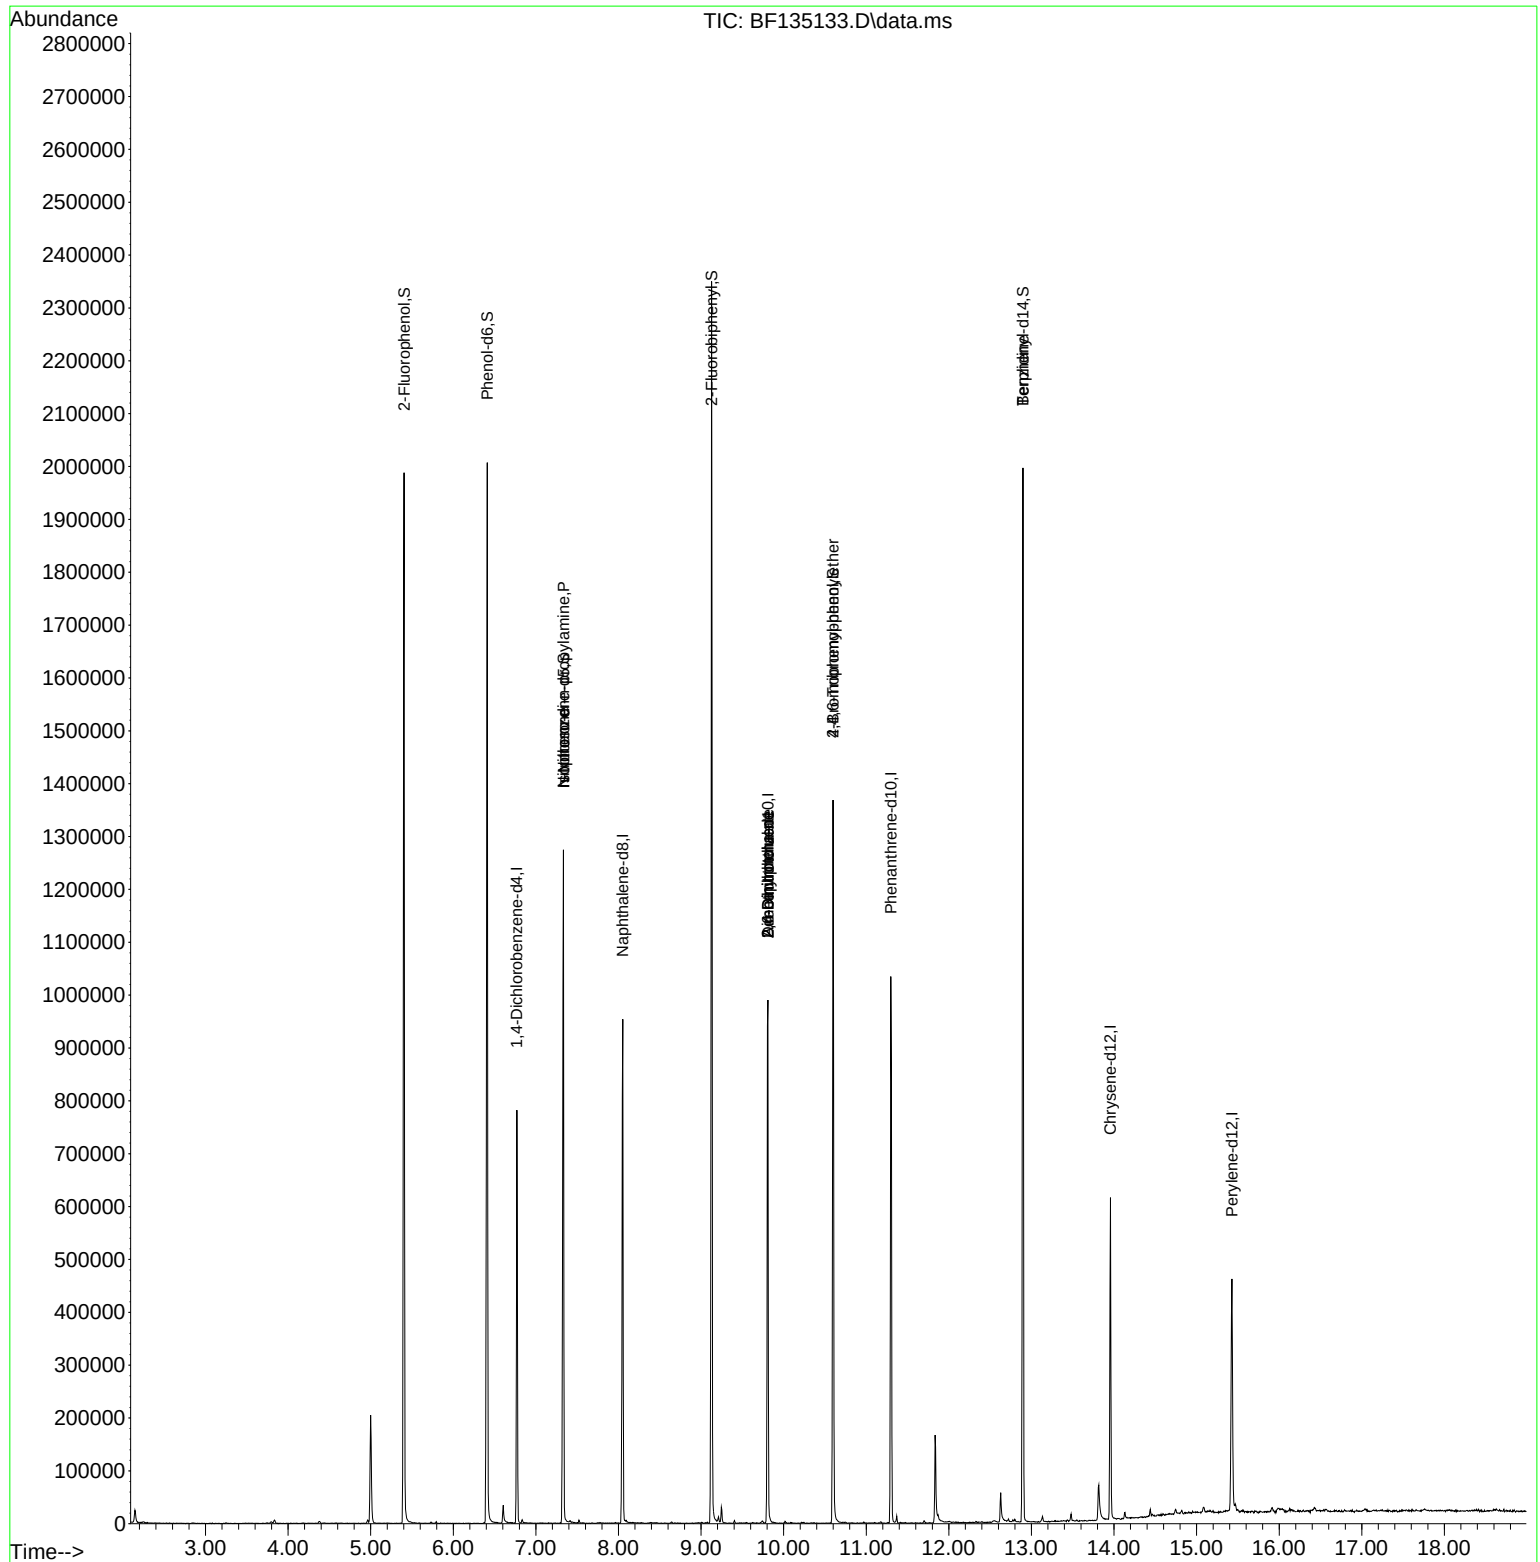


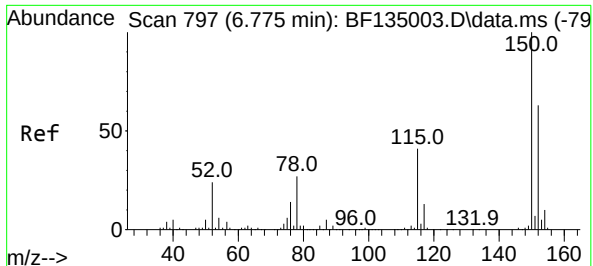

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.769 min Scan# 797
Delta R.T. -0.006 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26




Instrument :
BNA_F
ClientSampleId :
SB-3


Tgt Ion:152 Resp: 104286
Ion Ratio Lower Upper
152 100
150 155.4 126.2 189.4
115 65.1 51.2 76.8

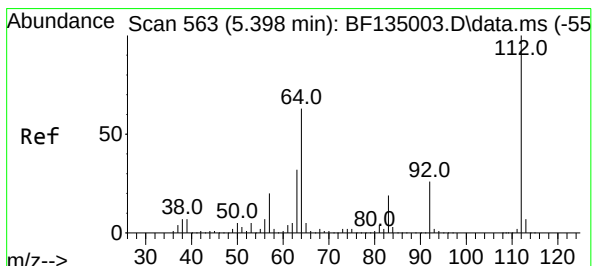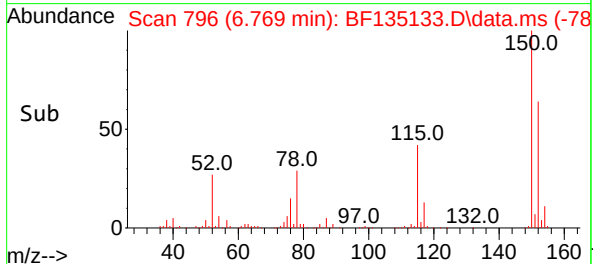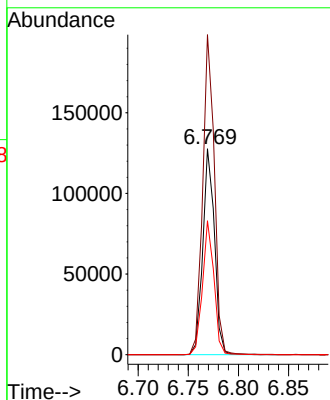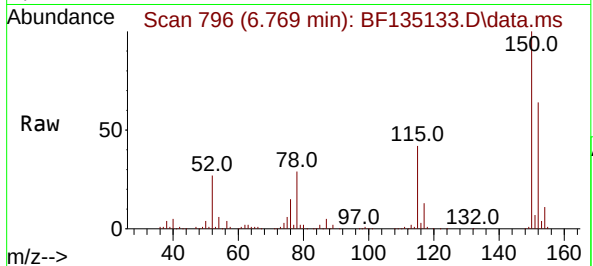

#5
2-Fluorophenol
Concen: 75.517 ng
RT: 5.404 min Scan# 564
Delta R.T. 0.006 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26

Tgt Ion:112 Resp: 509856
Ion Ratio Lower Upper
112 100
64 60.9 50.5 75.7
63 31.6 25.9 38.9


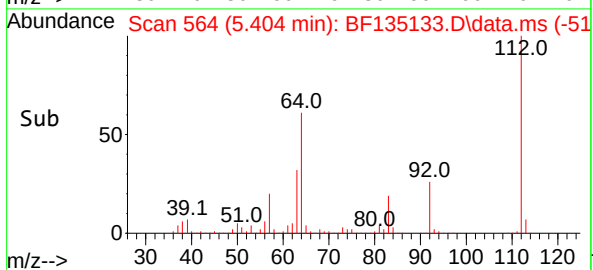
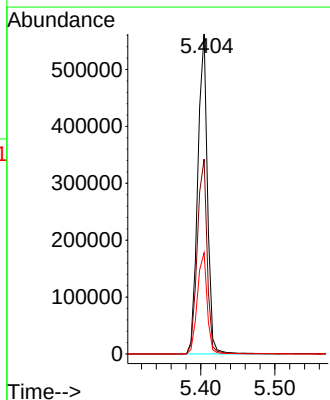
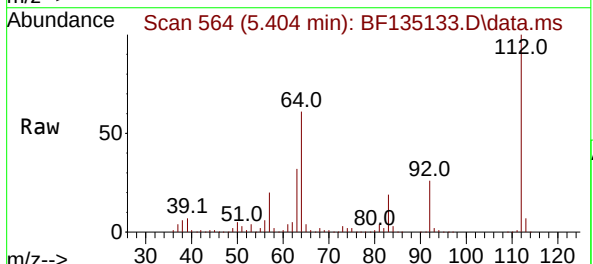


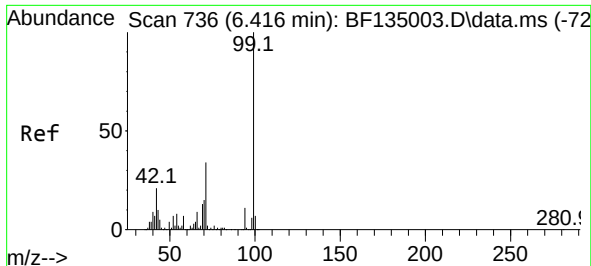

#7
Phenol-d6
Concen: 72.720 ng
RT: 6.410 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26




Instrument :
BNA_F
ClientSampleId :
SB-3


Tgt Ion: 99 Resp: 611964
Ion Ratio Lower Upper
99 100
42 20.8 16.6 25.0
71 36.2 27.0 40.6

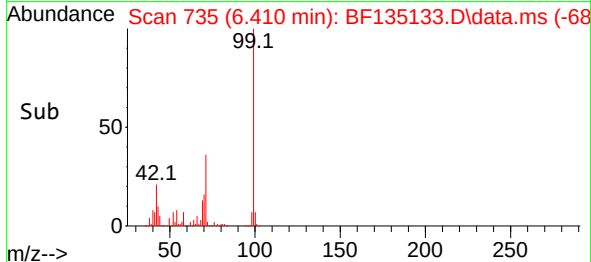

#19
n-Nitroso-di-n-propylamine
Concen: 10.177 ng
RT: 7.334 min Scan# 892
Delta R.T. 0.135 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26

Tgt Ion: 70 Resp: 50874
Ion Ratio Lower Upper
70 100
42 52.7 50.2 75.4
101 0.0 8.1 12.1#
130 2.0 19.3 28.9#


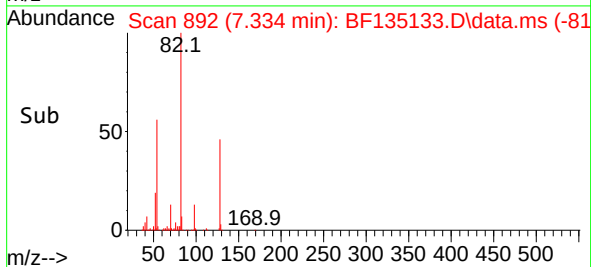

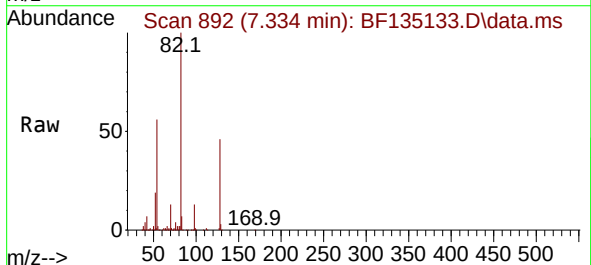




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.051 min Scan# 1014
Delta R.T. -0.006 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26




Instrument :
BNA_F
ClientSampleId :
SB-3


Tgt Ion:136 Resp: 422441
Ion Ratio Lower Upper
136 100
137 10.5 8.8 13.2
54 7.9 7.0 10.4
68 5.2 4.6 6.8

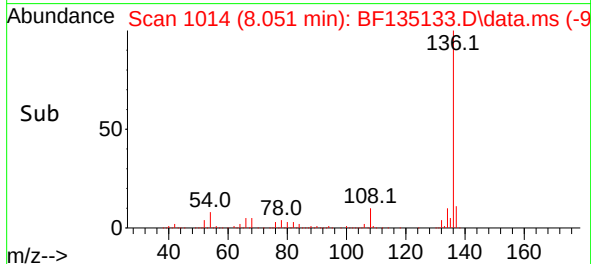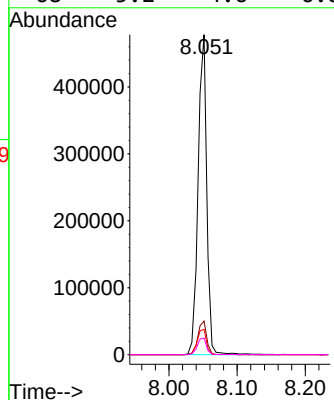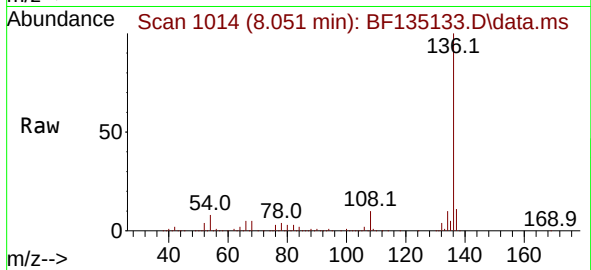

#23
Nitrobenzene-d5
Concen: 51.075 ng
RT: 7.334 min Scan# 892
Delta R.T. -0.012 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26

Tgt Ion: 82 Resp: 384046
Ion Ratio Lower Upper
82 100
128 45.6 37.8 56.8
54 55.9 45.0 67.6


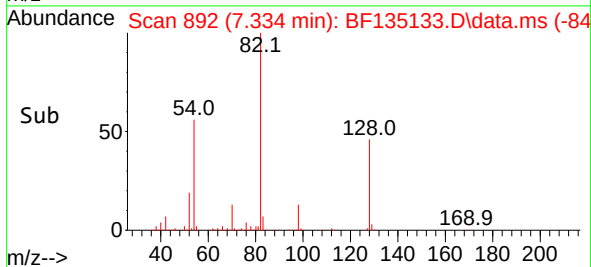
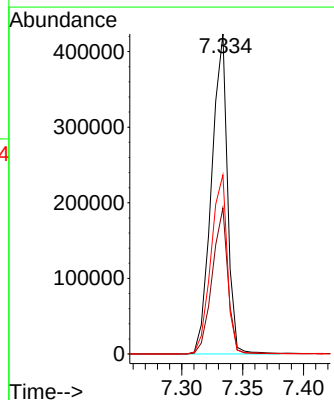
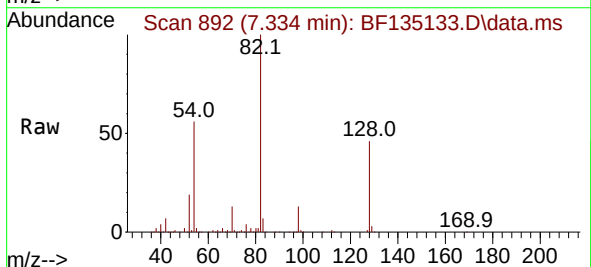


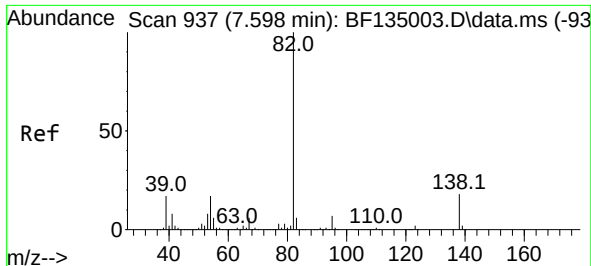

#25
Isophorone
Concen: 26.938 ng
RT: 7.334 min Scan# 892
Delta R.T. -0.265 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26




Instrument :
BNA_F
ClientSampleId :
SB-3


Tgt Ion: 82 Resp: 384040
Ion Ratio Lower Upper
82 100
95 0.0 5.6 8.4#
138 0.0 14.7 22.1#

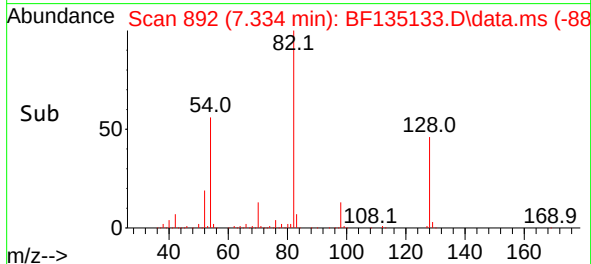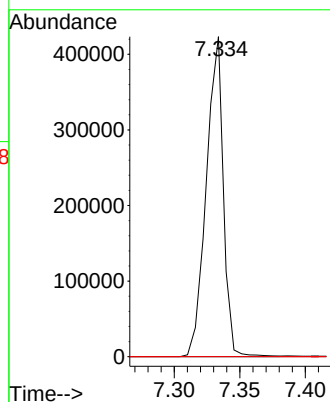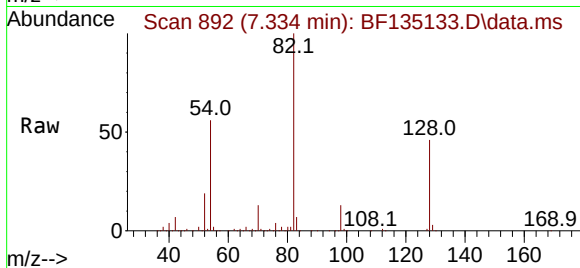

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.810 min Scan# 1313
Delta R.T. -0.006 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26

Tgt Ion:164 Resp: 213552
Ion Ratio Lower Upper
164 100
162 101.3 79.5 119.3
160 45.9 36.0 54.0


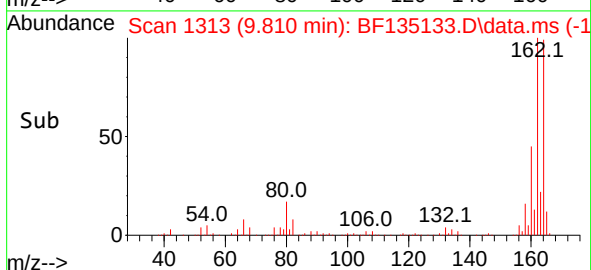
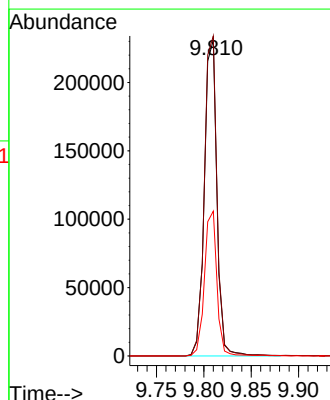
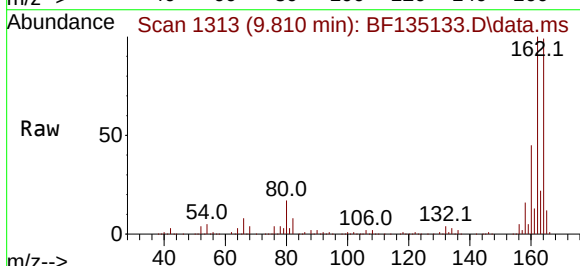


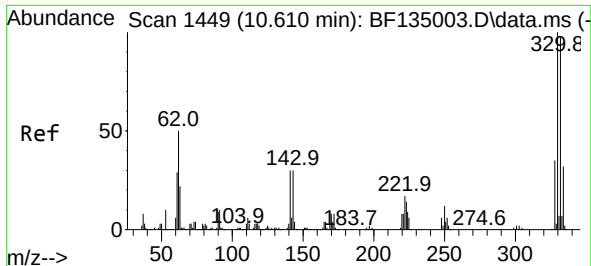

#42
 2,4,6-Tribromophenol
 Concen: 71.601 ng
 RT: 10.598 min Scan# 1447
 Delta R.T. -0.012 min
 Lab File: BF135133.D
 Acq: 07 Sep 2023 14:26




Instrument :
 BNA_F
 ClientSampleId :
 SB-3


Tgt Ion:330 Resp: 162200
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.6 116.4
 141 32.9 26.3 39.5

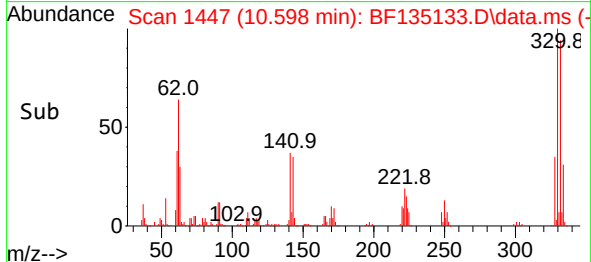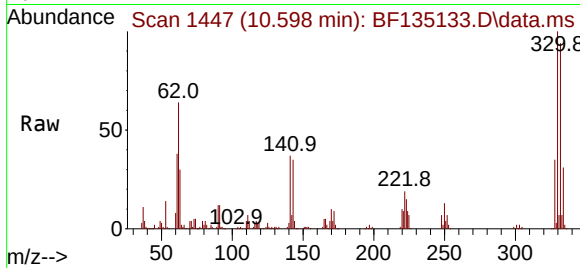

#45
 2-Fluorobiphenyl
 Concen: 53.694 ng
 RT: 9.128 min Scan# 1197
 Delta R.T. -0.012 min
 Lab File: BF135133.D
 Acq: 07 Sep 2023 14:26

Tgt Ion:172 Resp: 704285
 Ion Ratio Lower Upper
 172 100
 171 35.1 28.2 42.2
 170 23.5 19.0 28.4


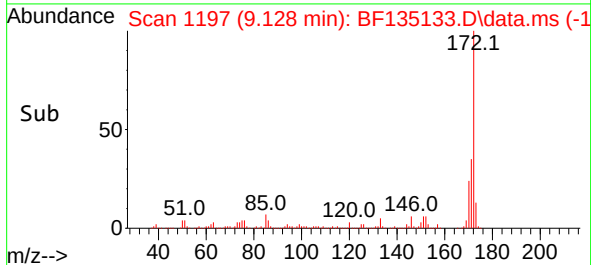

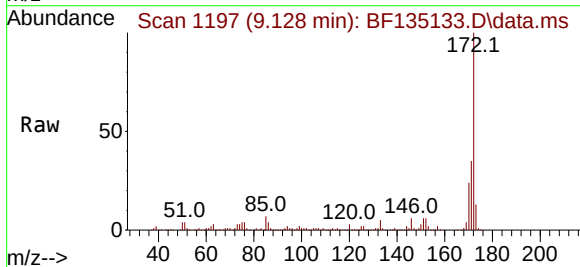


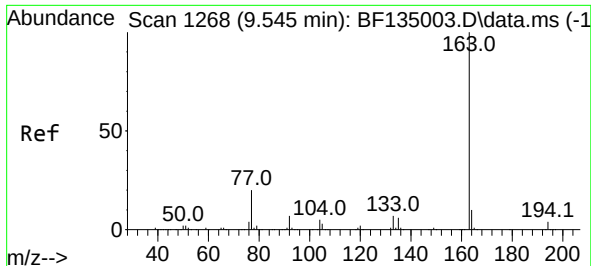

#50
Dimethylphthalate
Concen: 2.895 ng
RT: 9.810 min Scan# 11
Delta R.T. 0.265 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26




Instrument :
BNA_F
ClientSampleId :
SB-3


Tgt Ion:163 Resp: 43296
Ion Ratio Lower Upper
163 100
194 0.0 3.0 4.6#
164 459.1 8.1 12.1#

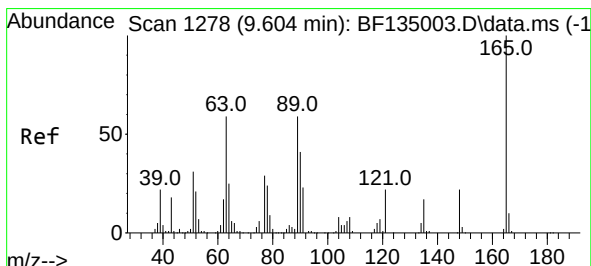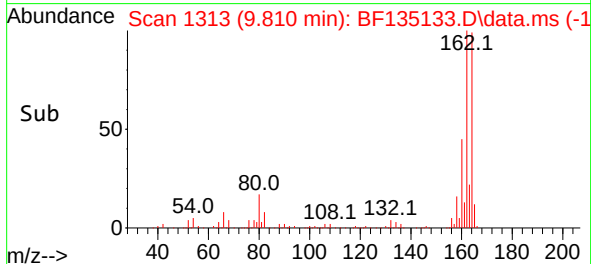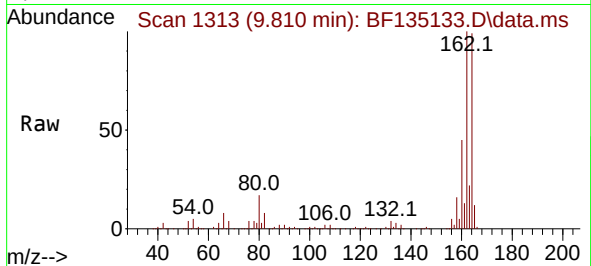

#51
2,6-Dinitrotoluene
Concen: 8.359 ng
RT: 9.810 min Scan# 1313
Delta R.T. 0.206 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26

Tgt Ion:165 Resp: 27427
Ion Ratio Lower Upper
165 100
63 2.0 50.4 75.6#
89 1.4 47.1 70.7#


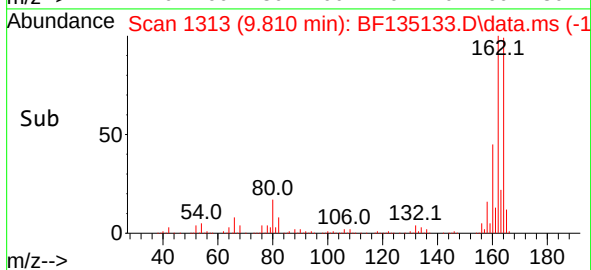

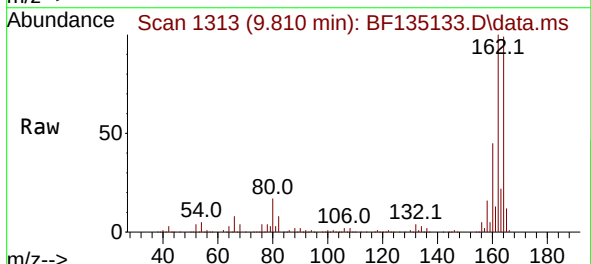


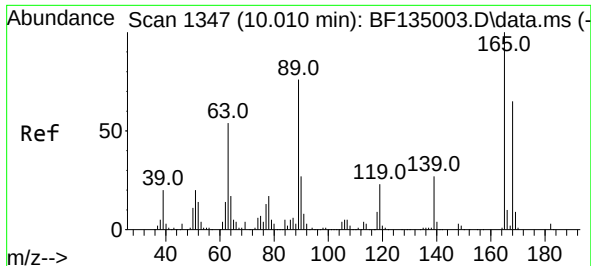

#57
2,4-Dinitrotoluene
Concen: 6.708 ng
RT: 9.810 min Scan# 11
Delta R.T. -0.200 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26




Instrument :
BNA_F
ClientSampleId :
SB-3


Tgt Ion:165 Resp: 27427
Ion Ratio Lower Upper
165 100
63 2.0 43.2 64.8#
89 1.4 60.8 91.2#
182 0.0 2.0 3.0#

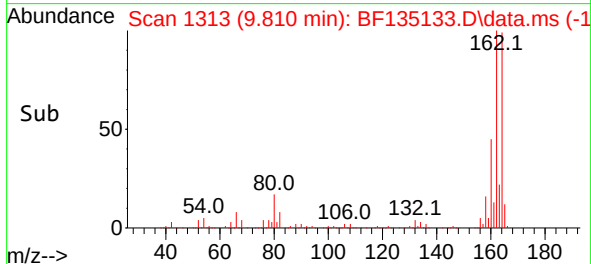

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.298 min Scan# 1566
Delta R.T. -0.012 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26

Tgt Ion:188 Resp: 369525
Ion Ratio Lower Upper
188 100
94 9.6 7.0 10.4
80 11.0 7.4 11.2


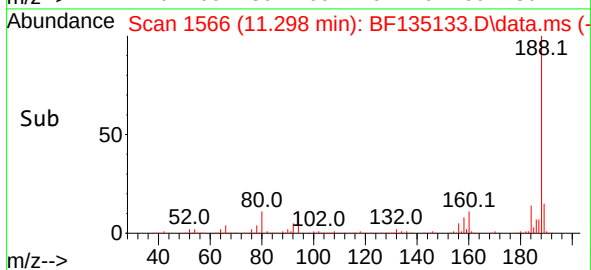

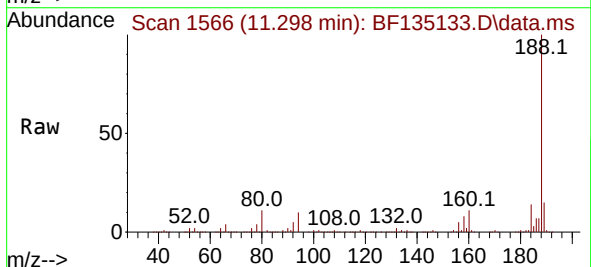


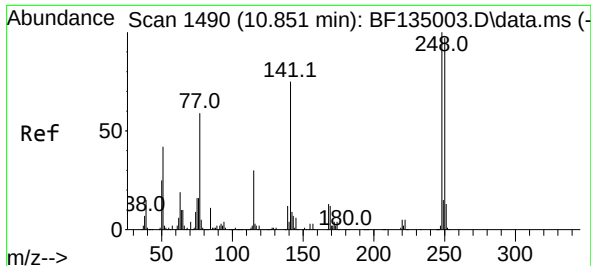

#67
4-Bromophenyl-phenylether
Concen: 2.701 ng
RT: 10.598 min Scan# 1490
Delta R.T. -0.253 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26




Instrument :
BNA_F
ClientSampleId :
SB-3


Tgt Ion:248 Resp: 10586
Ion Ratio Lower Upper
248 100
250 183.3 77.9 116.9#
141 508.4 59.8 89.8#

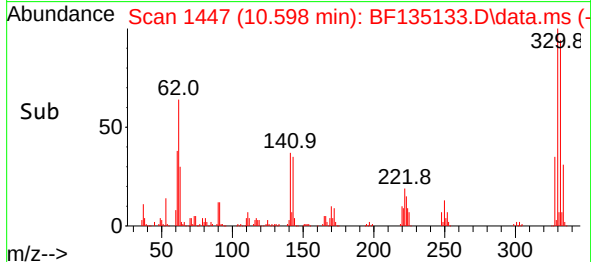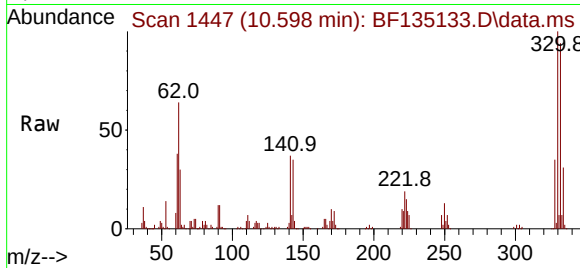

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.957 min Scan# 2018
Delta R.T. -0.006 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26

Tgt Ion:240 Resp: 189758
Ion Ratio Lower Upper
240 100
120 10.4 10.2 15.2
236 25.6 21.3 31.9


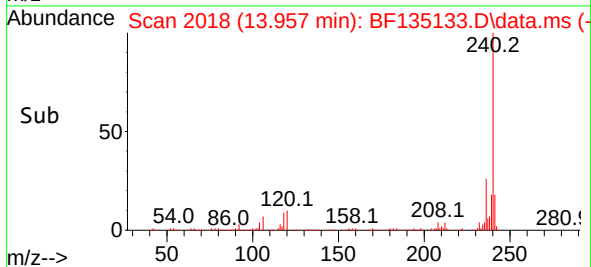

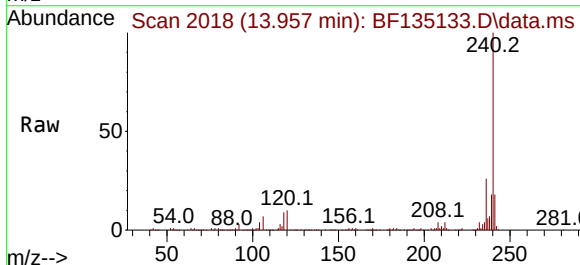




#77
Benzidine
Concen: 2.468 ng
RT: 12.898 min Scan# 1838
Delta R.T. 0.247 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26




Instrument :
BNA_F
ClientSampleId :
SB-3


Tgt Ion:184 Resp: 8441
Ion Ratio Lower Upper
184 100
185 15.4 12.0 18.0
183 6.8 9.0 13.6#

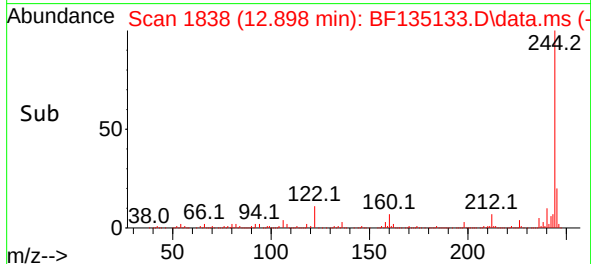

#79
Terphenyl-d14
Concen: 54.771 ng
RT: 12.898 min Scan# 1838
Delta R.T. -0.006 min
Lab File: BF135133.D
Acq: 07 Sep 2023 14:26

Tgt Ion:244 Resp: 636883
Ion Ratio Lower Upper
244 100
212 6.9 5.6 8.4
122 11.1 9.8 14.6

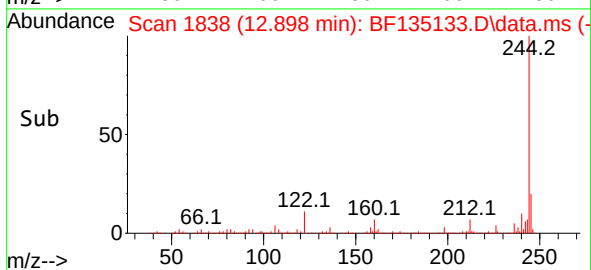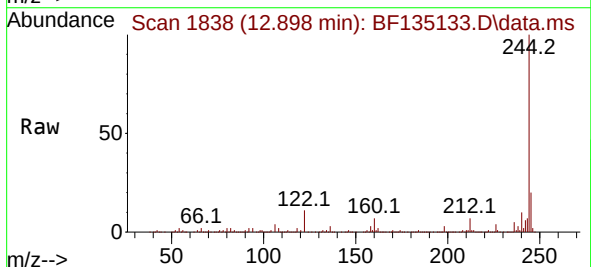

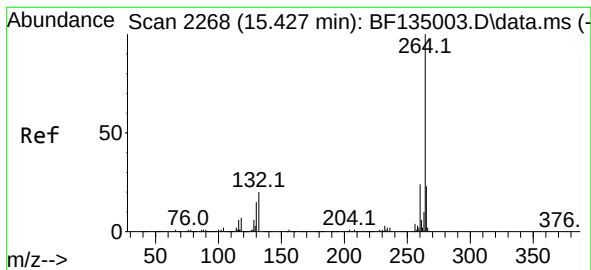

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.427 min Scan# 21

Delta R.T. 0.000 min

Lab File: BF135133.D


Acq: 07 Sep 2023 14:26

Instrument :

BNA_F

ClientSampleId :

SB-3

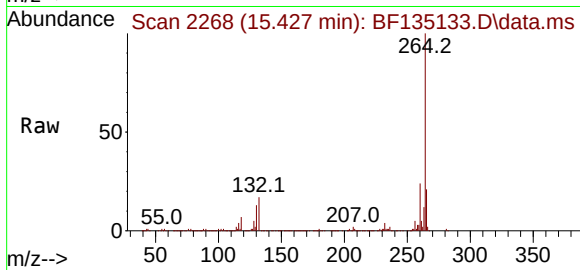

Tgt Ion:264 Resp: 208239

Ion Ratio Lower Upper

264 100

260 23.8 19.0 28.6

265 20.8 18.2 27.2

