


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090723\
Data File : BF135125.D
Acq On : 07 Sep 2023 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 31 03:48:08 2023

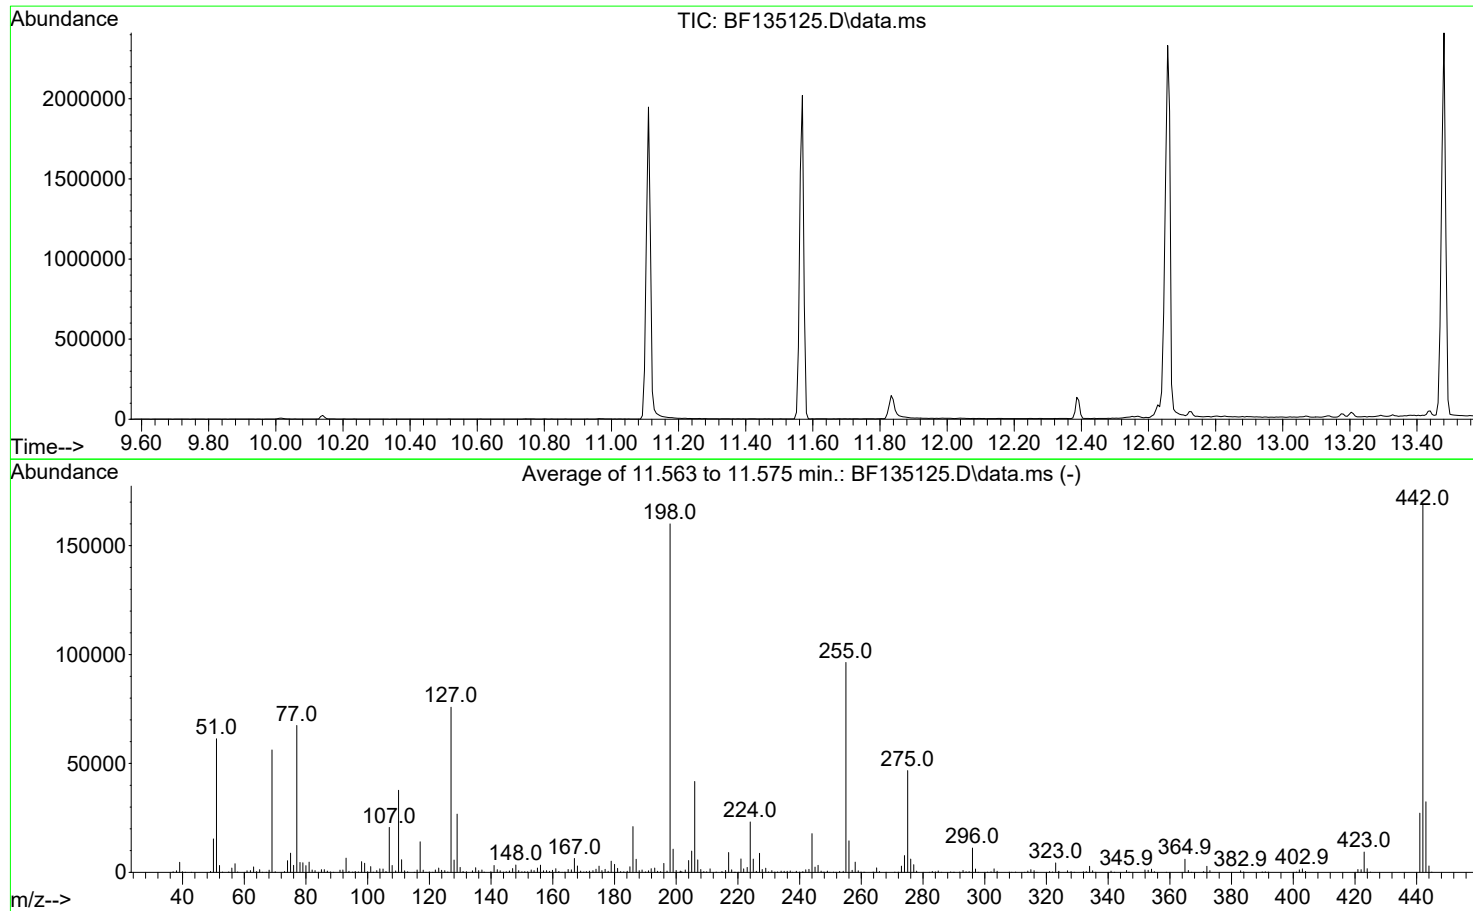




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	61362	PASS
68	69	0.00	2	1.8	1018	PASS
69	198	0.00	100	35.1	56213	PASS
70	69	0.00	2	0.5	308	PASS
127	198	10	80	47.4	75835	PASS
197	198	0.00	2	0.4	562	PASS
198	198	100	100	100.0	160024	PASS
199	198	5	9	6.7	10655	PASS
275	198	10	60	29.2	46731	PASS
365	198	1	100	3.8	6038	PASS
441	198	0.01	100	17.0	27181	PASS
442	442	50	100	100.0	168907	PASS
443	442	15	24	19.2	32419	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090723\
Data File : BF135125.D
Acq On : 07 Sep 2023 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 07 10:54:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

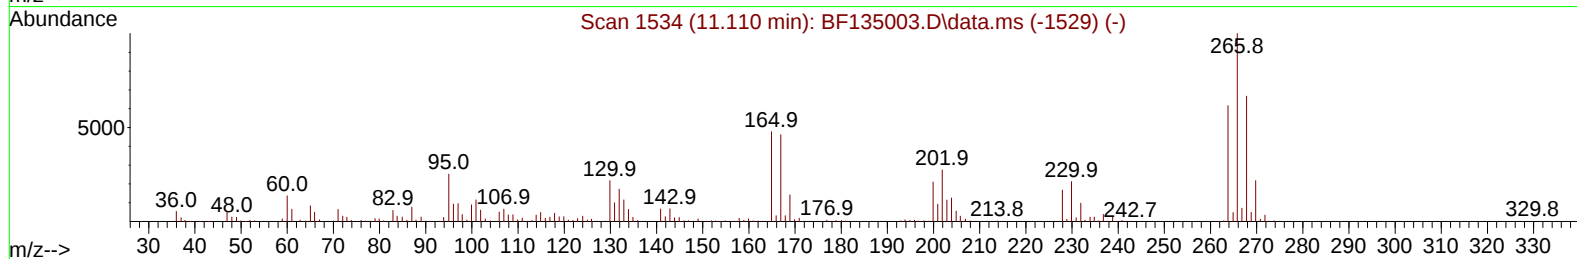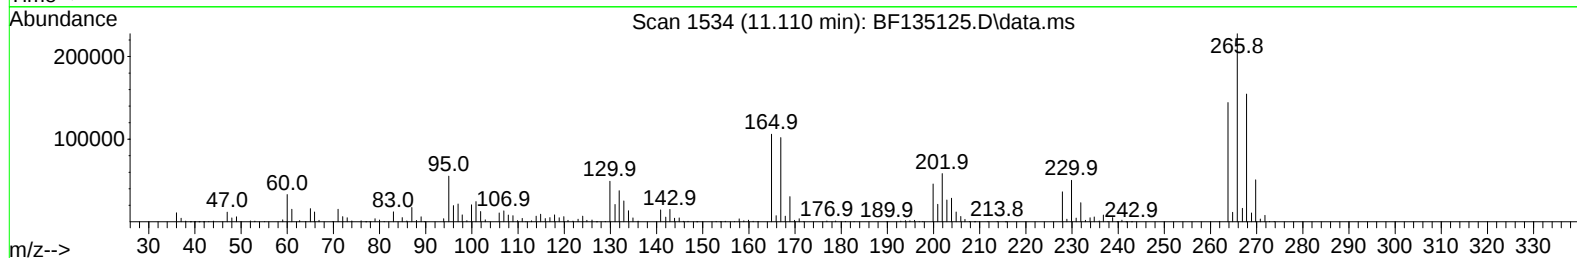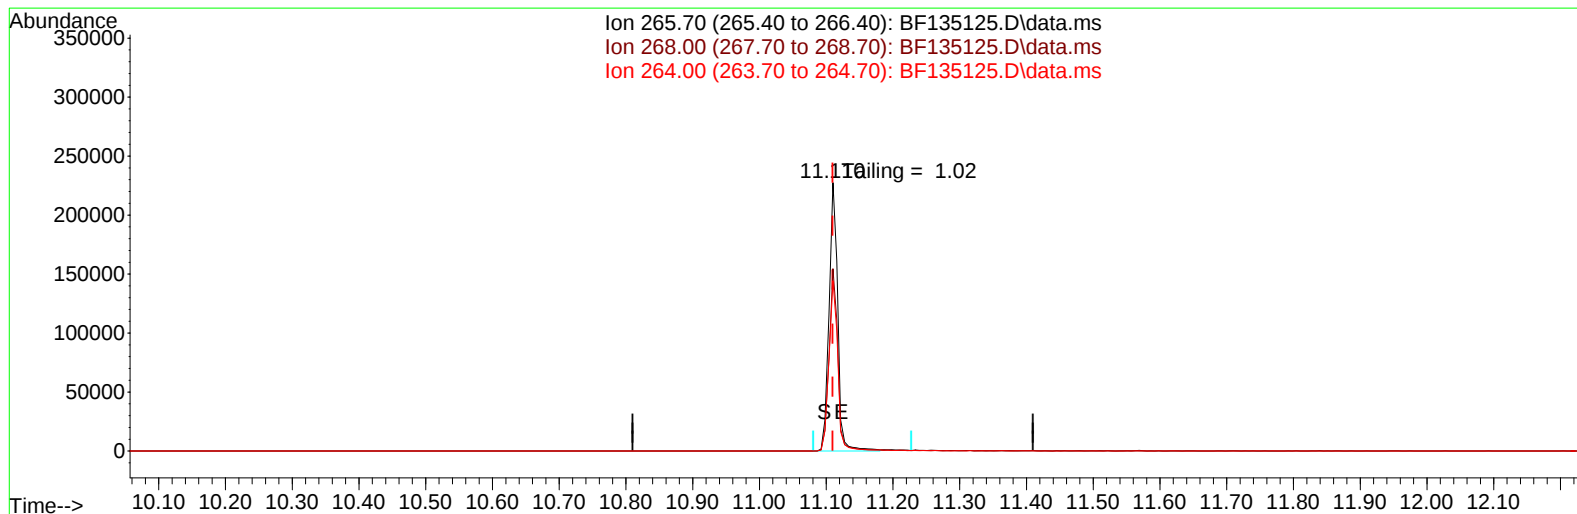

TIC: BF135125.D\data.ms

(70) Pentachlorophenol (C)

11.110min (+ 0.000) 32307.53 ng m

response 206862

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	67.93
264.00	61.60	63.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/7/2023	BNA_F	<u>BF135125.D</u>
Compound Name	Response	Retention Time
DDT	417119	13.48
DDD	8557	13.204
DDE	210	12.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8767	425886	2.06

Instrument :
BNA_F
ClientSampleId :
DFTPP