


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090823\
 Data File : BF135147.D
 Acq On : 08 Sep 2023 14:46
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 09 03:05:29 2023

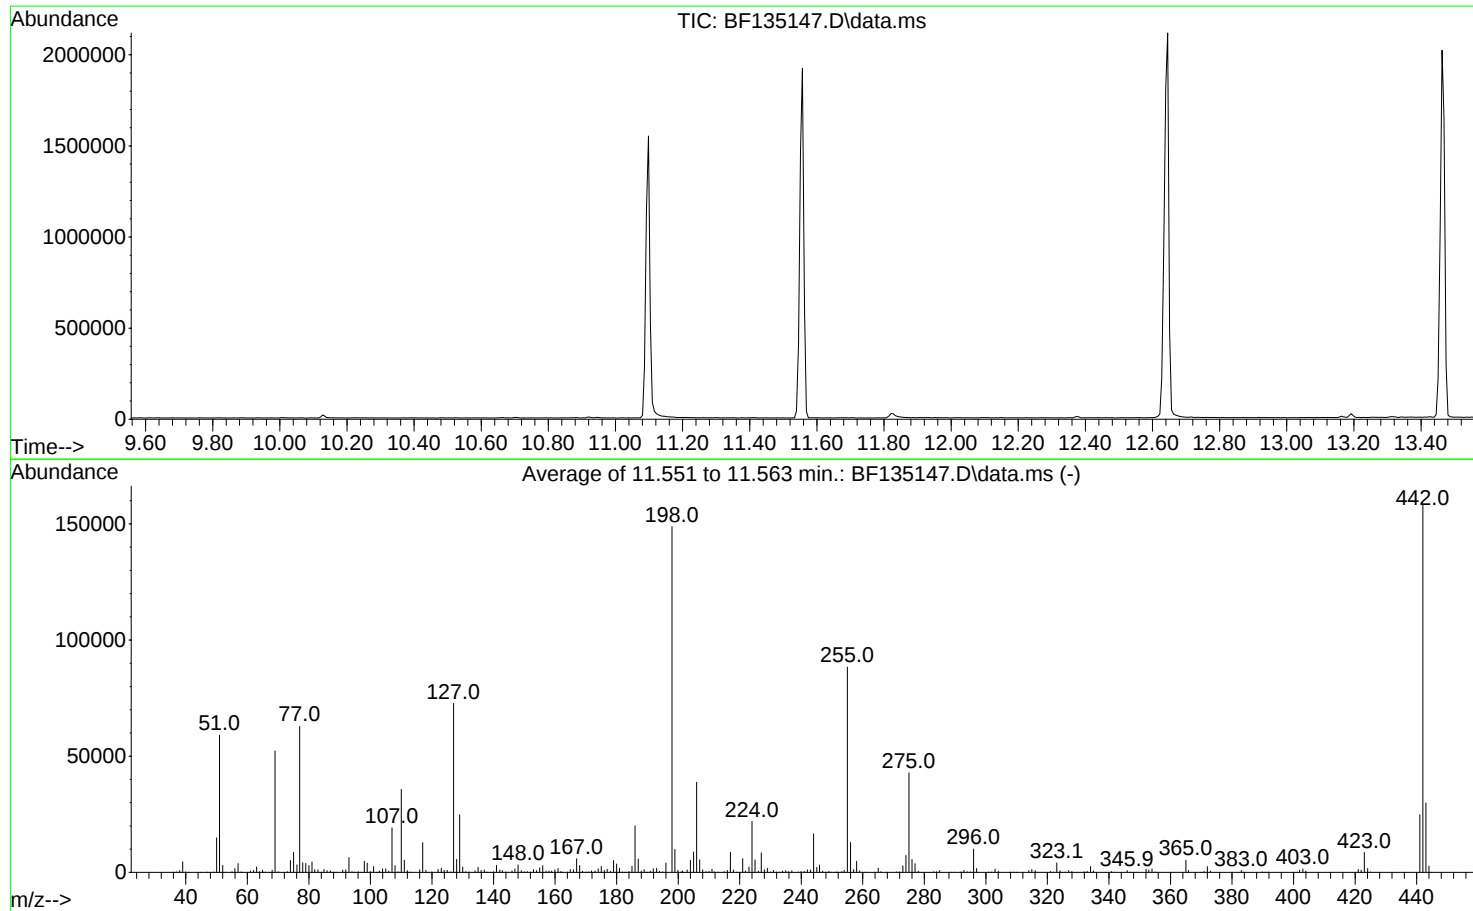




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	59026	PASS
68	69	0.00	2	1.9	975	PASS
69	198	0.00	100	35.1	52291	PASS
70	69	0.00	2	0.5	276	PASS
127	198	10	80	48.8	72717	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	148864	PASS
199	198	5	9	6.6	9884	PASS
275	198	10	60	28.8	42816	PASS
365	198	1	100	3.5	5270	PASS
441	198	0.01	100	16.7	24797	PASS
442	442	50	100	100.0	158355	PASS
443	442	15	24	18.9	29899	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090823\
Data File : BF135146.D
Acq On : 08 Sep 2023 14:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 08 17:01:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 02:45:19 2023
Response via : Initial Calibration

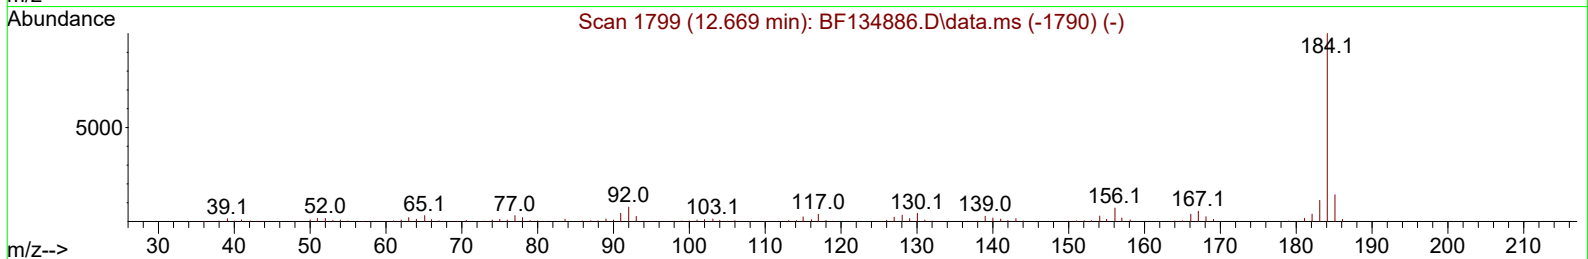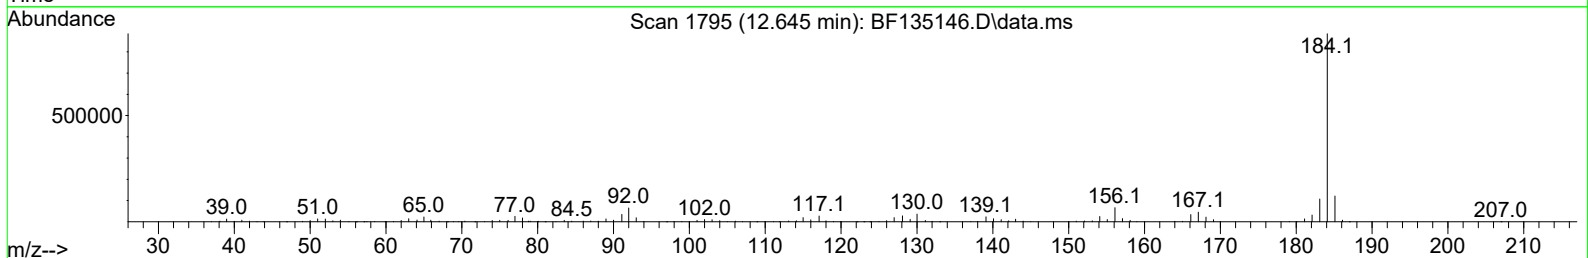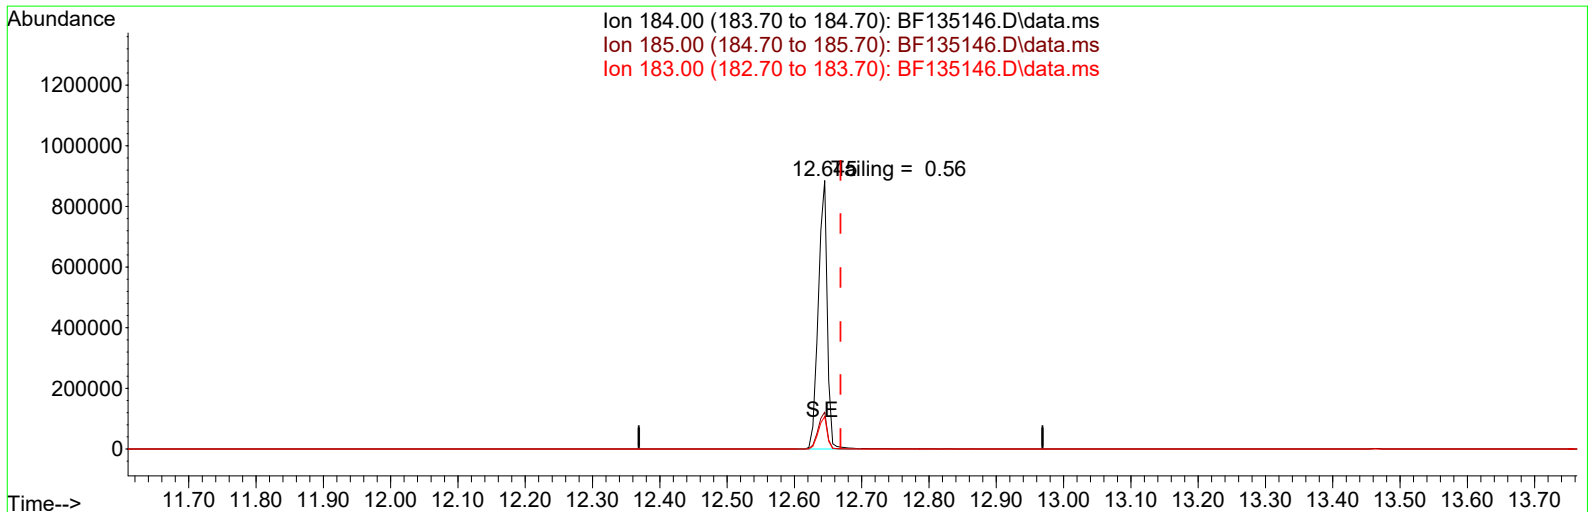

TIC: BF135146.D\data.ms

(77) Benzidine

12.645min (-0.024) 0.00 ng




response 820129

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.76
183.00	11.20	12.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090823\
Data File : BF135146.D
Acq On : 08 Sep 2023 14:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 08 17:01:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 02:45:19 2023
Response via : Initial Calibration

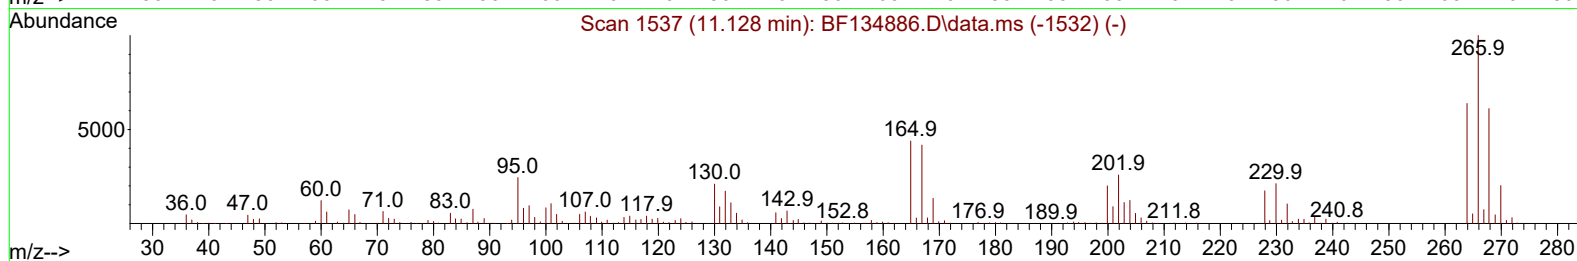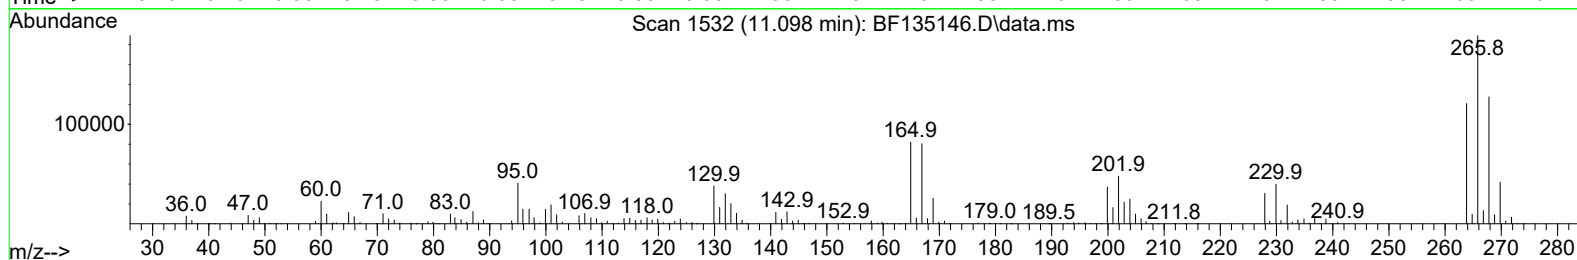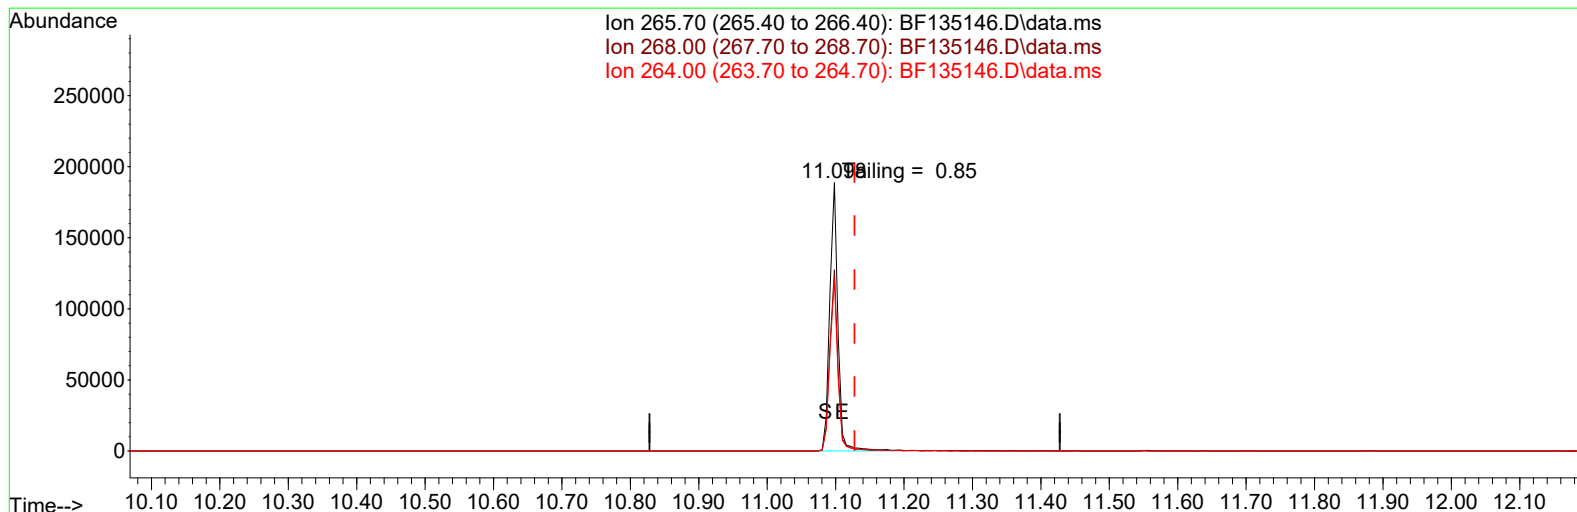

TIC: BF135146.D\data.ms

(70) Pentachlorophenol (C)

11.098min (-0.030) 345097.18 ng

response 155444

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.50
264.00	63.80	63.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/8/2023	BNA_F	<u>BF135147.D</u>
Compound Name	Response	Retention Time
DDT	367473	13.463
DDD	5220	13.192
DDE	58	12.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5278	372751	1.42

Instrument :
BNA_F
ClientSampleId :
DFTPP