
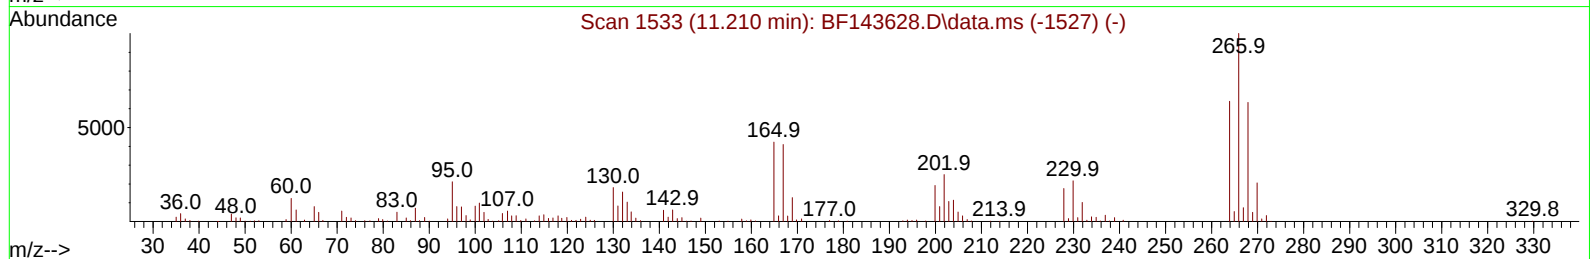
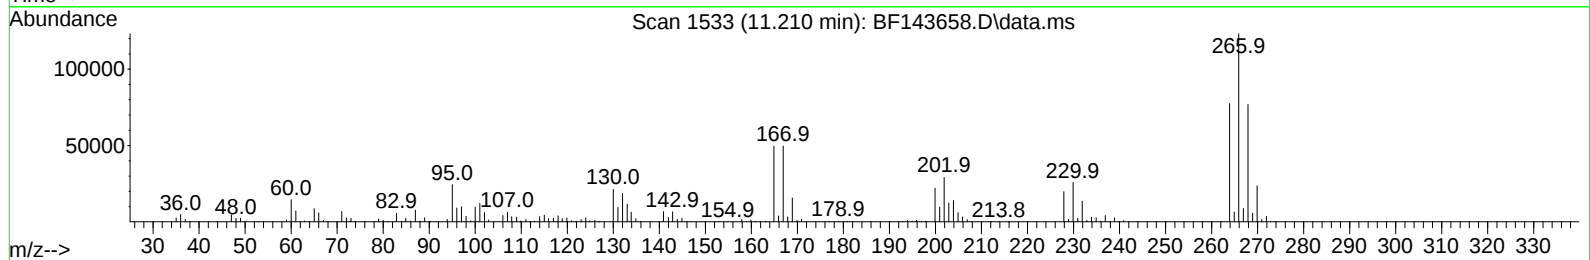


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090825\
Data File : BF143658.D
Acq On : 08 Sep 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 11:46:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 03 18:35:49 2025
Response via : Initial Calibration

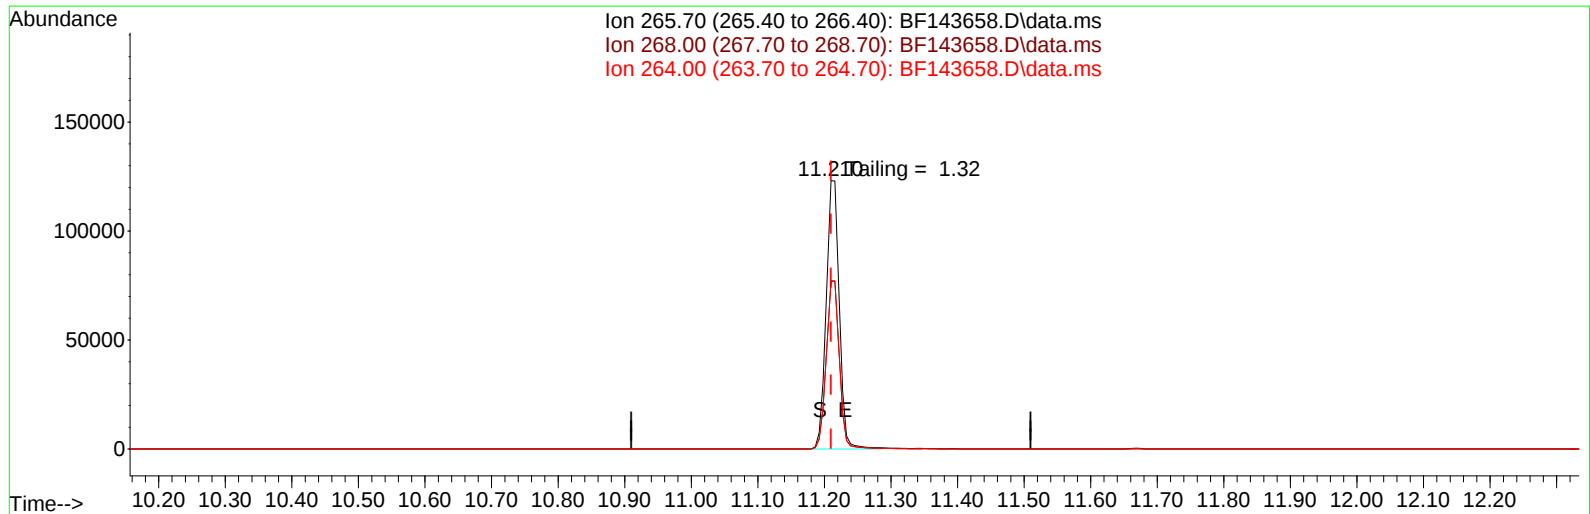

TIC: BF143658.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 67614.04 ng

response 169815

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.45
264.00	64.00	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090825\
Data File : BF143658.D
Acq On : 08 Sep 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 11:46:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 03 18:35:49 2025
Response via : Initial Calibration

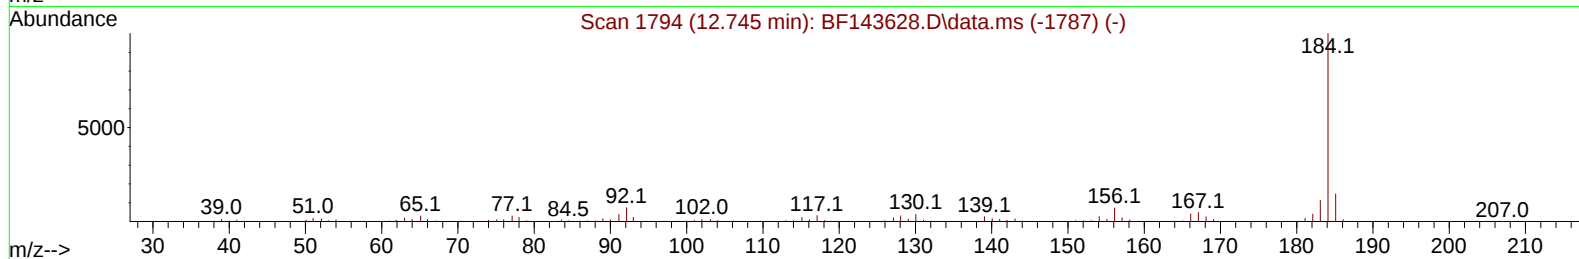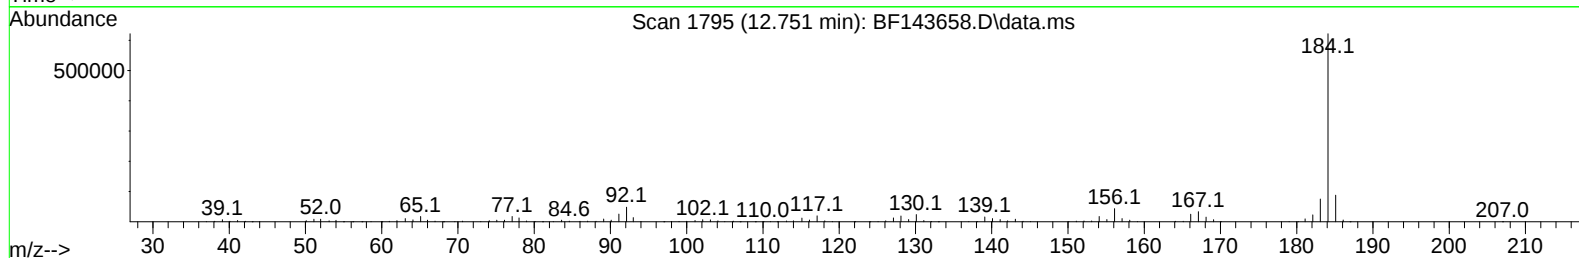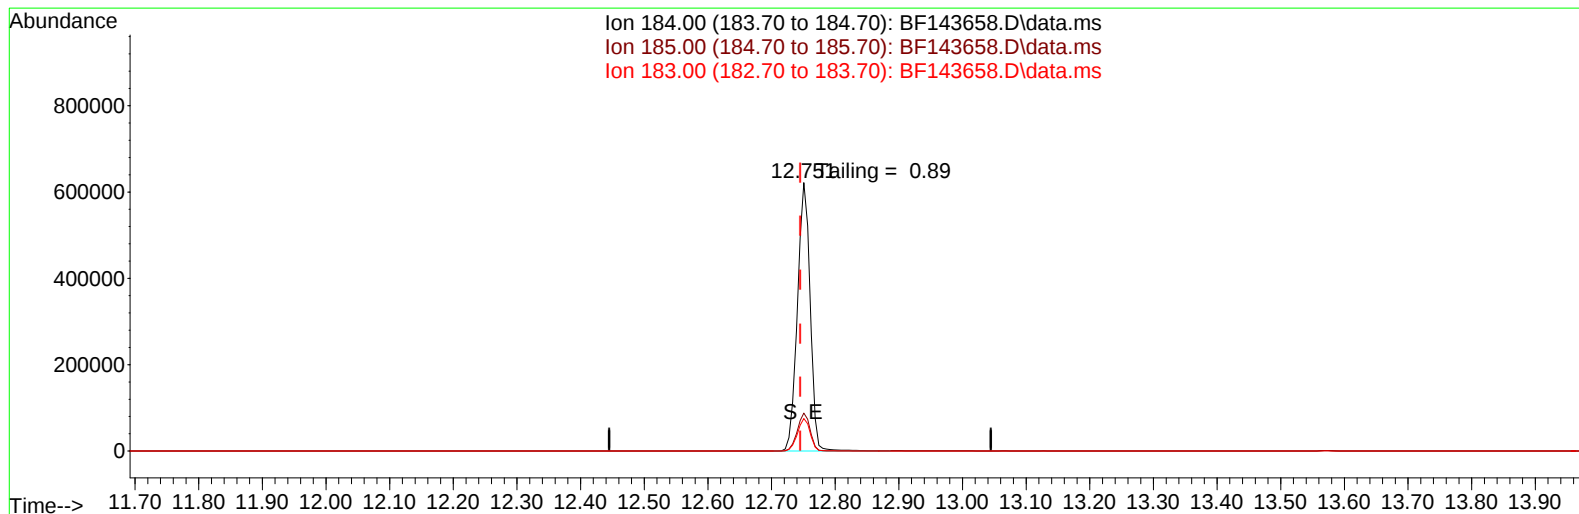

TIC: BF143658.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 16121.87 ng

response 871595

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.17
183.00	11.30	12.12
0.00	0.00	0.00