
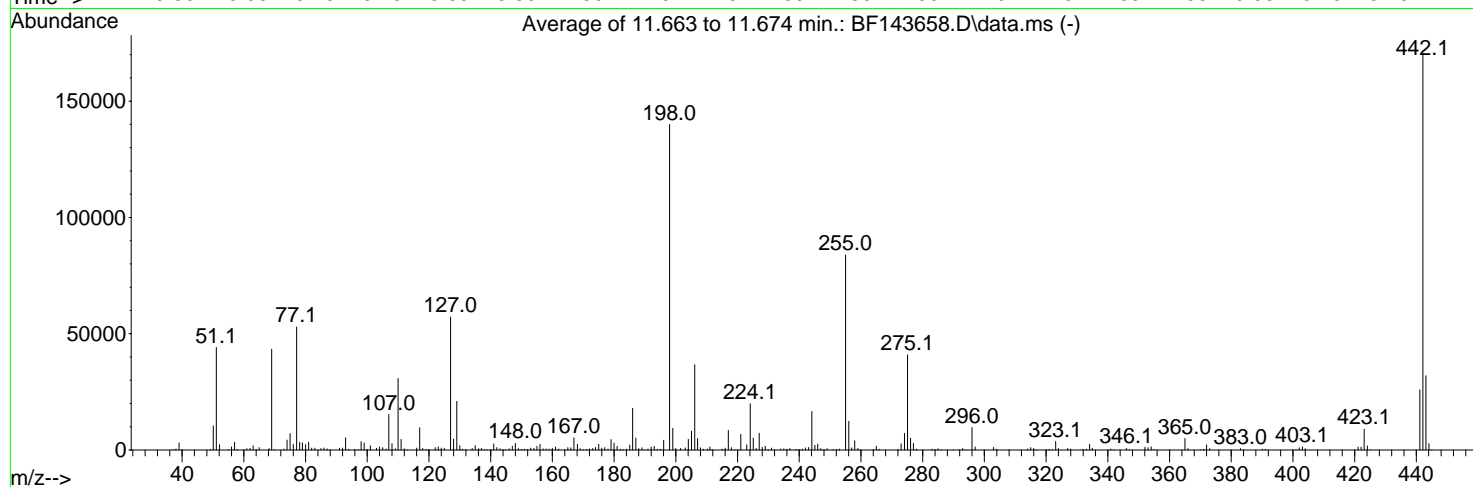


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090825\
 Data File : BF143658.D
 Acq On : 08 Sep 2025 08:53
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 03 18:35:49 2025

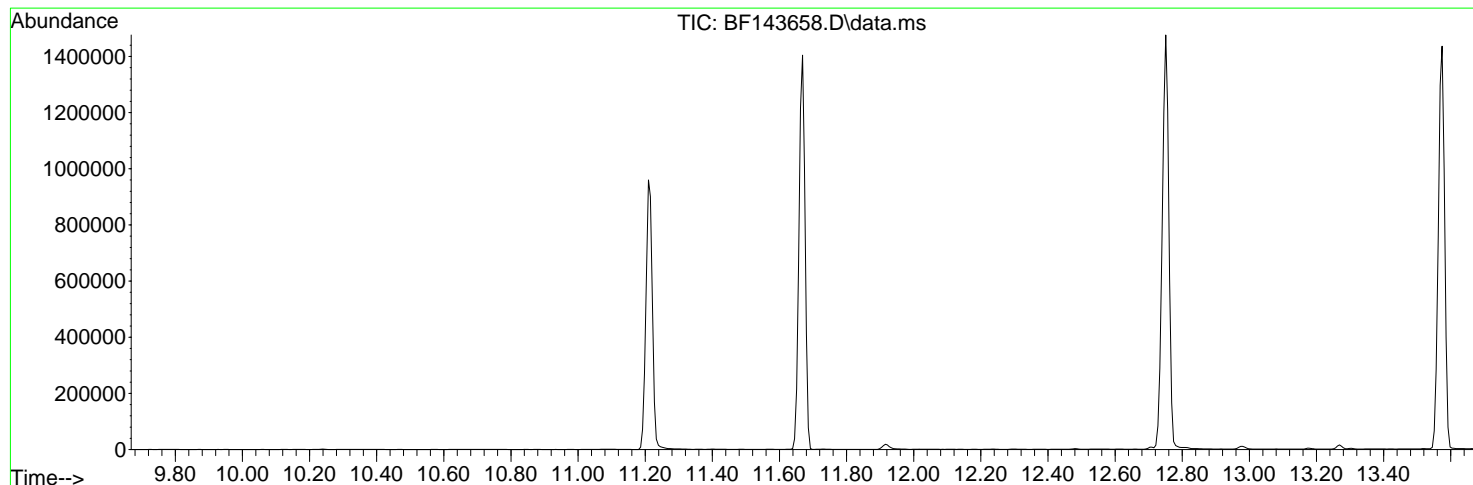




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.4	593	PASS
69	69	100	100	100.0	43368	PASS
70	69	0.00	2	0.4	159	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	139981	PASS
199	198	5	9	6.7	9337	PASS
365	198	1	100	3.6	4983	PASS
441	443	0.01	150	81.0	25851	PASS
442	442	100	100	100.0	169771	PASS
443	442	15	24	18.8	31933	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090825\
 Data File : BF143658.D
 Acq On : 08 Sep 2025 08:53
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 08 11:46:19 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 03 18:35:49 2025
 Response via : Initial Calibration

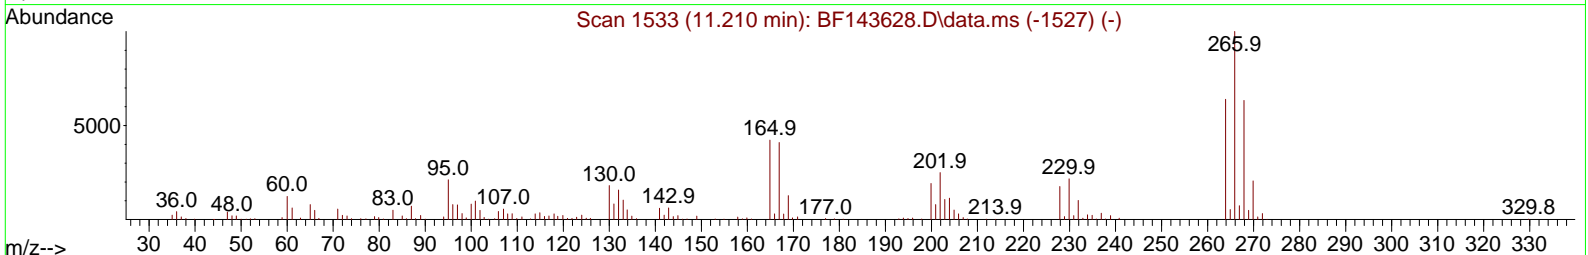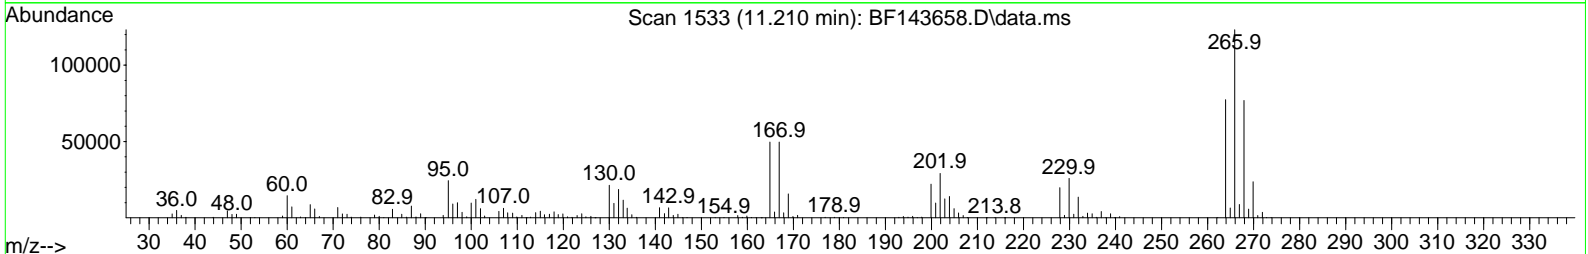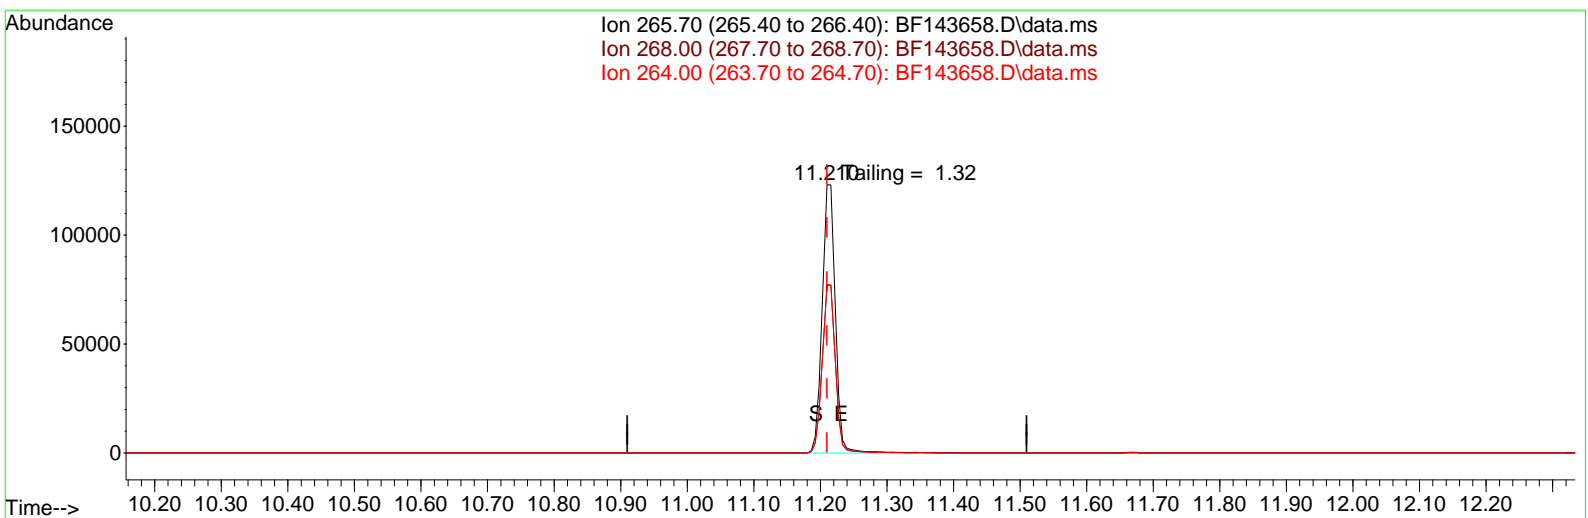

TIC: BF143658.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 67614.04 ng




response 169815

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.45
264.00	64.00	62.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090825\
 Data File : BF143658.D
 Acq On : 08 Sep 2025 08:53
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 08 11:46:19 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 03 18:35:49 2025
 Response via : Initial Calibration

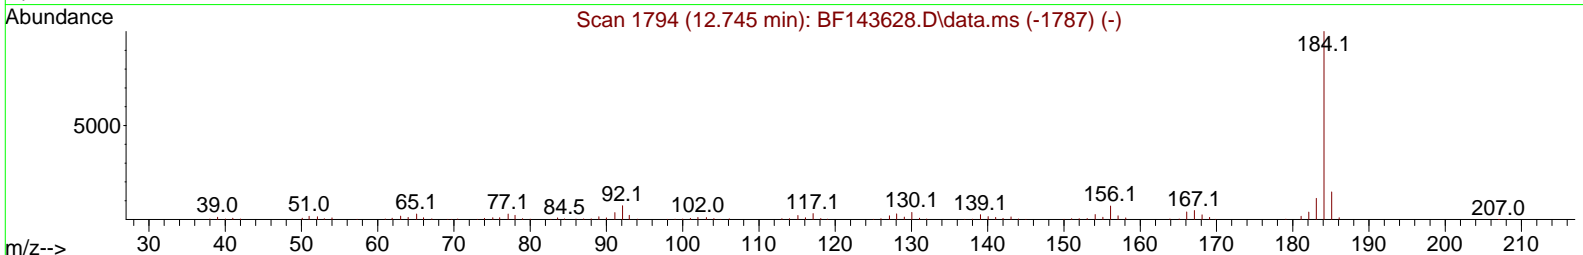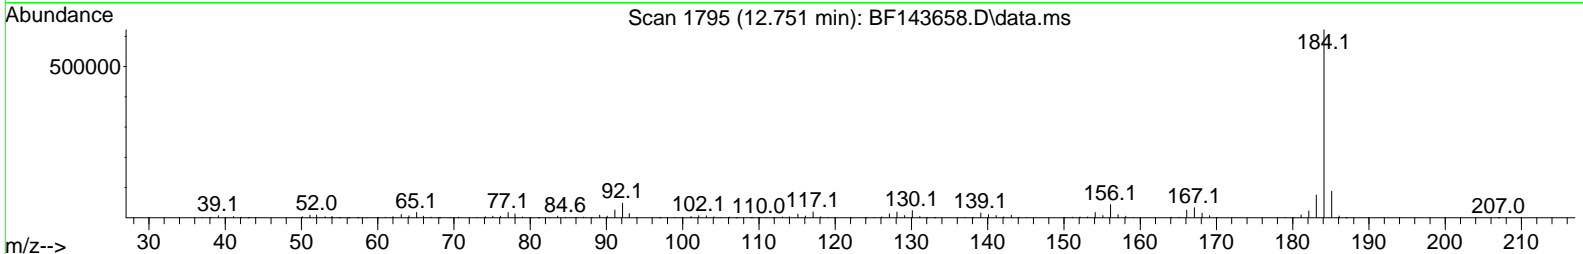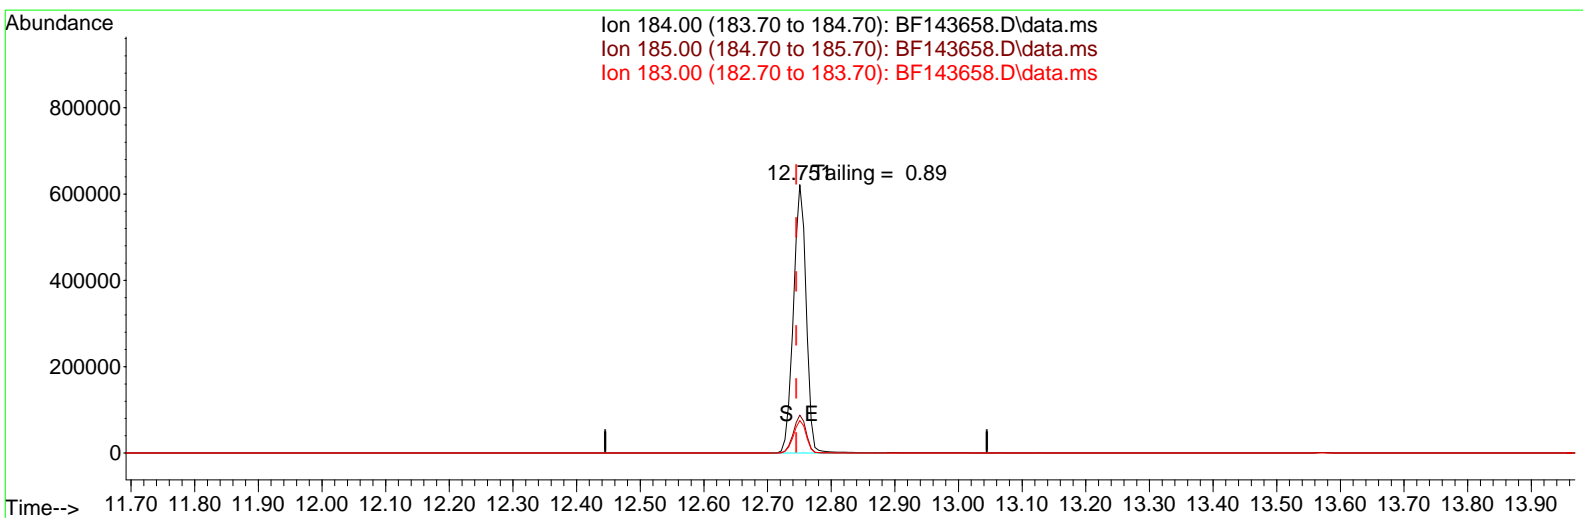

TIC: BF143658.D\data.ms

(77) Benzidine

12.751min (+ 0.006) 16121.87 ng

response 871595

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.17
183.00	11.30	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/9/2025	BNA_F	<u>BF1436458.D</u>
Compound Name	Response	Retention Time
DDT	360172	13.574
DDD	5234	13.268
DDE	60	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5294	365466	1.45

Instrument :
 BNA_F
 ClientSampled :
 DFTPP