


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090919\
 Data File : BF116894.D
 Acq On : 9 Sep 2019 13:52
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 20:02:30 2019

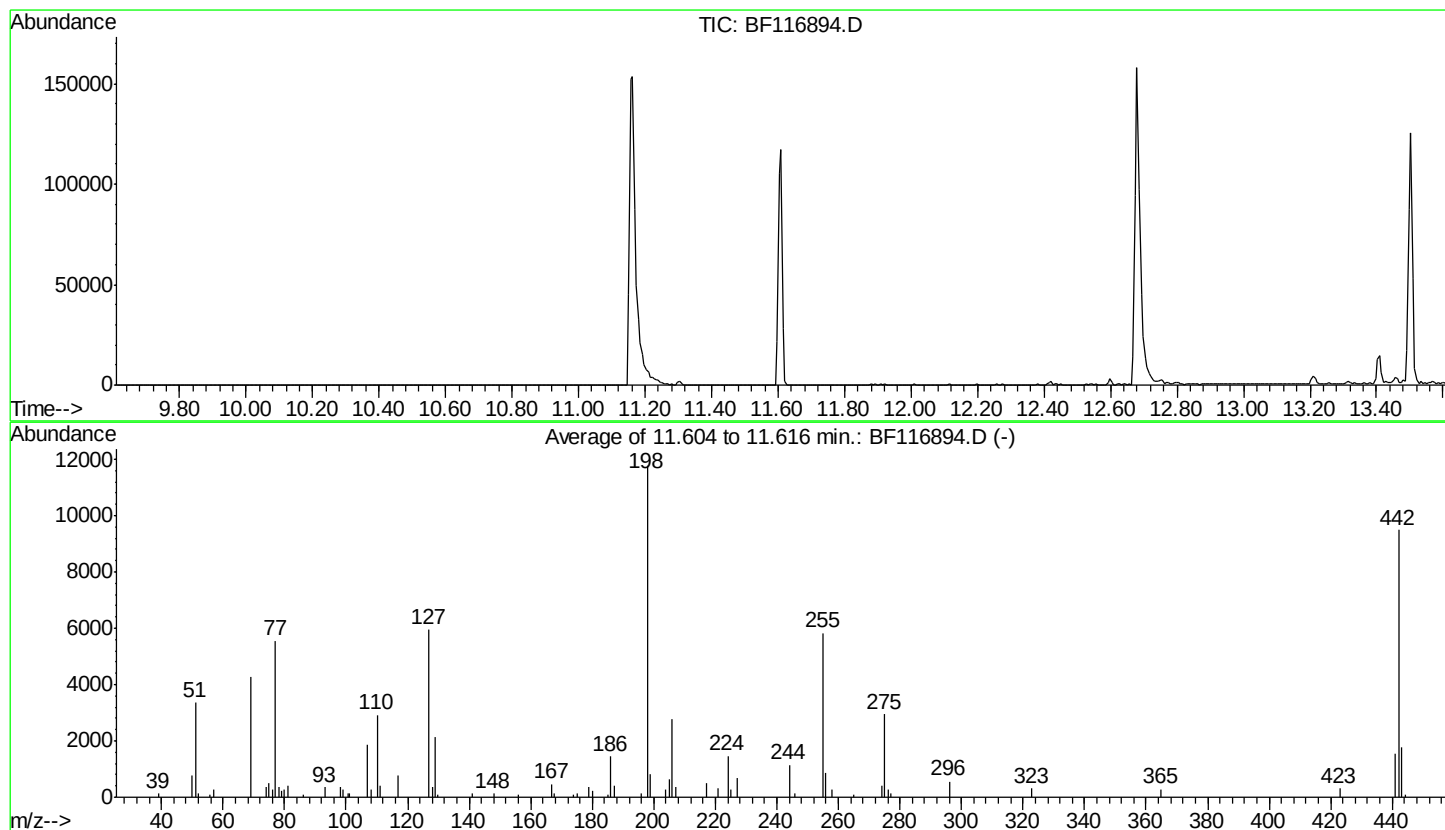

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	3357	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.3	4277	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	5949	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11776	PASS
199	198	5	9	6.8	806	PASS
275	198	10	60	25.0	2939	PASS
365	198	1	100	2.3	274	PASS
441	198	0.01	100	13.1	1537	PASS
442	198	50	100	80.5	9480	PASS
443	442	15	24	18.8	1786	PASS