
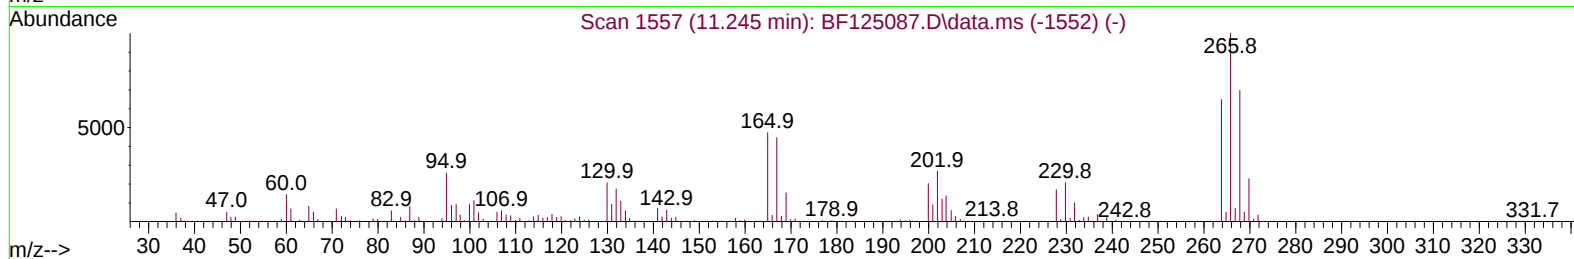
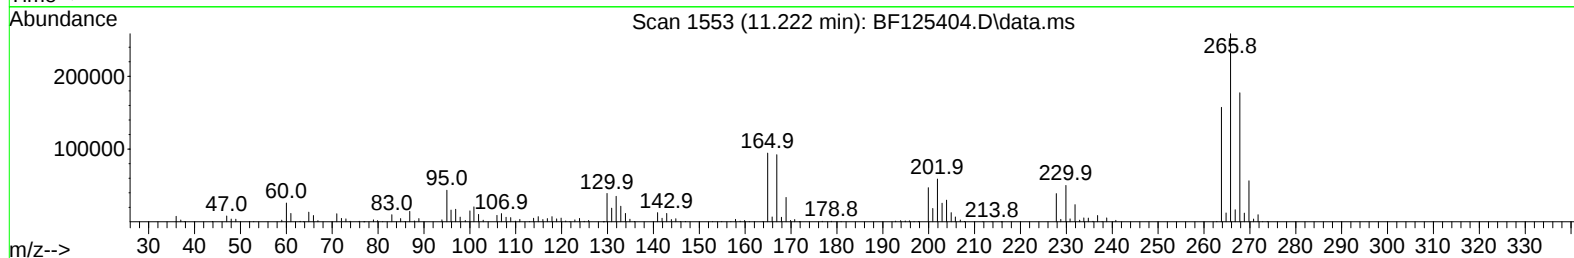


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090921\
Data File : BF125404.D
Acq On : 9 Sep 2021 9:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 11:44:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 08 14:14:01 2021
Response via : Initial Calibration

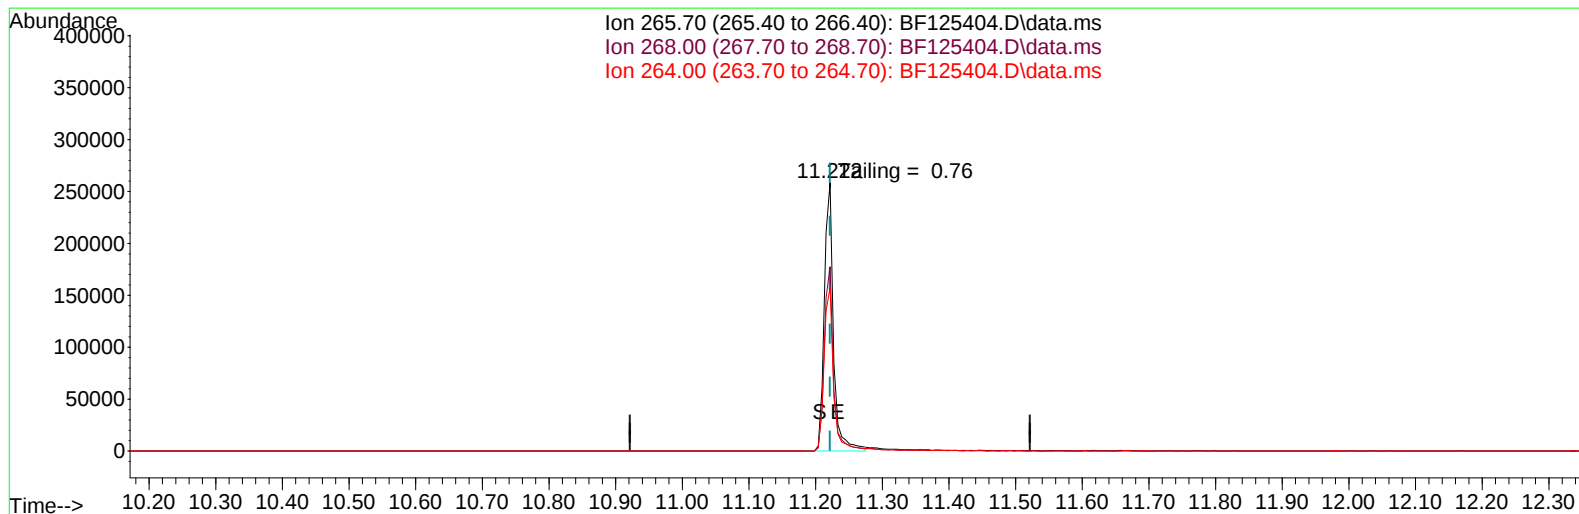

TIC: BF125404.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.000) 36835.53 ng

response 253740

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.61
264.00	69.90	60.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090921\
Data File : BF125404.D
Acq On : 9 Sep 2021 9:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 11:44:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 08 14:14:01 2021
Response via : Initial Calibration

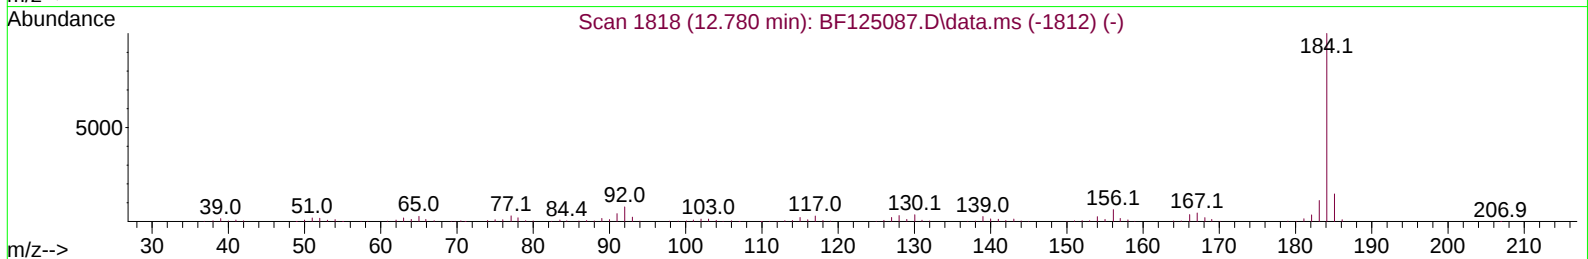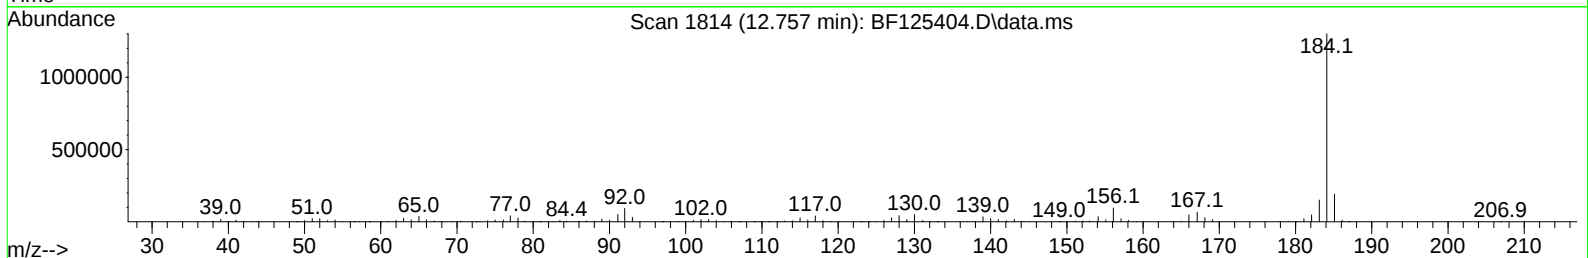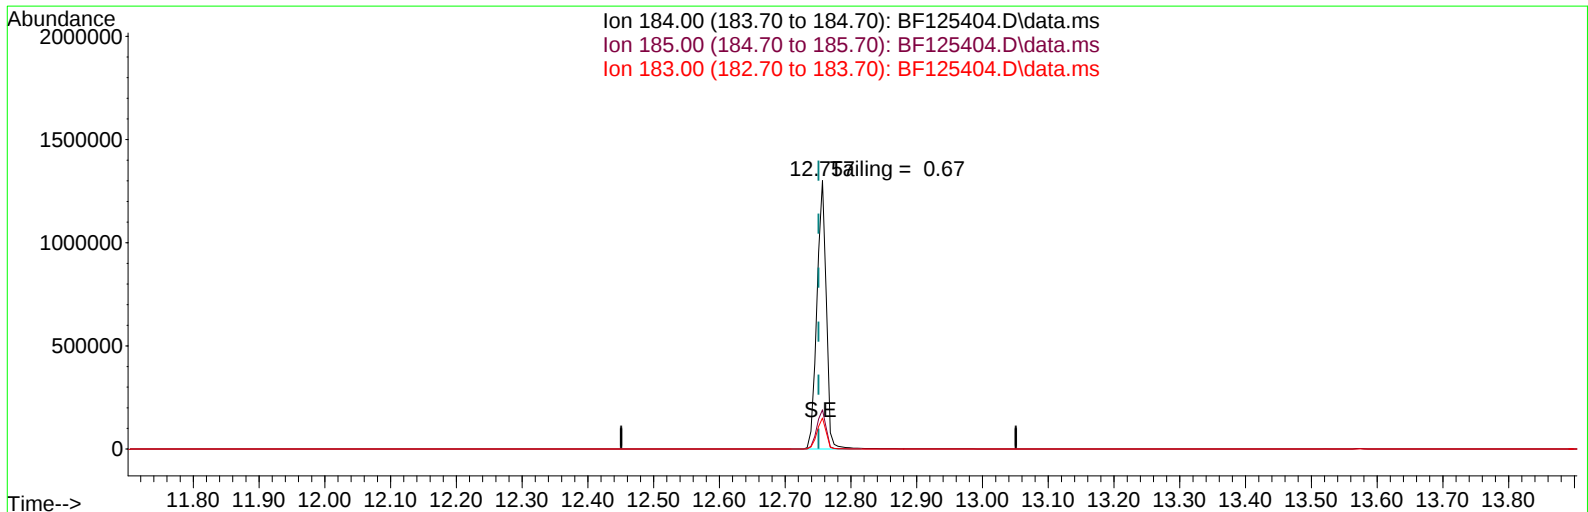

TIC: BF125404.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 1296291

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.63
183.00	10.10	11.57
0.00	0.00	0.00