
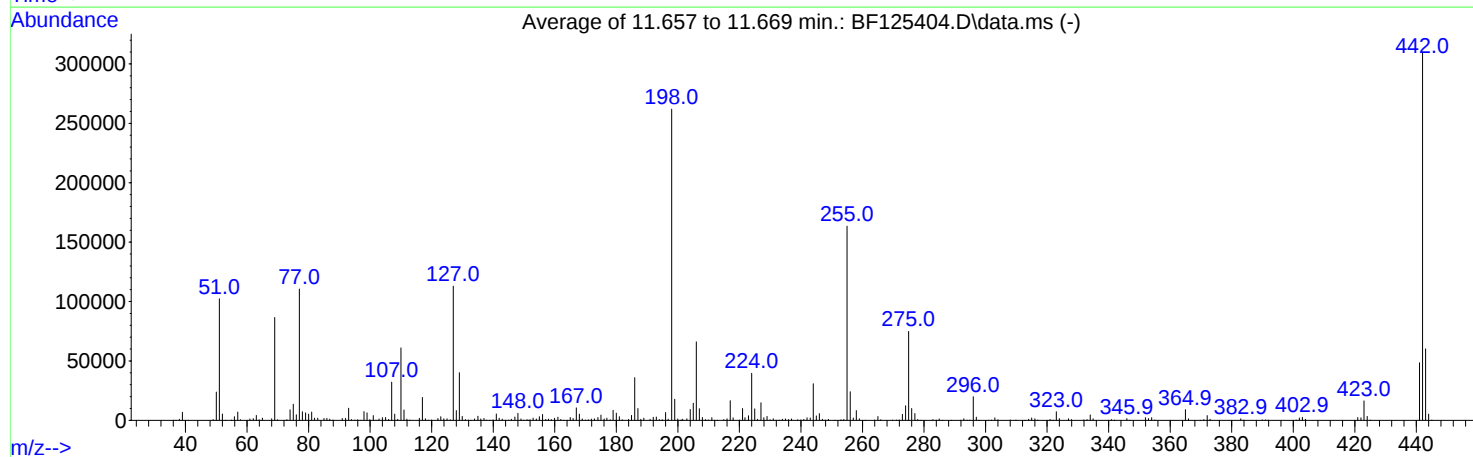


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090921\
 Data File : BF125404.D
 Acq On : 9 Sep 2021 9:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 08 14:14:01 2021

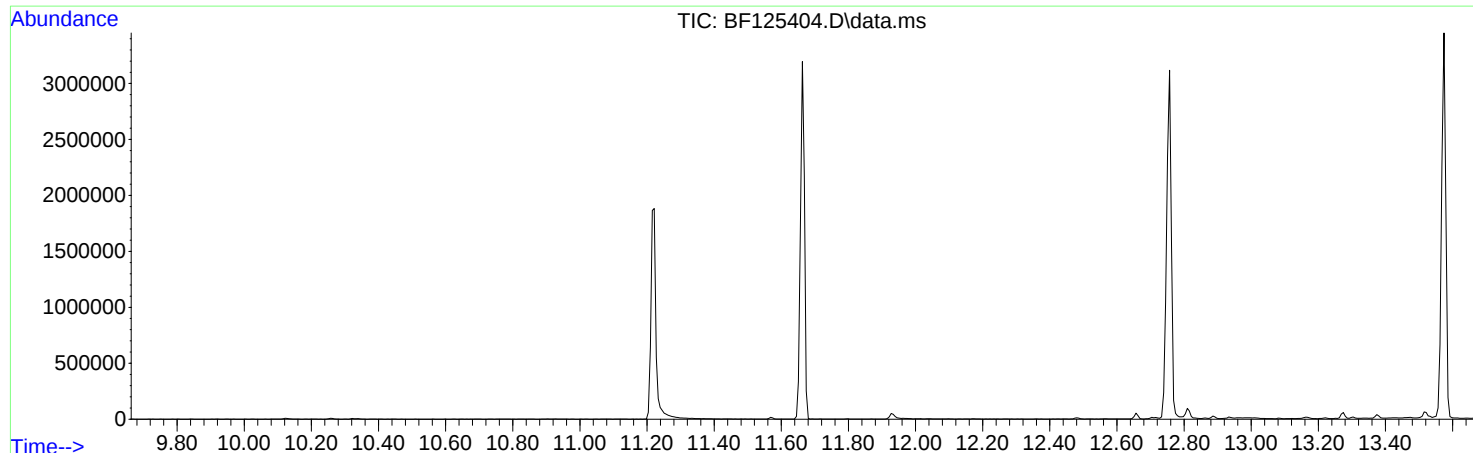




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	102421	PASS
68	69	0.00	2	1.6	1386	PASS
69	198	0.00	100	33.1	86629	PASS
70	69	0.00	2	0.6	547	PASS
127	198	10	80	43.1	112976	PASS
197	198	0.00	2	0.4	1118	PASS
198	198	100	100	100.0	261909	PASS
199	198	5	9	6.8	17839	PASS
275	198	10	60	28.6	74901	PASS
365	198	1	100	3.4	8979	PASS
441	198	0.01	100	18.5	48483	PASS
442	442	50	100	100.0	309619	PASS
443	442	15	24	19.4	60192	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090921\
 Data File : BF125404.D
 Acq On : 9 Sep 2021 9:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 09 11:44:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 08 14:14:01 2021
 Response via : Initial Calibration

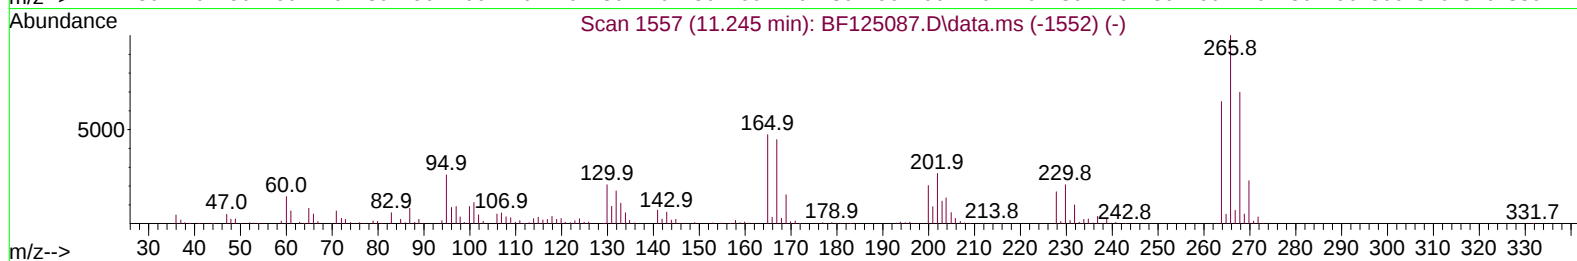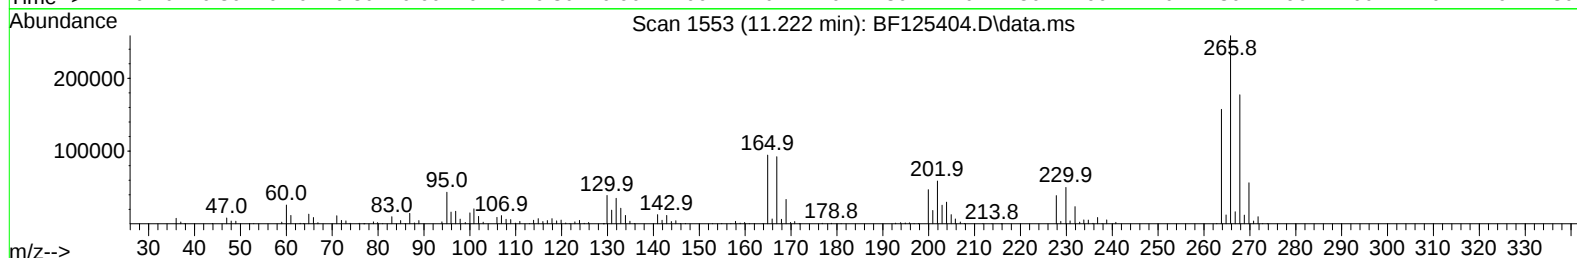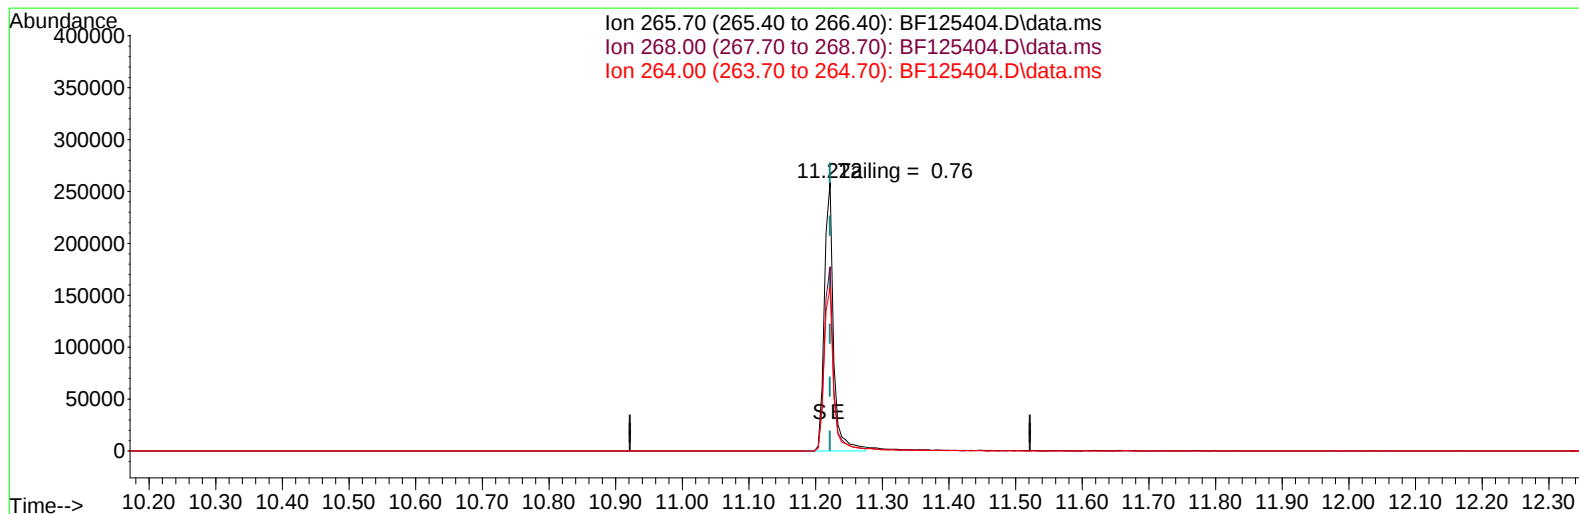

TIC: BF125404.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.000) 36835.53 ng




response 253740

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.61
264.00	69.90	60.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090921\
 Data File : BF125404.D
 Acq On : 9 Sep 2021 9:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 09 11:44:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 08 14:14:01 2021
 Response via : Initial Calibration

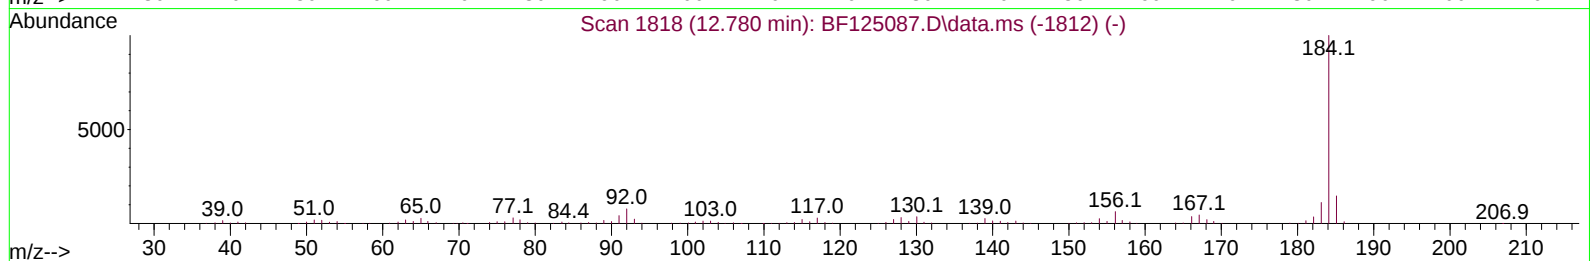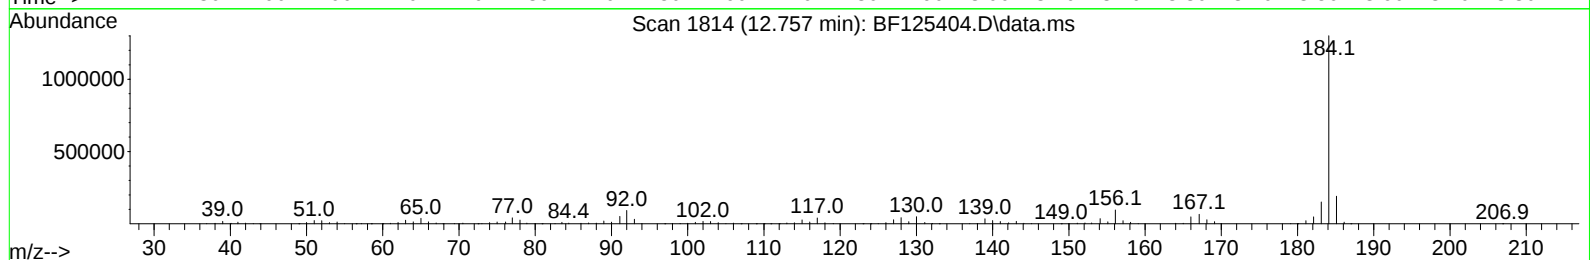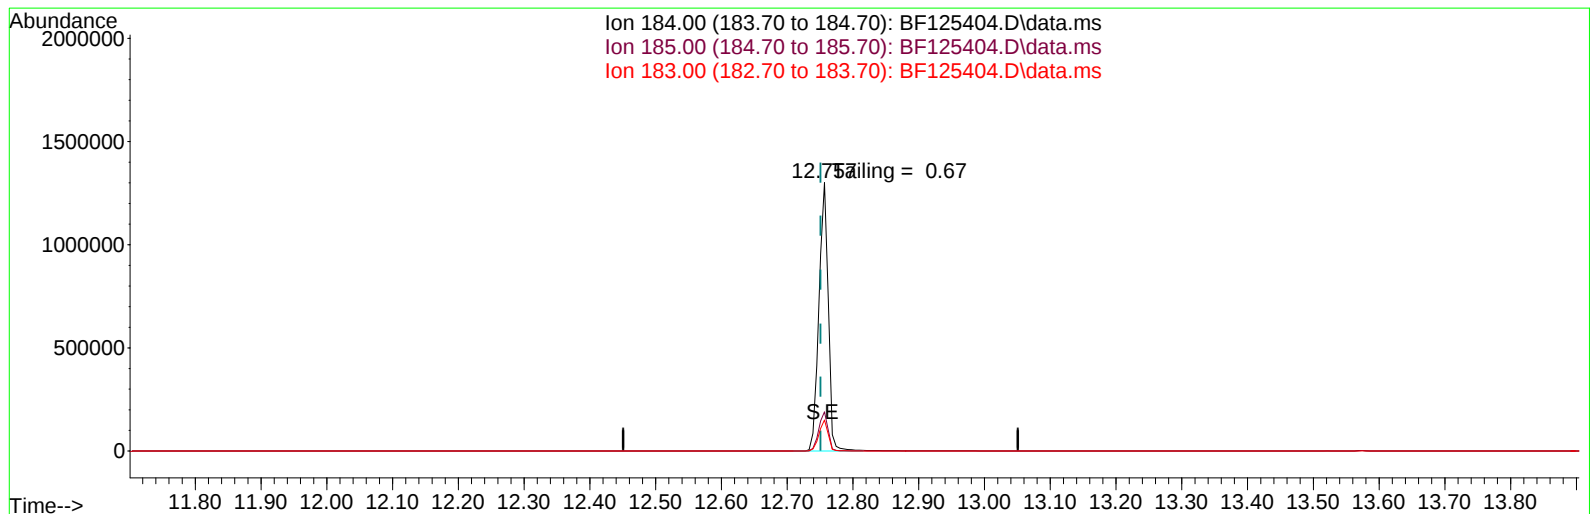

TIC: BF125404.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 1296291

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.63
183.00	10.10	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/9/2021	BNA_F	<u>BF125404.D</u>
Compound Name	Response	Retention Time
DDT	622361	13.57
DDD	11242	13.27
DDE	1936	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13178	635539	2.07

Instrument :
BNA_F
ClientSampleId :
DFTPP