

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090922\
 Data File : BF130193.D
 Acq On : 09 Sep 2022 12:52
 Operator : CG\JU
 Sample : PB147529BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147529BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.910	442	446	455	rVB	115593	157019	2.21%	0.456%
2	5.304	507	513	516	rBV	3739030	4271400	59.99%	12.413%
3	6.328	681	687	690	rBV	3260403	3828636	53.77%	11.126%
4	6.692	745	749	752	rBV	1048614	828621	11.64%	2.408%
5	7.257	839	845	848	rBV	2396636	2491987	35.00%	7.242%
6	7.975	962	967	970	rBV	1230828	1120983	15.74%	3.258%
7	9.051	1144	1150	1153	rBV	5063825	5060263	71.07%	14.705%
8	9.722	1259	1264	1268	rBV	1549070	1373600	19.29%	3.992%
9	10.510	1392	1398	1401	rBV	3642195	3676209	51.63%	10.683%
10	11.204	1512	1516	1519	rBV	1874813	1498312	21.04%	4.354%
11	12.798	1781	1787	1790	rBV	6651875	7120423	100.00%	20.692%
12	13.833	1958	1963	1966	rBV	1839055	1609262	22.60%	4.676%
13	15.233	2195	2201	2206	rBV	1196582	1375028	19.31%	3.996%




Sum of corrected areas: 34411743

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090922\
Data File : BF130193.D
Acq On : 09 Sep 2022 12:52
Operator : CG\JU
Sample : PB147529BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147529BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

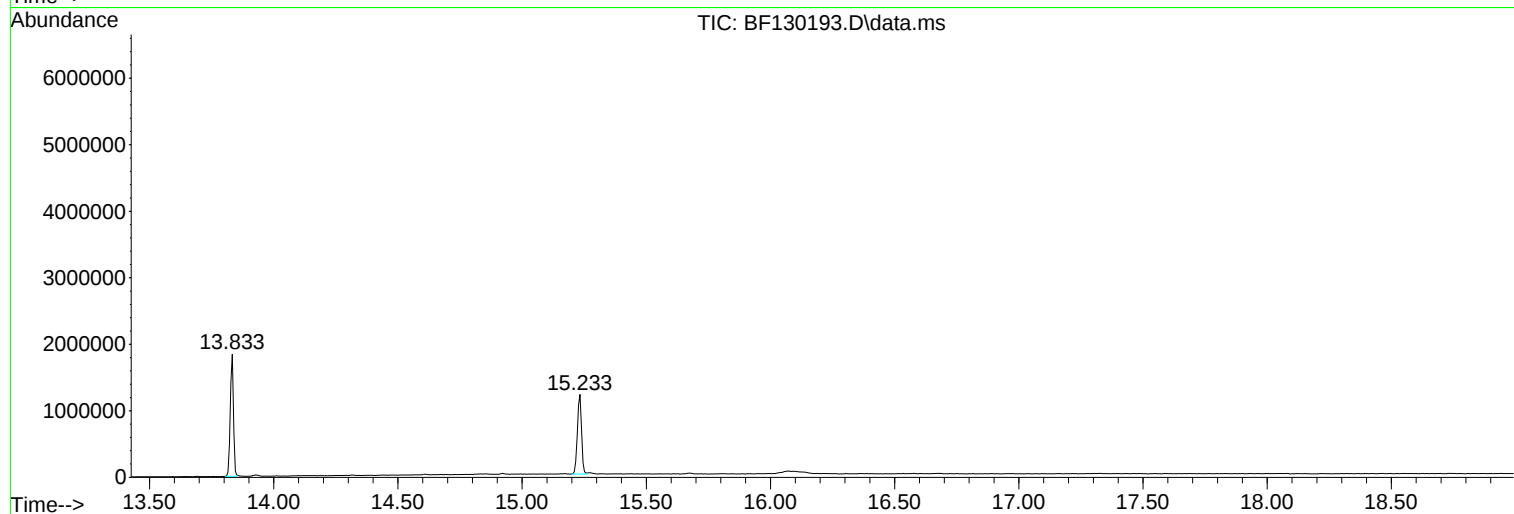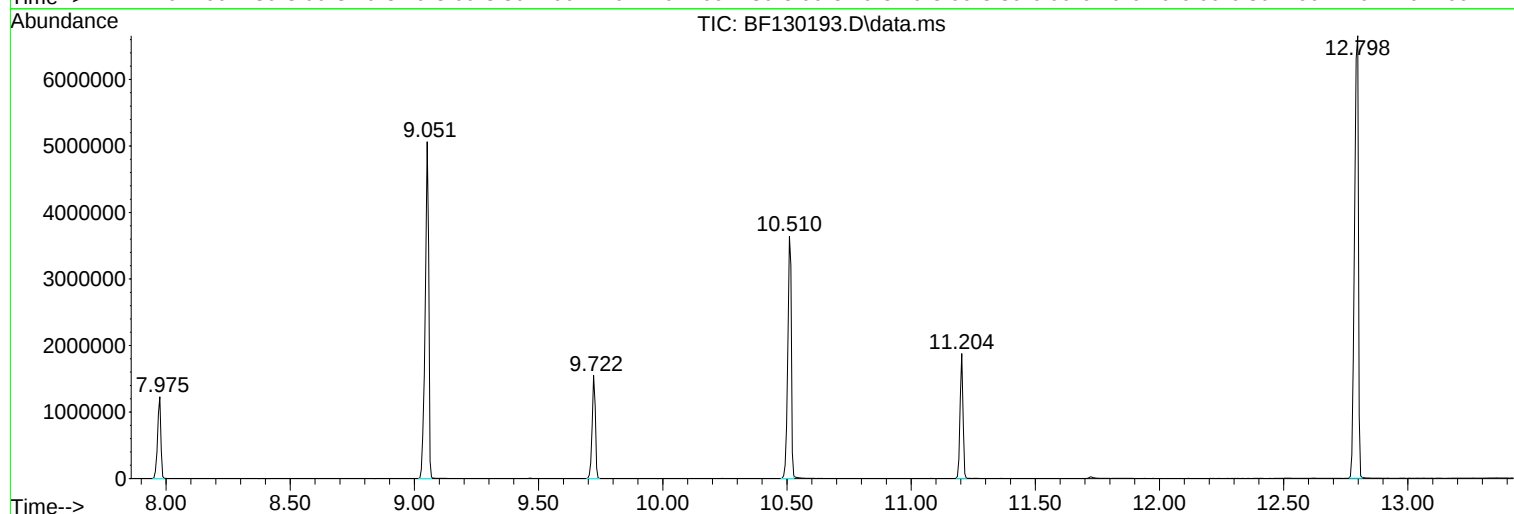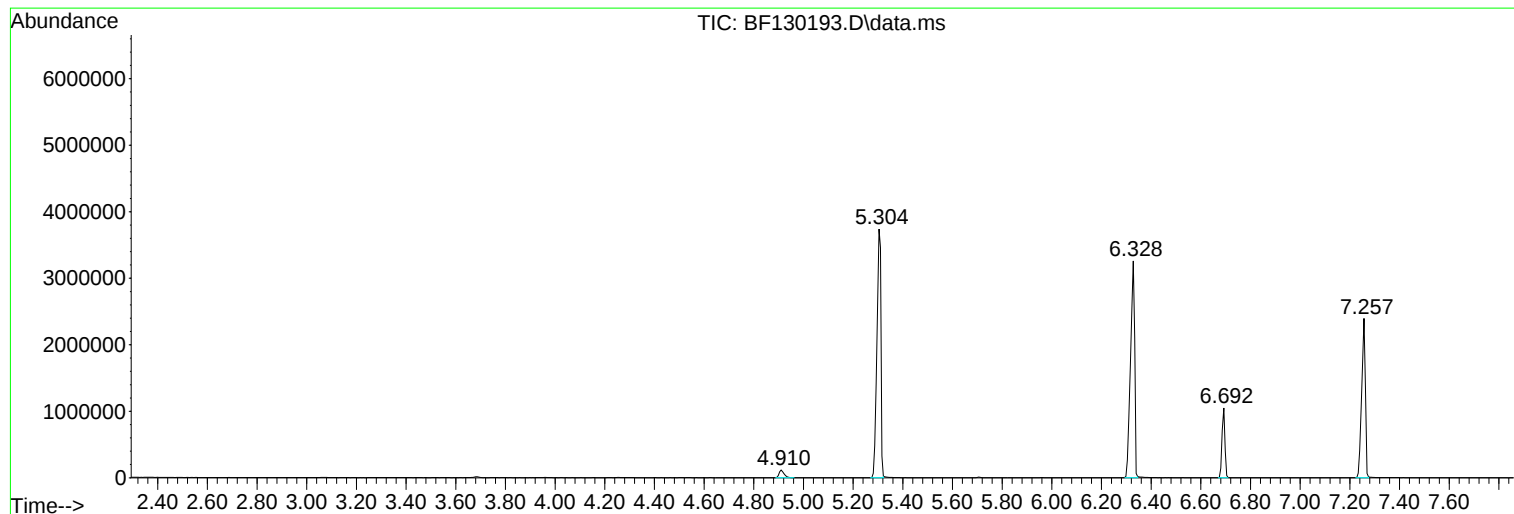

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090922\
Data File : BF130193.D
Acq On : 09 Sep 2022 12:52
Operator : CG\JU
Sample : PB147529BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147529BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090922\
Data File : BF130193.D
Acq On : 09 Sep 2022 12:52
Operator : CG\JU
Sample : PB147529BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147529BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------