


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090922\
Data File : BF130191.D
Acq On : 09 Sep 2022 11:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 07 02:05:07 2022

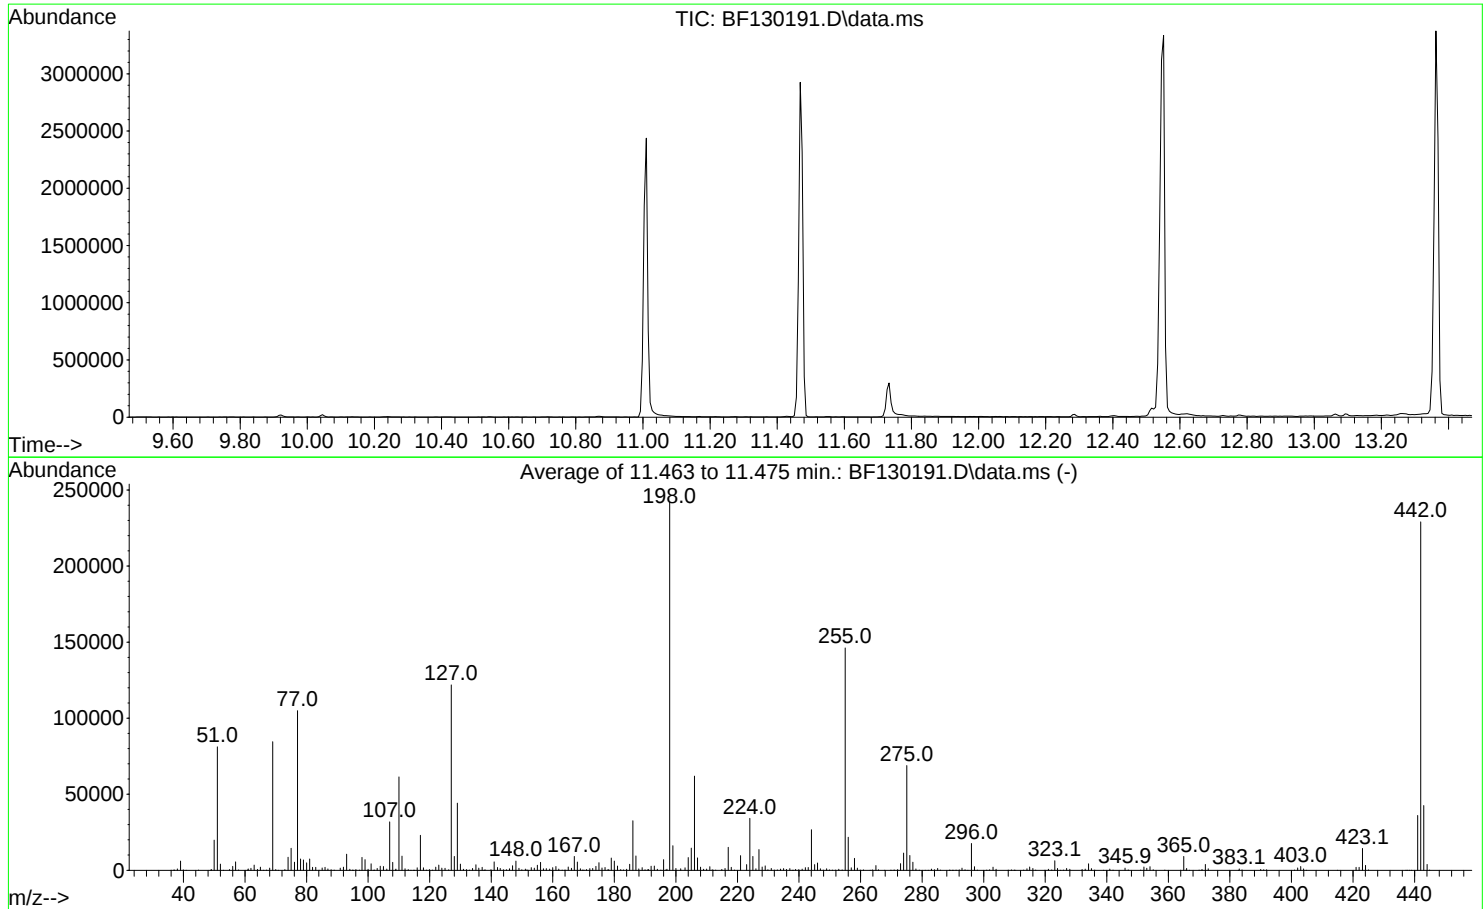




AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	81197	PASS
68	69	0.00	2	1.7	1454	PASS
69	198	0.00	100	34.9	84500	PASS
70	69	0.00	2	0.6	482	PASS
127	198	10	80	50.4	121837	PASS
197	198	0.00	2	0.3	656	PASS
198	198	100	100	100.0	241856	PASS
199	198	5	9	6.7	16182	PASS
275	198	10	60	28.5	68893	PASS
365	198	1	100	3.8	9138	PASS
441	198	0.01	100	14.9	36053	PASS
442	442	50	100	100.0	229093	PASS
443	442	15	24	18.6	42566	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090922\
 Data File : BF130191.D
 Acq On : 09 Sep 2022 11:20
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 10 04:46:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 07 02:05:07 2022
 Response via : Initial Calibration

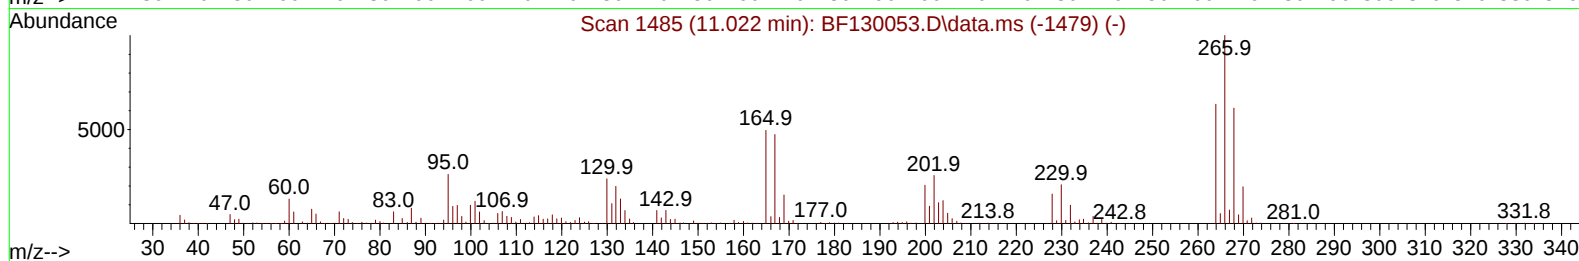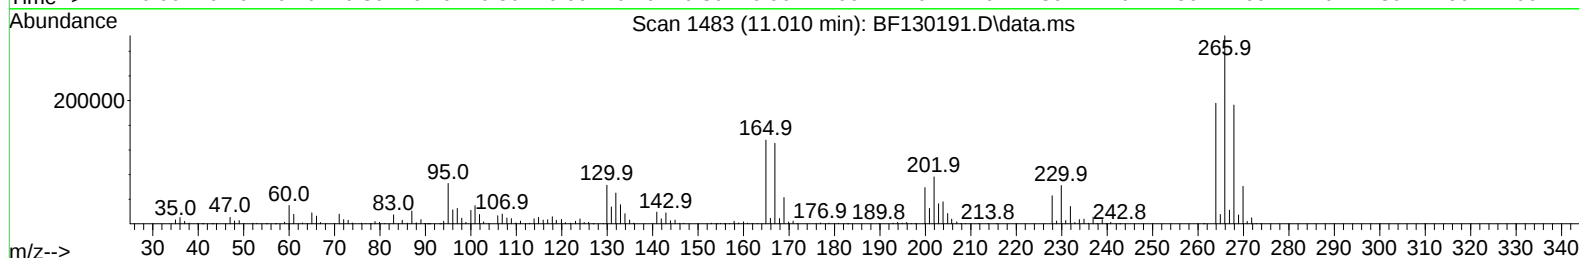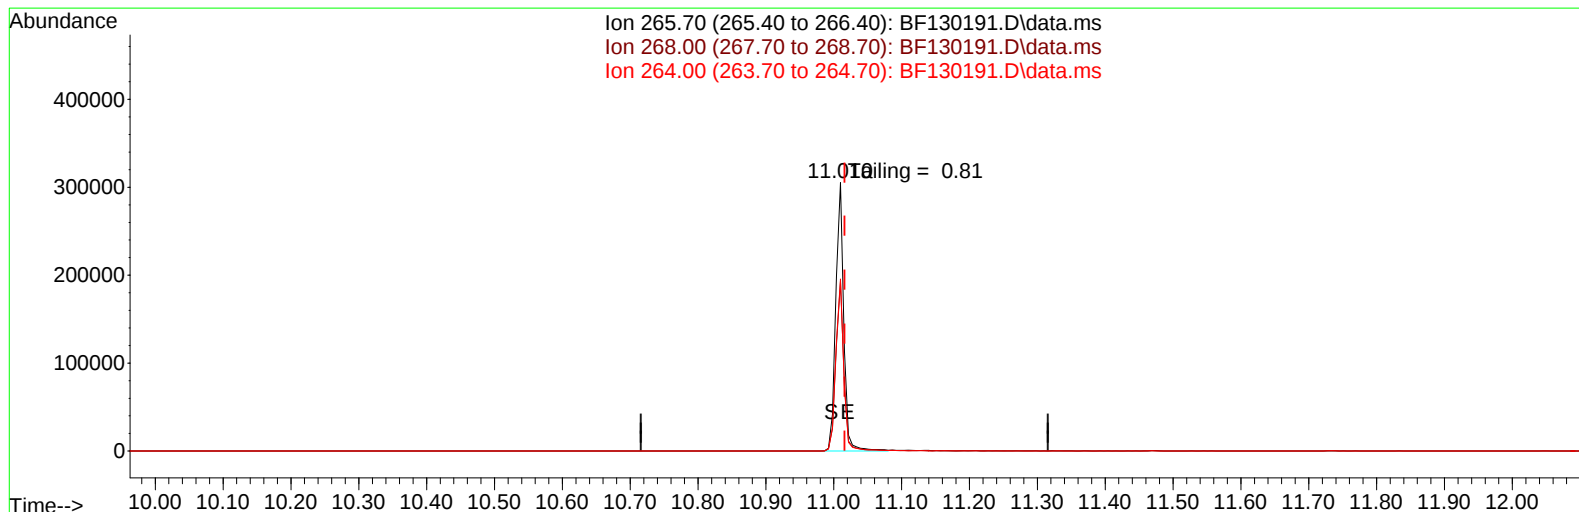

TIC: BF130191.D\data.ms

(70) Pentachlorophenol (C)

11.010min (-0.006) 587208.13 ng




response 250722

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.19
264.00	59.90	64.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090922\
 Data File : BF130191.D
 Acq On : 09 Sep 2022 11:20
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 10 04:46:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 07 02:05:07 2022
 Response via : Initial Calibration

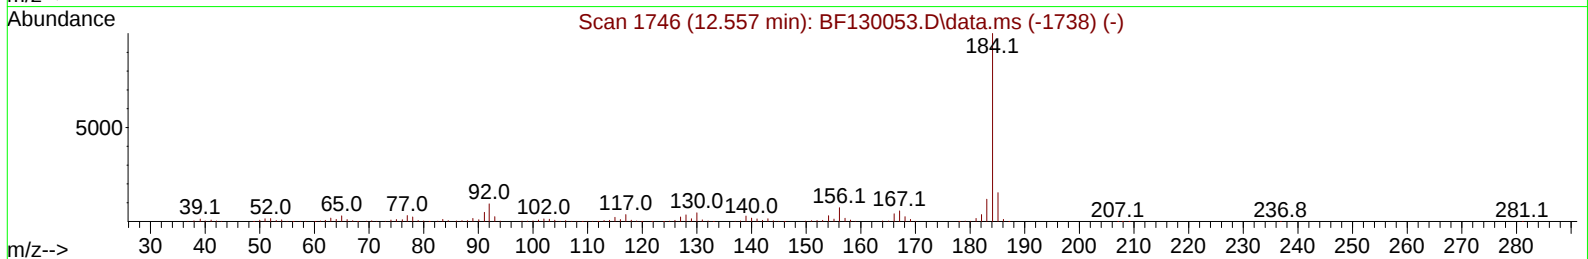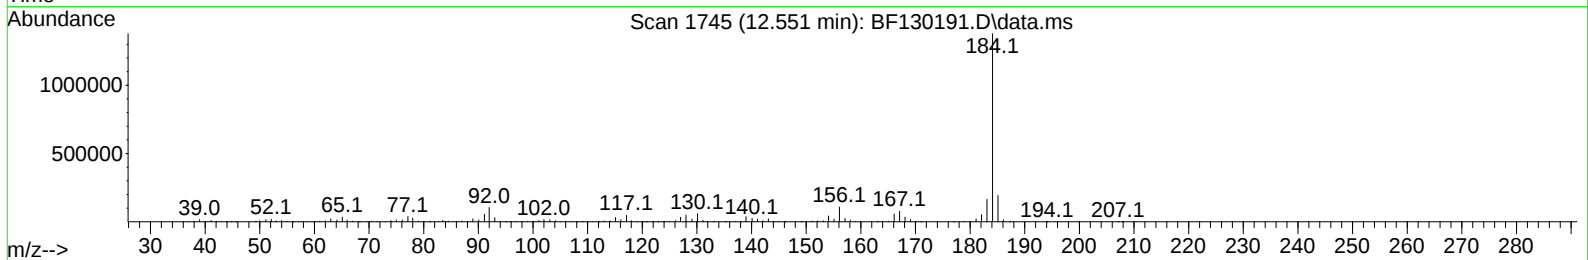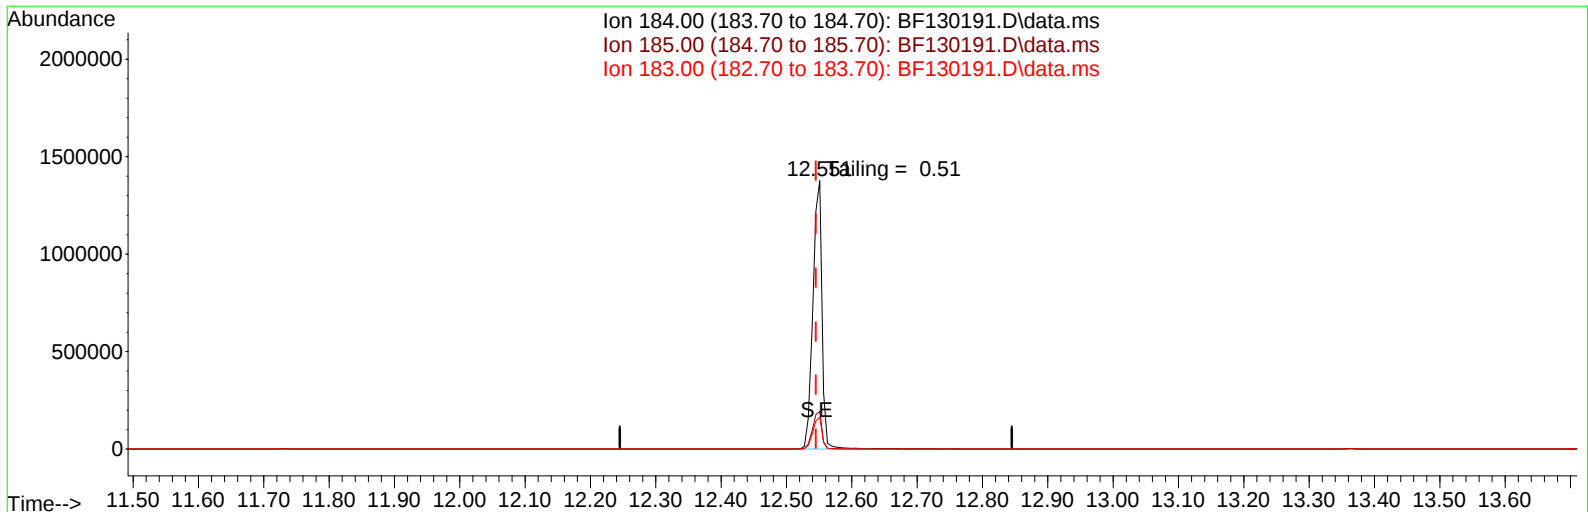

TIC: BF130191.D\data.ms

(77) Benzidine

12.551min (+ 0.006) 86185.53 ng

response 1337980

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.01
183.00	11.80	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/9/2022	BNA_F	<u>BF130191.D</u>
Compound Name	Response	Retention Time
DDT	552269	13.363
DDD	5428	13.063
DDE	626	12.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6054	558323	1.08

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP