
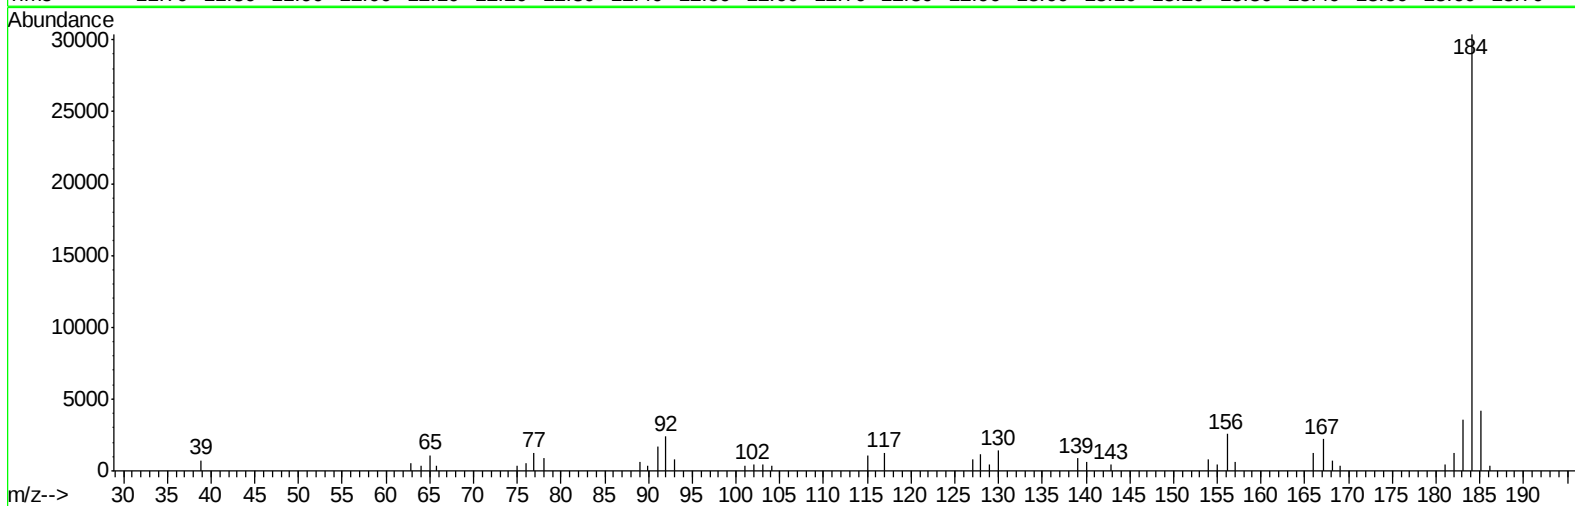


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091019\
Data File : BF116918.D
Acq On : 10 Sep 2019 13:49
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 06:36:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 17:49:40 2019
Response via : Initial Calibration

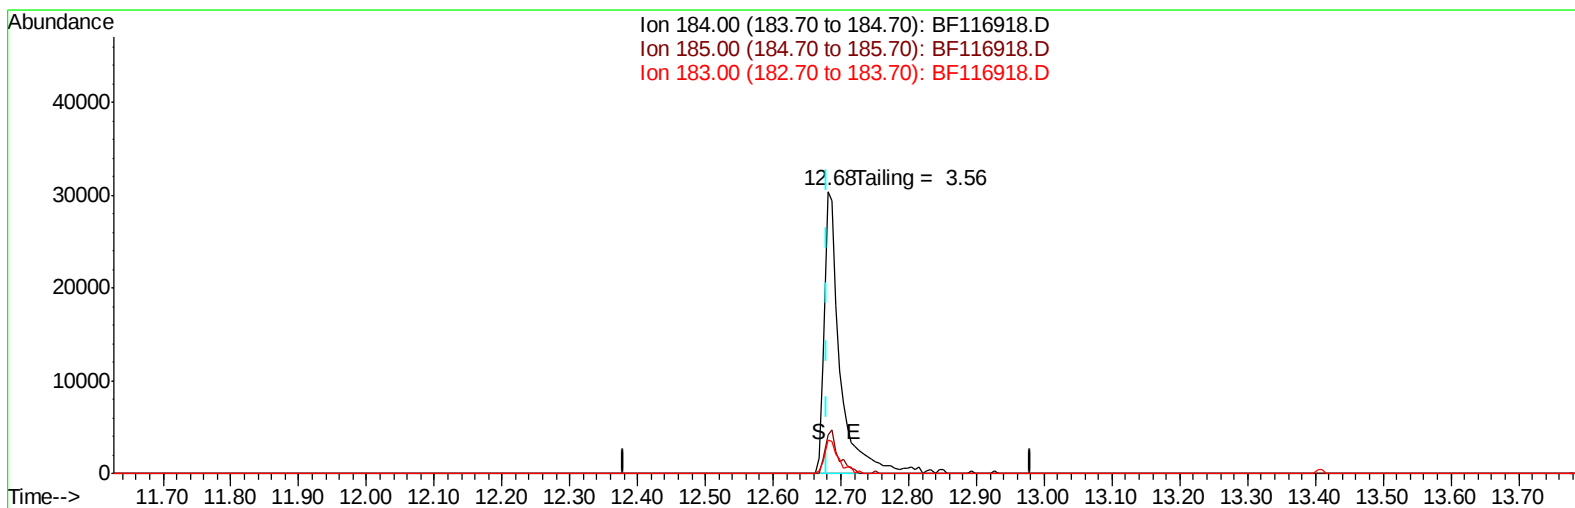

TIC: BF116918.D

(77) Benzidine



12.680min (+0.000) 0.00ng

response 47746

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.86
183.00	11.50	11.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091019\
Data File : BF116918.D
Acq On : 10 Sep 2019 13:49
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 06:36:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 17:49:40 2019
Response via : Initial Calibration

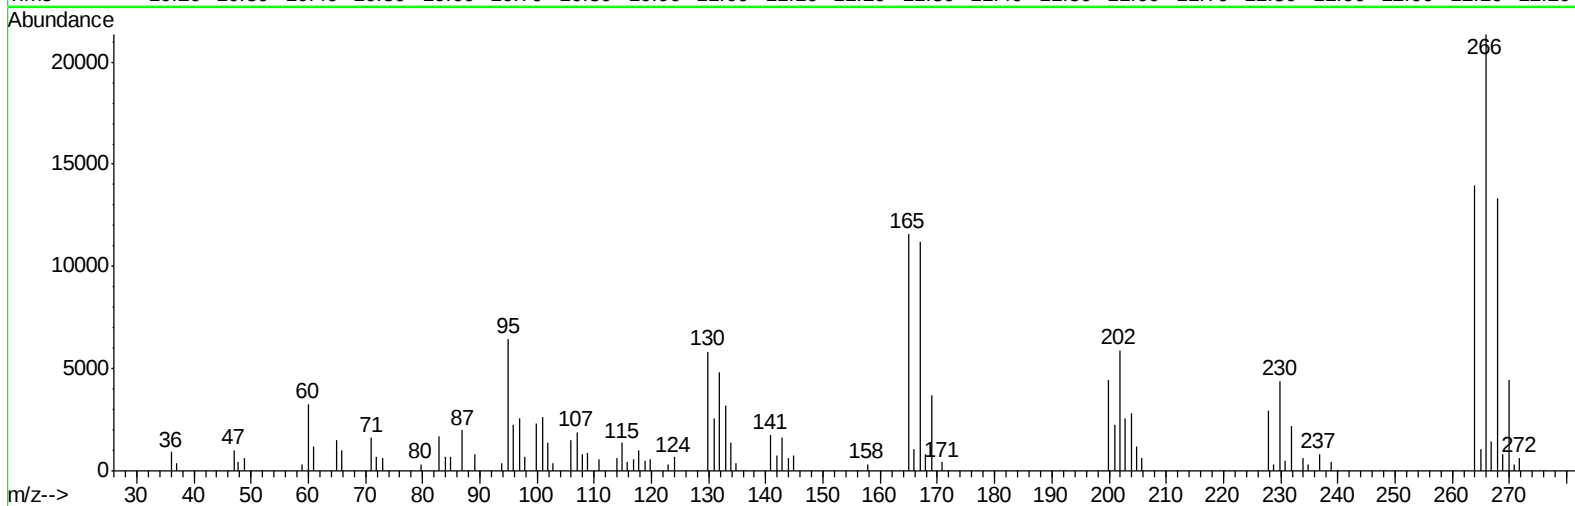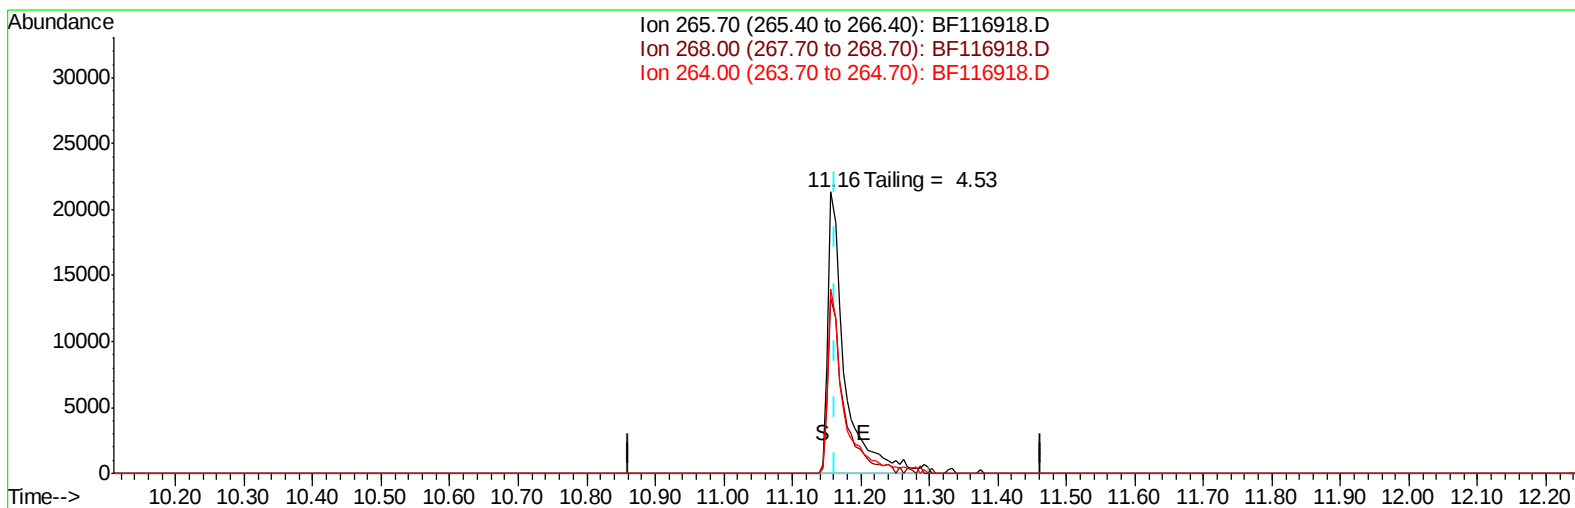

TIC: BF116918.D

(70) Pentachlorophenol (C)

11.157min (-0.006) 0.00ng

response 34194

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	62.43
264.00	64.90	65.51
0.00	0.00	0.00