

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091019\
 Data File : BF116924.D
 Acq On : 10 Sep 2019 16:33
 Operator : HP/JU
 Sample : PB122923BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB122923TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	10	14	19	rVB	32291	42935	1.34%	0.191%
2	5.463	569	574	577	rBV	2178171	2127292	66.17%	9.473%
3	6.469	739	745	748	rBV	2206903	2277009	70.83%	10.140%
4	6.604	764	768	772	rBV	2335815	2379483	74.02%	10.596%
5	6.833	803	807	818	rVB	661336	541874	16.86%	2.413%
6	6.992	829	834	837	rBV	2072601	1791235	55.72%	7.977%
7	7.392	897	902	905	rBV	1374217	1408253	43.81%	6.271%
8	8.116	1020	1025	1046	rBV	681250	711842	22.14%	3.170%
9	9.186	1202	1207	1222	rBV	3056099	2966945	92.29%	13.212%
10	9.869	1318	1323	1341	rBB	779395	829284	25.80%	3.693%
11	10.657	1452	1457	1474	rBV	1611573	1747162	54.35%	7.780%
12	11.351	1571	1575	1590	rVB	802384	826712	25.72%	3.681%
13	12.933	1839	1844	1847	rBV	3398249	3214743	100.00%	14.316%
14	13.980	2018	2022	2034	rVB	644868	685617	21.33%	3.053%
15	14.745	2147	2152	2157	rBV	45879	51053	1.59%	0.227%
16	15.080	2205	2209	2214	rVB	53656	58353	1.82%	0.260%
17	15.433	2263	2269	2280	rBV	407021	623632	19.40%	2.777%
18	15.880	2336	2345	2350	rBV2	49791	75392	2.35%	0.336%
19	16.374	2421	2429	2436	rBV3	30876	57779	1.80%	0.257%
20	16.950	2520	2527	2535	rBV7	17287	39393	1.23%	0.175%


Sum of corrected areas: 22455988

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091019\
Data File : BF116924.D
Acq On : 10 Sep 2019 16:33
Operator : HP/JU
Sample : PB122923BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB122923TB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

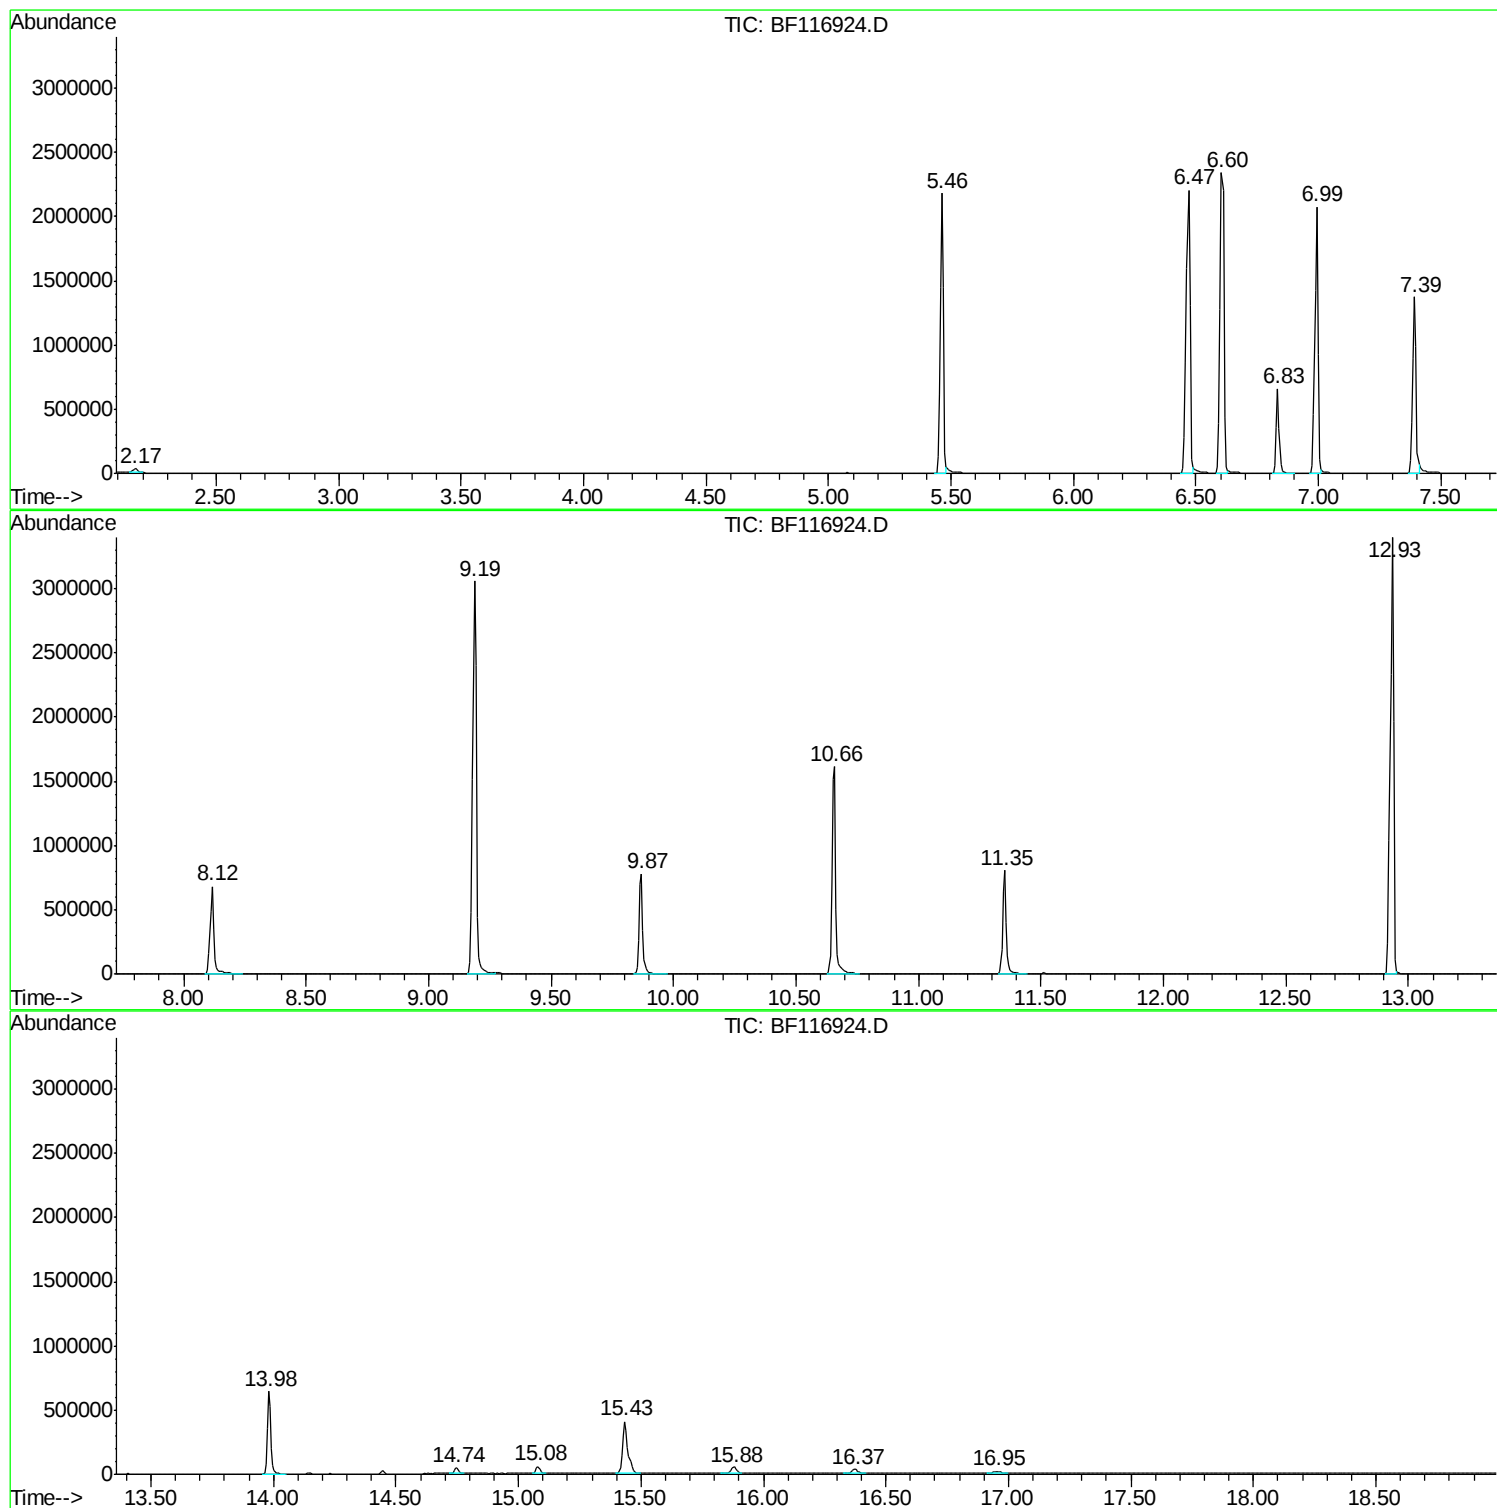

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091019\
Data File : BF116924.D
Acq On : 10 Sep 2019 16:33
Operator : HP/JU
Sample : PB122923BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB122923TB










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	87.82 ng	2379480	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27	
2	Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12	
3	5-Aminoindole	132	C8H8N2	005192-03-0	12	
4	Xenon	132	Xe	007440-63-3	9	
5	Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9	

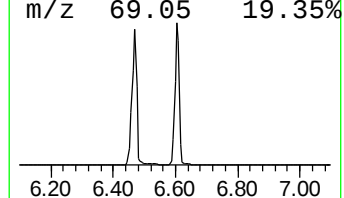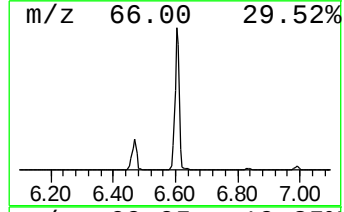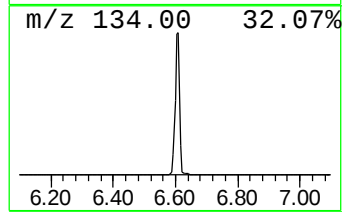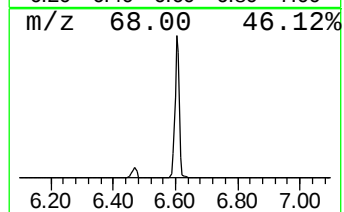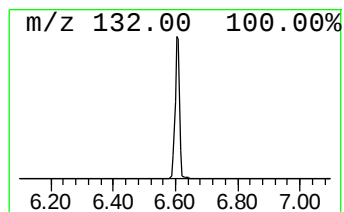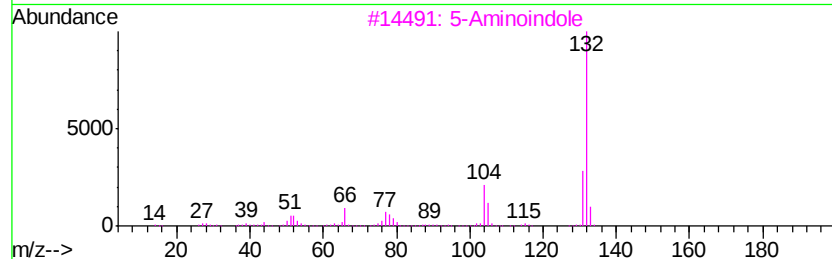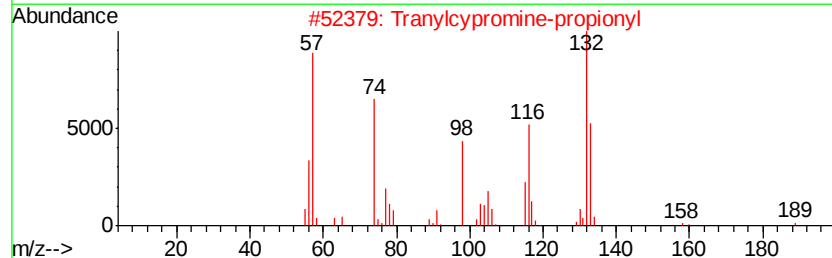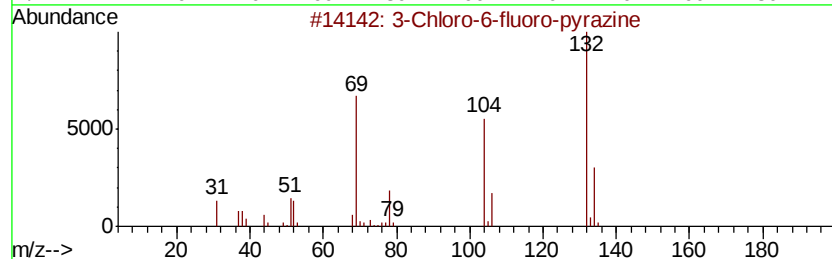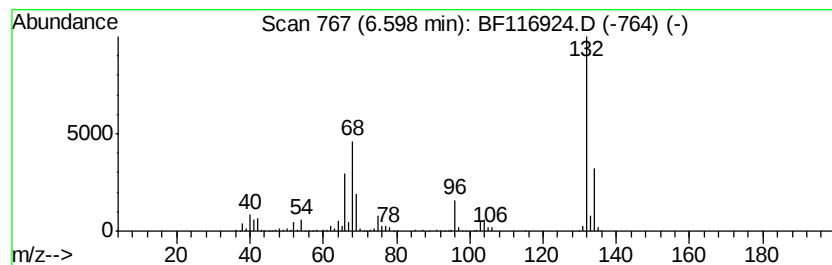

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091019\
Data File : BF116924.D
Acq On : 10 Sep 2019 16:33
Operator : HP/JU
Sample : PB122923BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB122923TB










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Eicosane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.88	2.42 ng	75392	Perylene-d12	15.43

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Eicosane	282	C20H42	000112-95-8	93
2		2-methyltetracosane	352	C25H52	1000376-72-6	91
3		2-methyloctacosane	408	C29H60	1000376-72-8	91
4		Heneicosane	296	C21H44	000629-94-7	80
5		Hexacosane	366	C26H54	000630-01-3	80

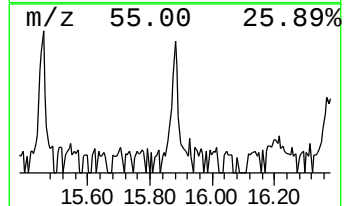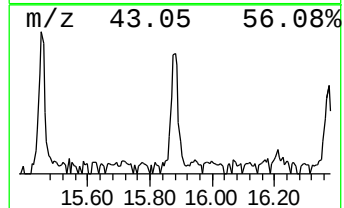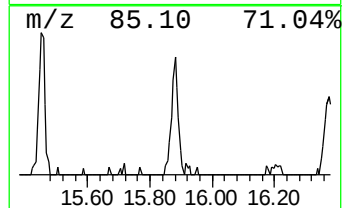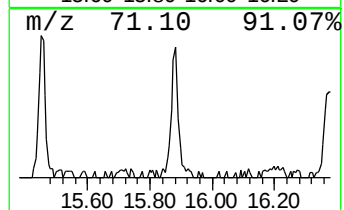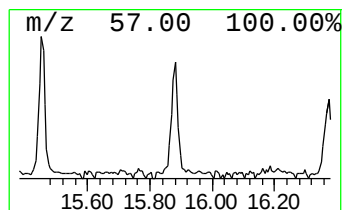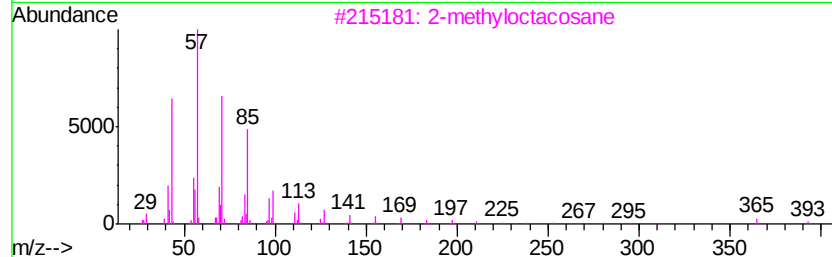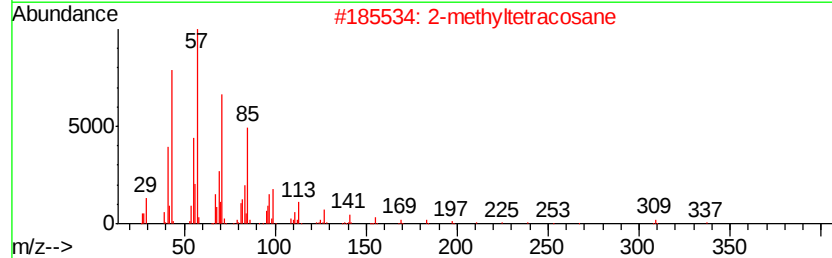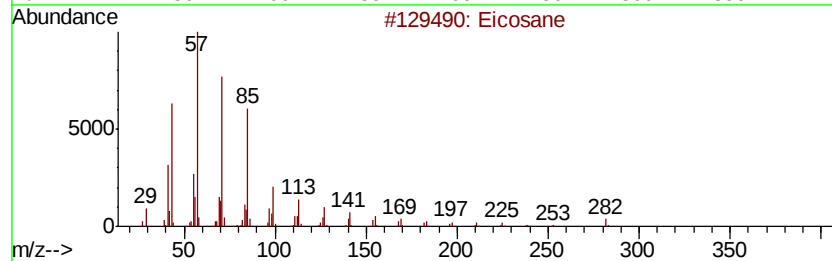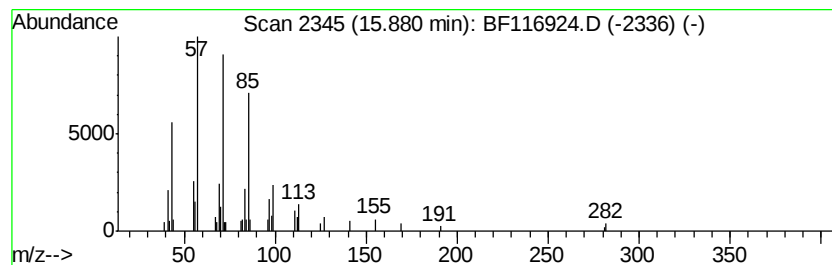

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091019\
Data File : BF116924.D
Acq On : 10 Sep 2019 16:33
Operator : HP/JU
Sample : PB122923BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB122923TB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.60	6.60	87.8	ng	2379480	1	6.83	541874	20.0
Eicosane	15.88	2.4	ng	75392	6	15.43	623632	20.0