


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091019\
 Data File : BF116918.D
 Acq On : 10 Sep 2019 13:49
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 10 17:49:40 2019

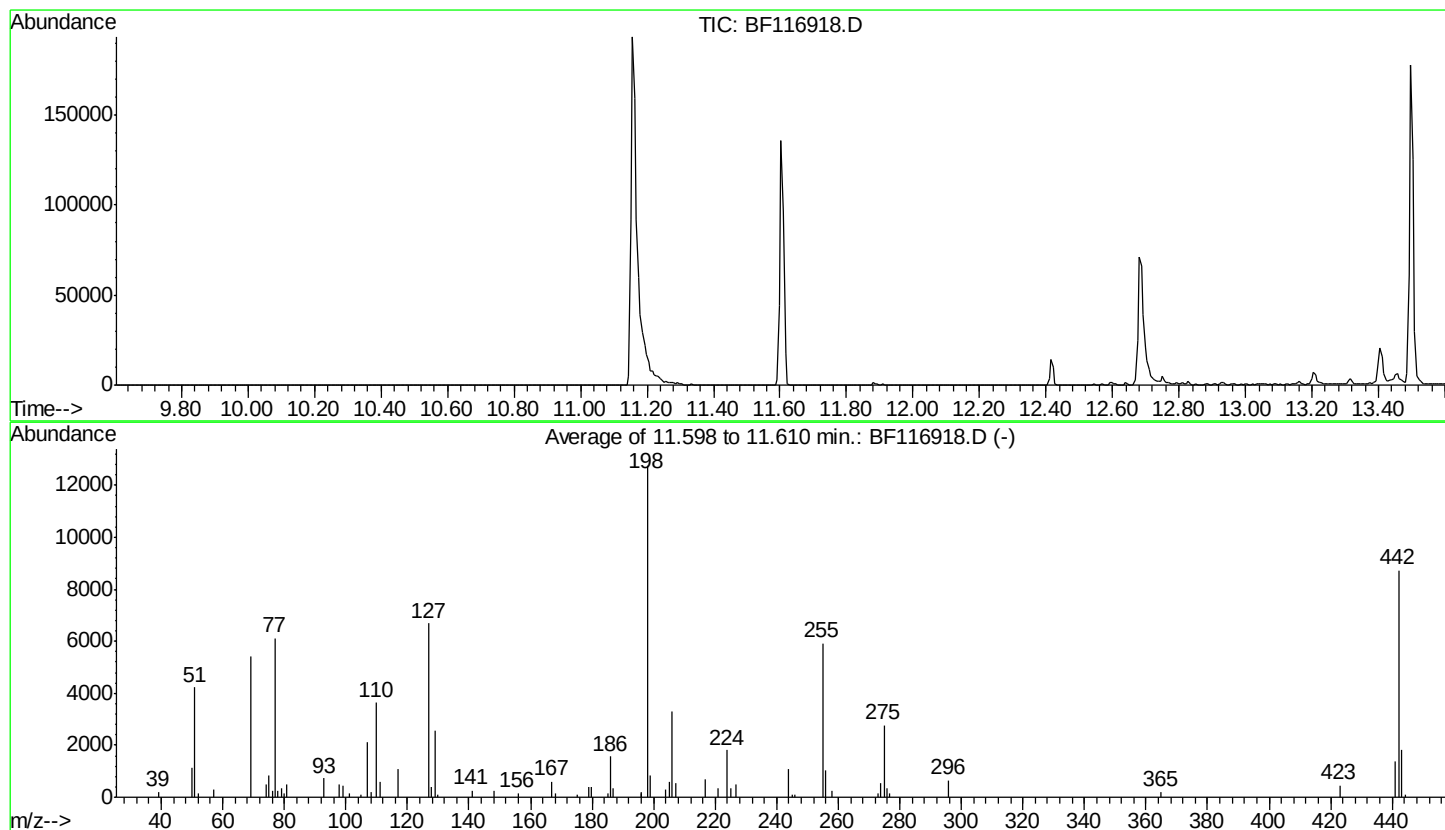

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	4228	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.5	5425	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	6696	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12754	PASS
199	198	5	9	6.7	849	PASS
275	198	10	60	21.7	2772	PASS
365	198	1	100	1.6	206	PASS
441	198	0.01	100	11.0	1397	PASS
442	198	50	100	68.4	8728	PASS
443	442	15	24	20.6	1802	PASS