


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091019\
 Data File : BF116943.D
 Acq On : 11 Sep 2019 2:07
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 10 17:49:40 2019

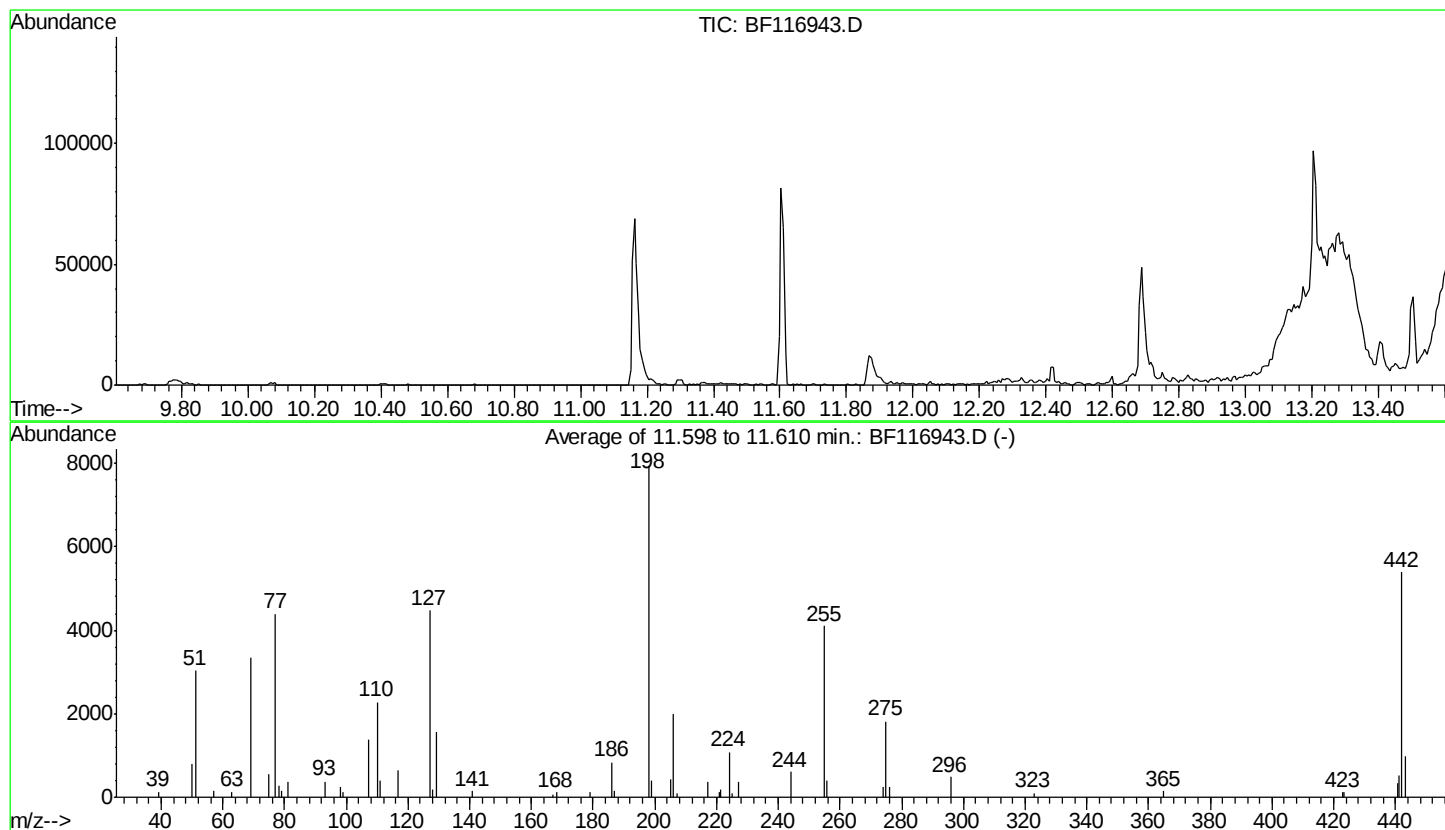

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	3032	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.2	3348	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.2	4466	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	7943	PASS
199	198	5	9	5.2	412	PASS
275	198	10	60	22.9	1819	PASS
365	198	1	100	1.9	151	PASS
441	198	0.01	100	6.4	508	PASS
442	198	50	100	67.8	5386	PASS
443	442	15	24	18.3	987	PASS