


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091118\
 Data File : BF108926.D
 Acq On : 11 Sep 2018 11:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 05 18:03:31 2018

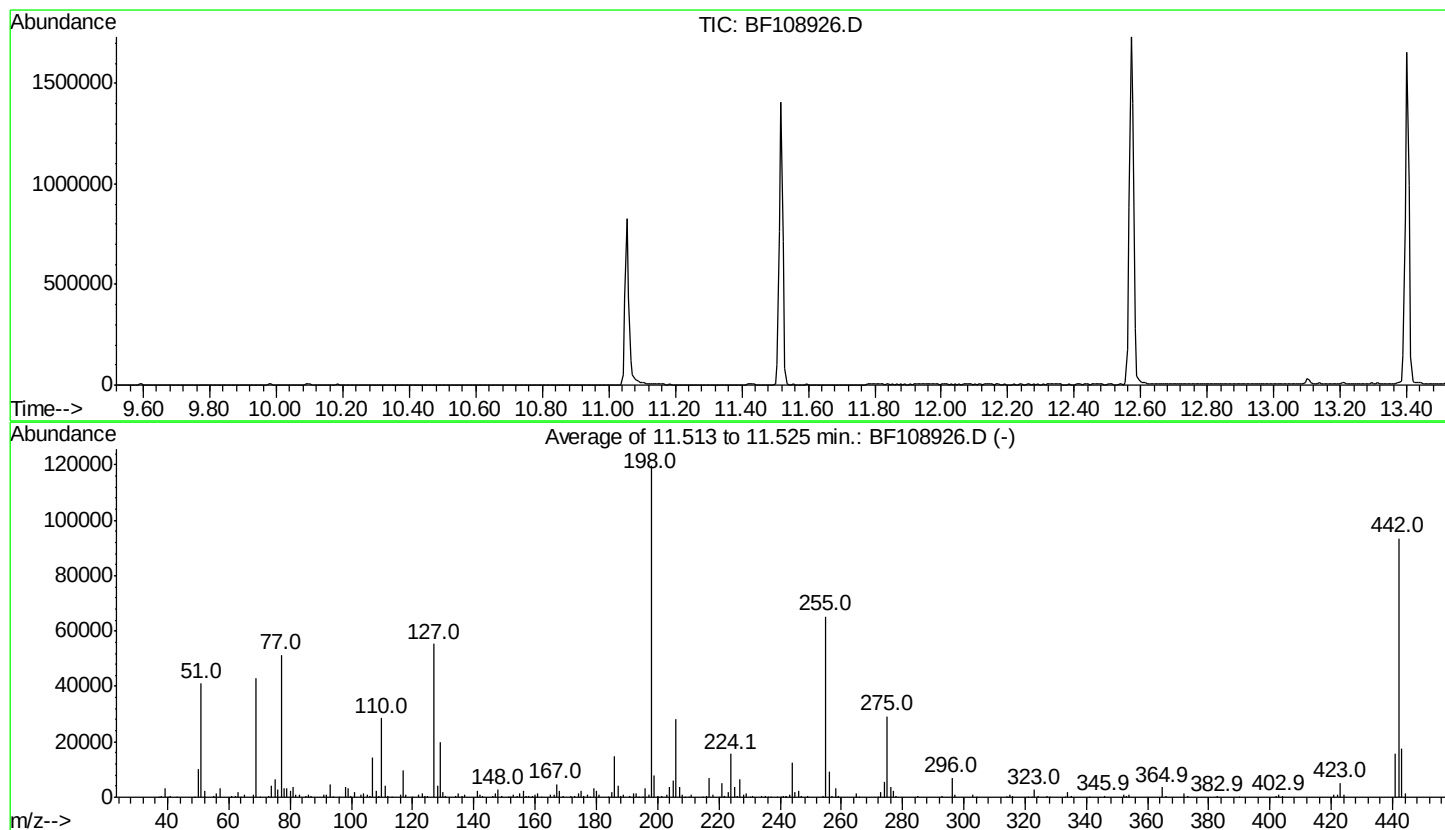

AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	41024	PASS
68	69	0.00	2	1.8	783	PASS
69	198	0.00	100	36.0	43066	PASS
70	69	0.00	2	0.3	112	PASS
127	198	10	80	46.2	55330	PASS
197	198	0.00	2	0.6	725	PASS
198	198	100	100	100.0	119728	PASS
199	198	5	9	6.6	7857	PASS
275	198	10	60	24.5	29362	PASS
365	198	1	100	3.1	3656	PASS
441	198	0.01	100	13.0	15554	PASS
442	198	50	100	78.1	93448	PASS
443	442	15	24	18.6	17358	PASS