
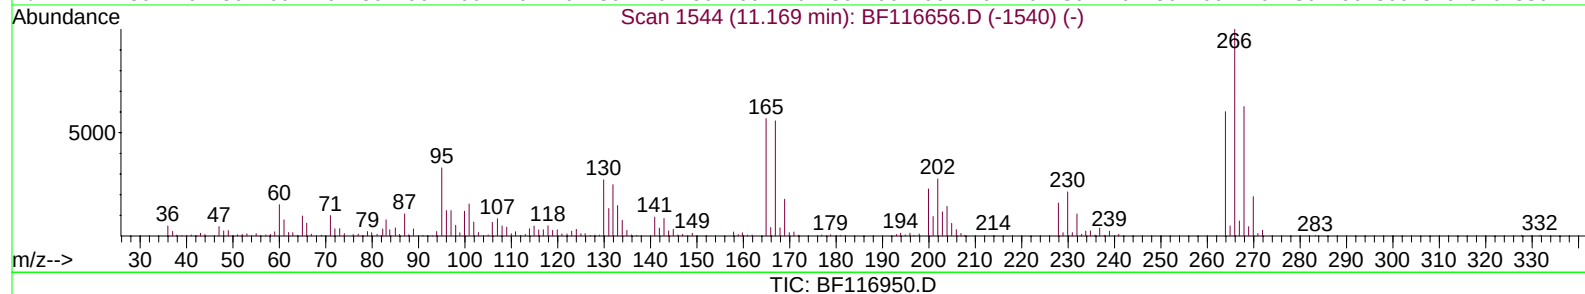
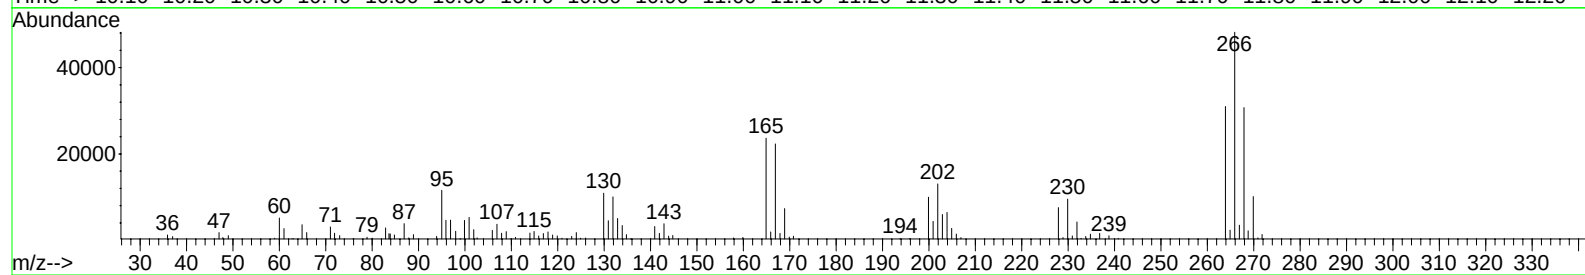


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091119\
Data File : BF116950.D
Acq On : 11 Sep 2019 16:34
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 18:22:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 12 08:24:39 2019
Response via : Initial Calibration

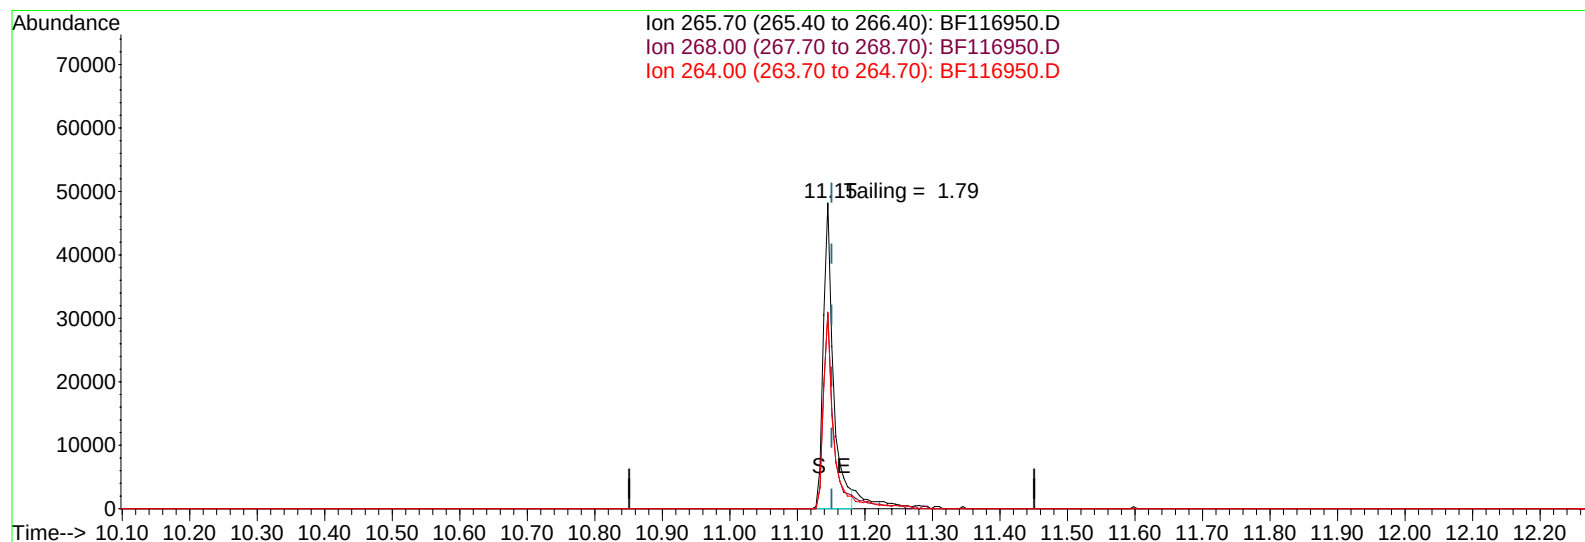

(70) Pentachlorophenol (C)




11.145min (-0.006) 77763.96ng

response 55576

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	63.74
264.00	65.10	64.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091119\
Data File : BF116950.D
Acq On : 11 Sep 2019 16:34
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 18:22:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 12 08:24:39 2019
Response via : Initial Calibration

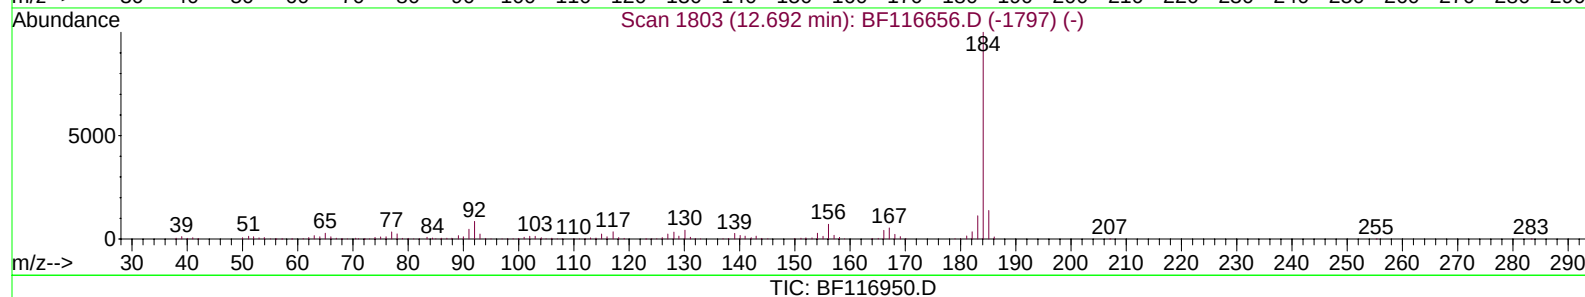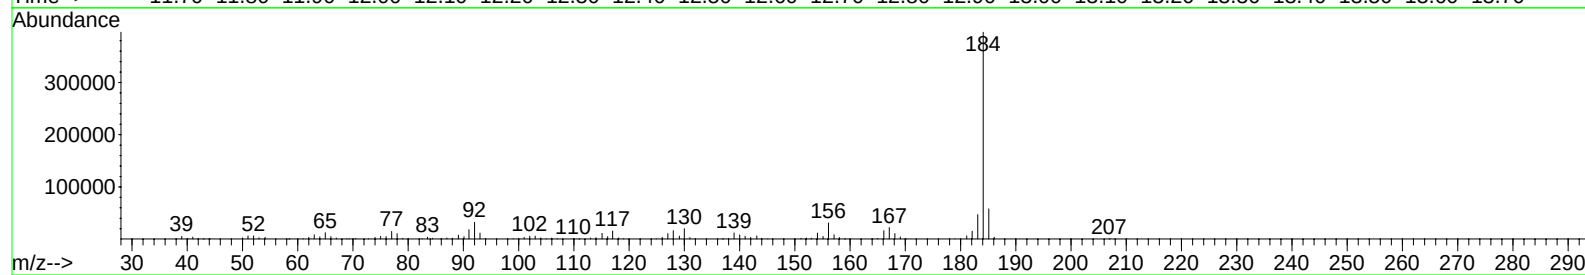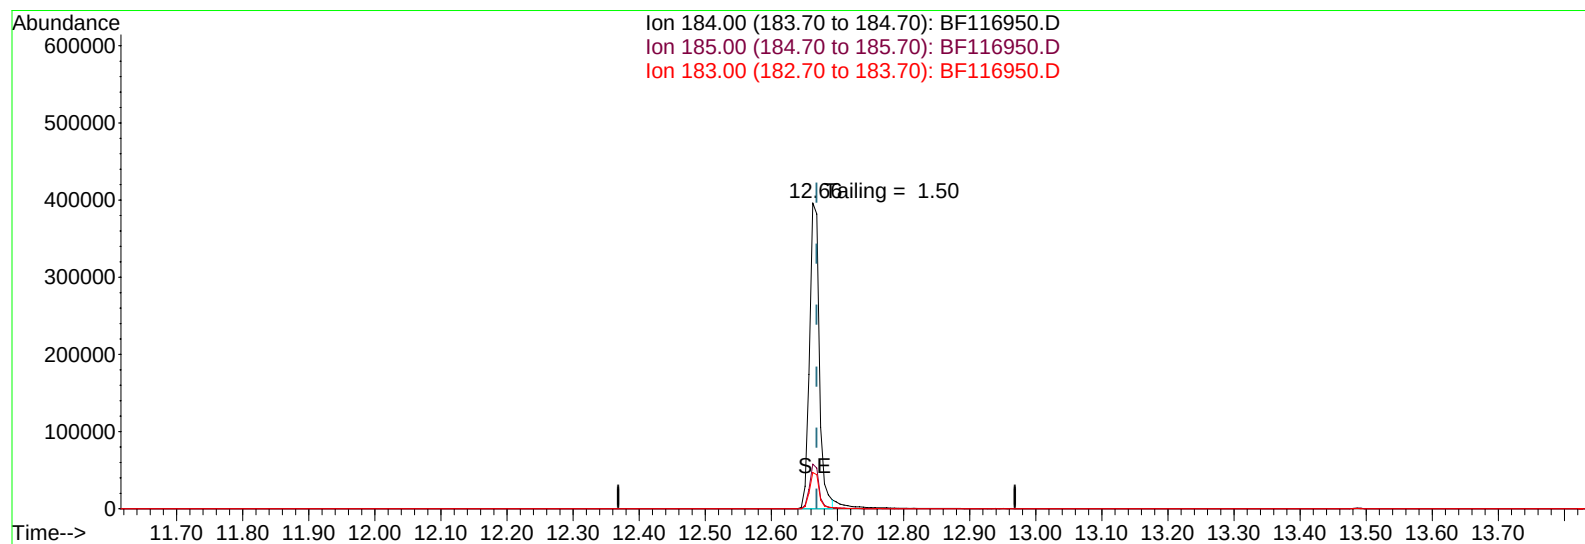

(77) Benzidine

12.663min (-0.006) 0.00ng

response 423029

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.62
183.00	11.50	11.81
0.00	0.00	0.00