

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091119\
 Data File : BF116973.D
 Acq On : 12 Sep 2019 3:20
 Operator : HP/JU
 Sample : K4787-01 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3-S(1-4)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	565	569	584	rBV	650833	590616	72.96%	6.770%
2	6.451	738	742	756	rBV	731295	661484	81.71%	7.582%
3	6.592	762	766	773	rBV	795272	681080	84.13%	7.806%
4	6.822	802	805	817	rBV	455270	382715	47.28%	4.387%
5	6.981	828	832	846	rBV	599138	515914	63.73%	5.913%
6	7.381	896	900	914	rBV	436707	403911	49.89%	4.630%
7	8.104	1019	1023	1030	rBV	586122	517055	63.87%	5.926%
8	9.175	1201	1205	1218	rBV	953325	809534	100.00%	9.279%
9	9.569	1268	1272	1279	rBV	68578	66160	8.17%	0.758%
10	9.857	1317	1321	1330	rBV	701081	647488	79.98%	7.421%
11	10.639	1450	1454	1463	rBV	490449	474948	58.67%	5.444%
12	10.757	1471	1474	1481	rBV3	7858	13268	1.64%	0.152%
13	11.333	1569	1572	1581	rBV	656204	662221	81.80%	7.590%
14	11.857	1659	1661	1666	rBV2	31078	33743	4.17%	0.387%
15	12.421	1753	1757	1762	rVB3	12039	11375	1.41%	0.130%
16	12.545	1775	1778	1781	rBV	46716	39400	4.87%	0.452%
17	12.645	1790	1795	1797	rBV3	12820	16761	2.07%	0.192%
18	12.774	1812	1817	1826	rVB	48035	54700	6.76%	0.627%
19	12.916	1837	1841	1844	rBV	877936	765314	94.54%	8.772%
20	13.098	1870	1872	1877	rVB5	17437	17809	2.20%	0.204%
21	13.363	1913	1917	1920	rBV6	9470	15439	1.91%	0.177%
22	13.610	1956	1959	1963	rBV5	8493	12460	1.54%	0.143%
23	13.821	1991	1995	2002	rBV8	26273	47099	5.82%	0.540%
24	13.968	2015	2020	2023	rBV	587372	534157	65.98%	6.122%
25	14.433	2097	2099	2105	rBV7	18438	22251	2.75%	0.255%
26	14.992	2192	2194	2197	rBV2	26540	33233	4.11%	0.381%
27	15.062	2204	2206	2210	rVB	32142	29641	3.66%	0.340%
28	15.351	2252	2255	2257	rBV	26504	36326	4.49%	0.416%
29	15.415	2261	2266	2277	rVB	394136	562575	69.49%	6.448%
30	15.862	2337	2342	2345	rBV5	26980	47466	5.86%	0.544%
31	16.339	2420	2423	2424	rBV3	15920	18511	2.29%	0.212%


Sum of corrected areas: 8724654

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091119\
Data File : BF116973.D
Acq On : 12 Sep 2019 3:20
Operator : HP/JU
Sample : K4787-01 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
TP-3-S(1-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

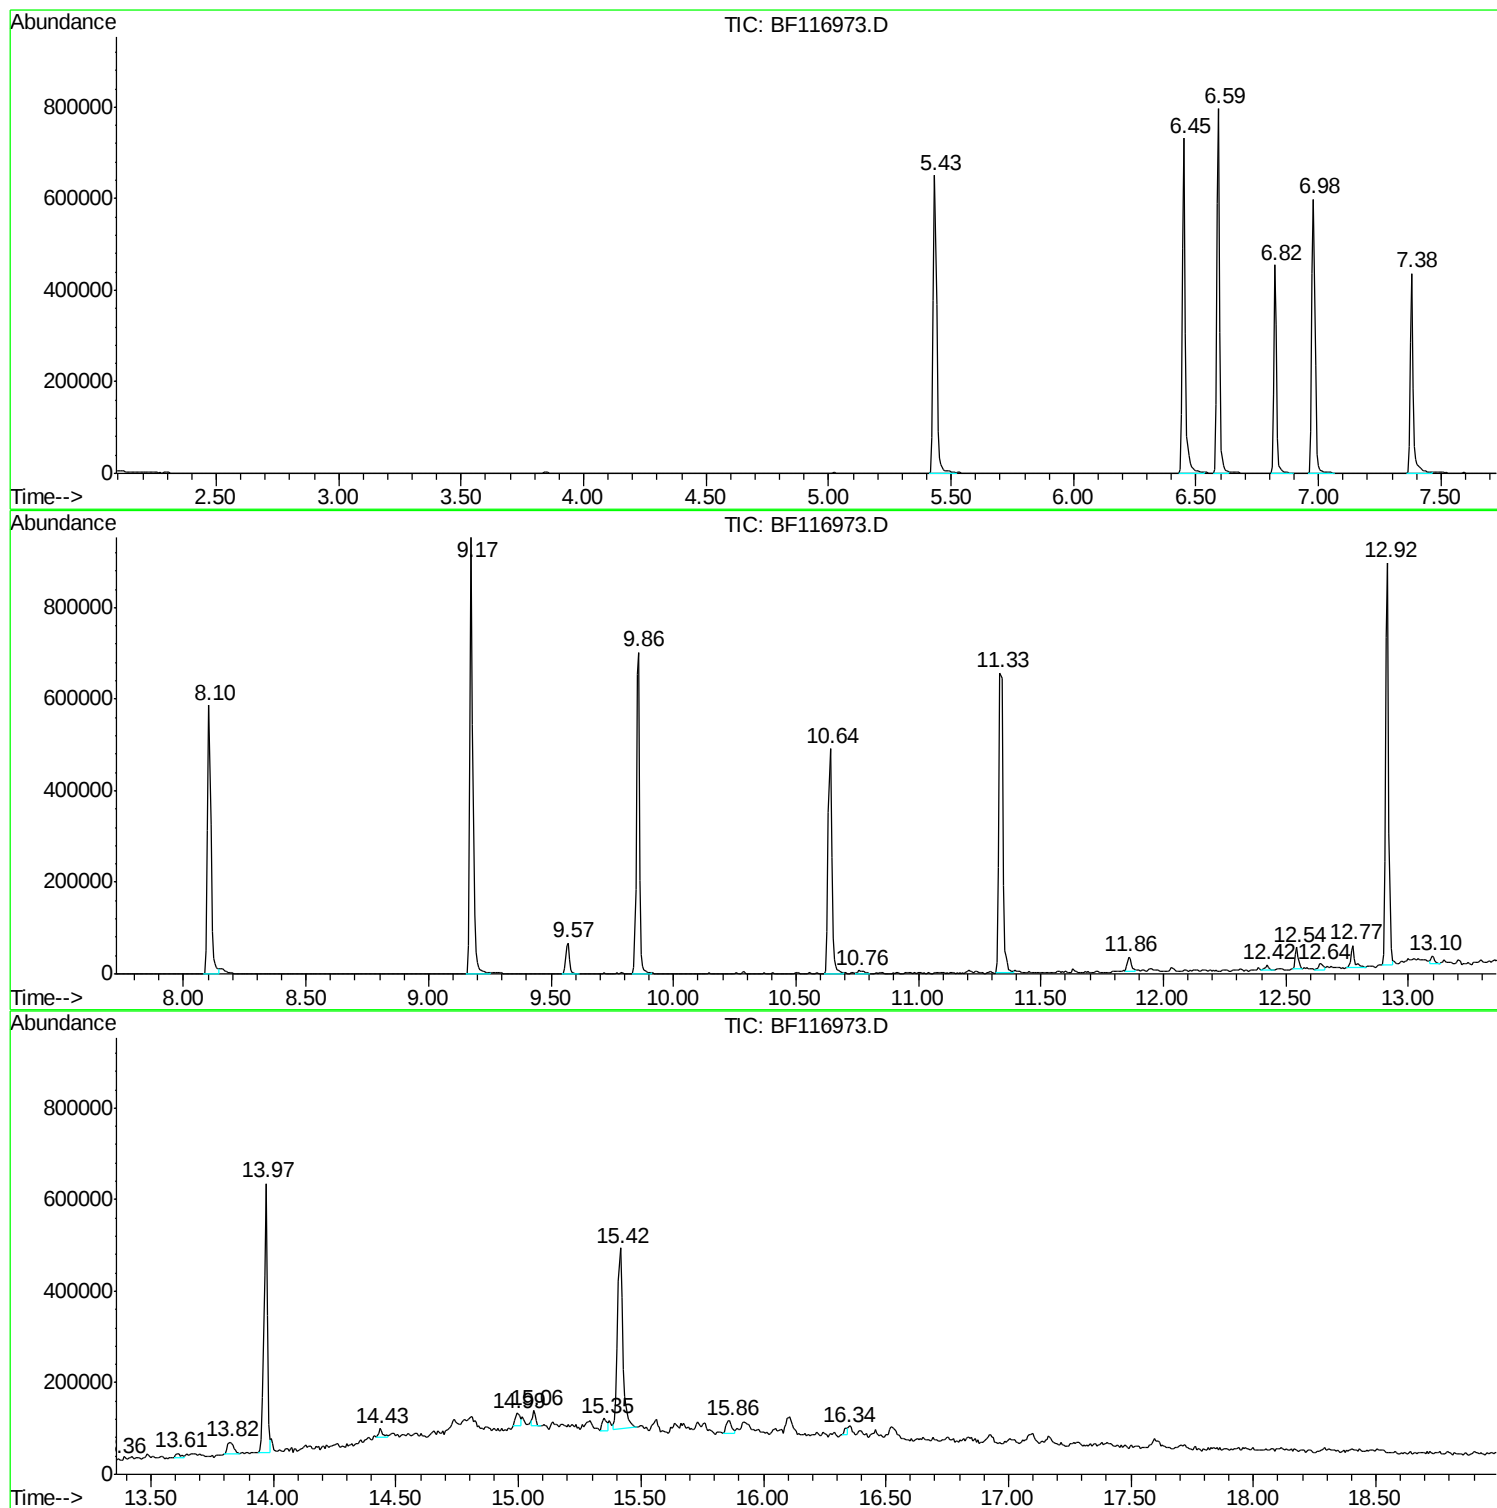

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091119\
Data File : BF116973.D
Acq On : 12 Sep 2019 3:20
Operator : HP/JU
Sample : K4787-01 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-S(1-4)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.59	35.59 ng	681080	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

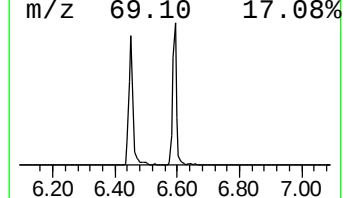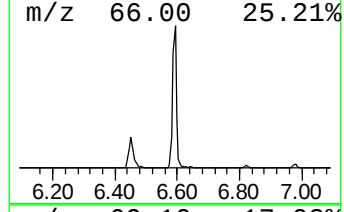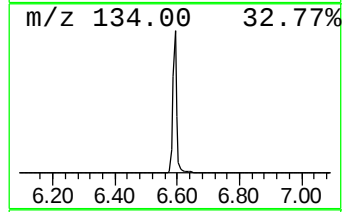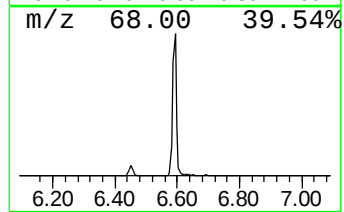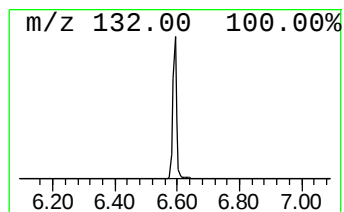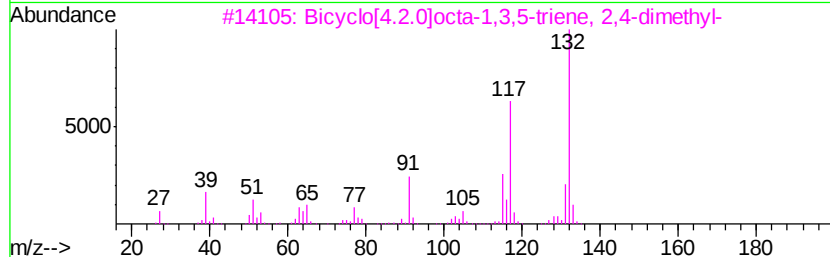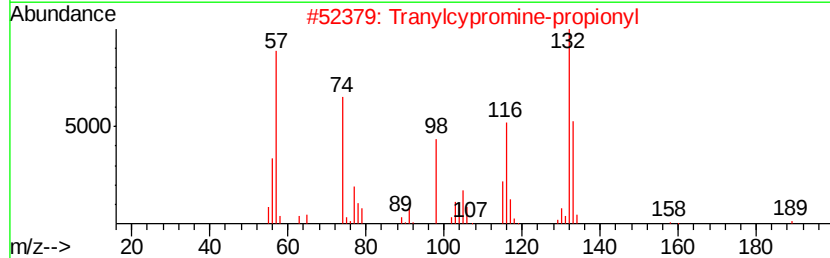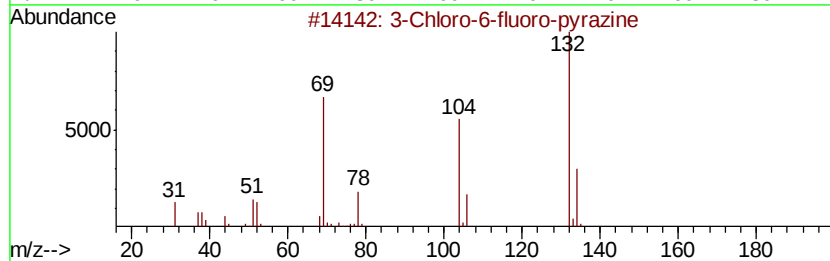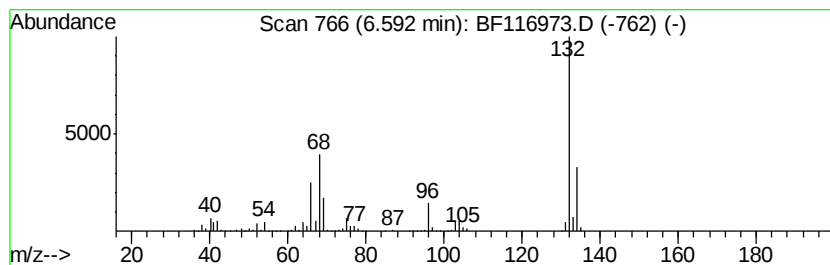

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091119\
Data File : BF116973.D
Acq On : 12 Sep 2019 3:20
Operator : HP/JU
Sample : K4787-01 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-S(1-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.59	6.59	35.6	ng	681080	1	6.82	382715	20.0