


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091119\
 Data File : BF116950.D
 Acq On : 11 Sep 2019 16:34
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 08:24:39 2019

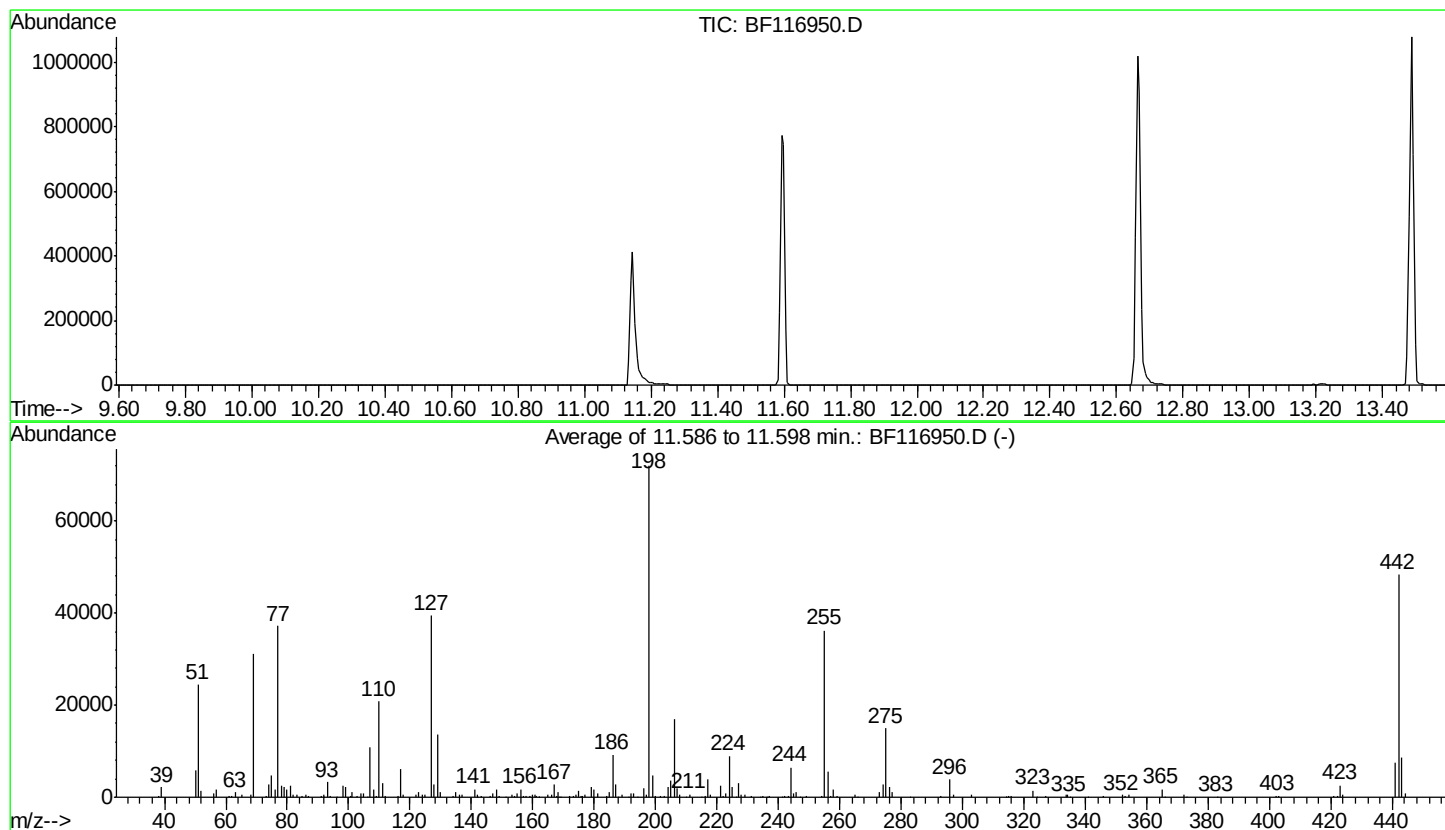

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	24348	PASS
68	69	0.00	2	1.5	473	PASS
69	198	0.00	100	43.3	31189	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.7	39376	PASS
197	198	0.00	2	0.8	574	PASS
198	198	100	100	100.0	72040	PASS
199	198	5	9	6.5	4712	PASS
275	198	10	60	20.7	14908	PASS
365	198	1	100	2.4	1696	PASS
441	198	0.01	100	10.5	7539	PASS
442	198	50	100	67.1	48310	PASS
443	442	15	24	18.1	8724	PASS