


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091119\
 Data File : BF116974.D
 Acq On : 12 Sep 2019 4:40
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 08:24:39 2019

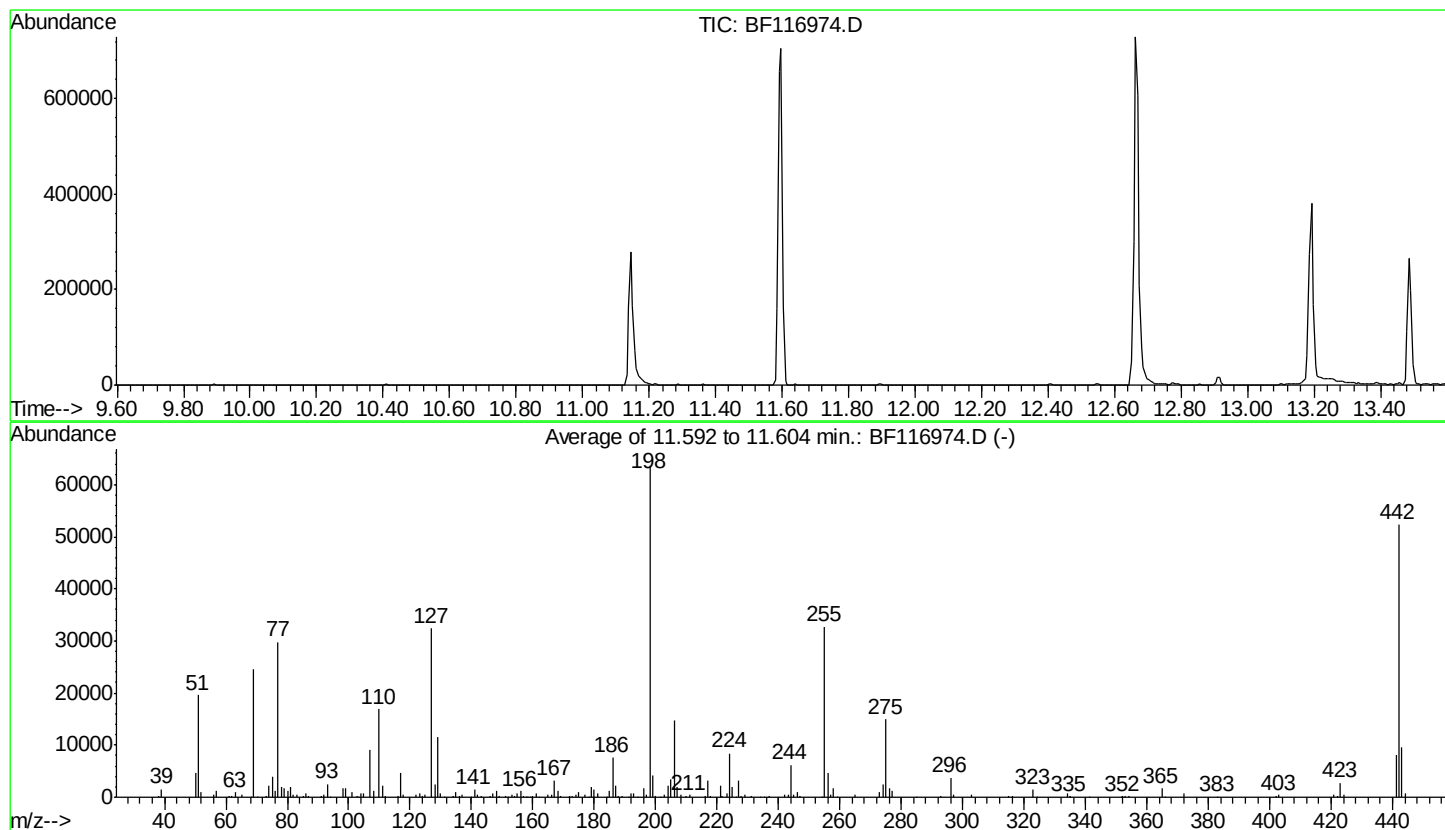

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	19611	PASS
68	69	0.00	2	0.5	130	PASS
69	198	0.00	100	38.6	24556	PASS
70	69	0.00	2	0.5	125	PASS
127	198	10	80	50.9	32411	PASS
197	198	0.00	2	0.7	434	PASS
198	198	100	100	100.0	63642	PASS
199	198	5	9	6.7	4264	PASS
275	198	10	60	23.5	14982	PASS
365	198	1	100	2.6	1654	PASS
441	198	0.01	100	12.9	8189	PASS
442	198	50	100	82.2	52325	PASS
443	442	15	24	18.2	9545	PASS