


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091123\
Data File : BF135158.D
Acq On : 11 Sep 2023 12:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023

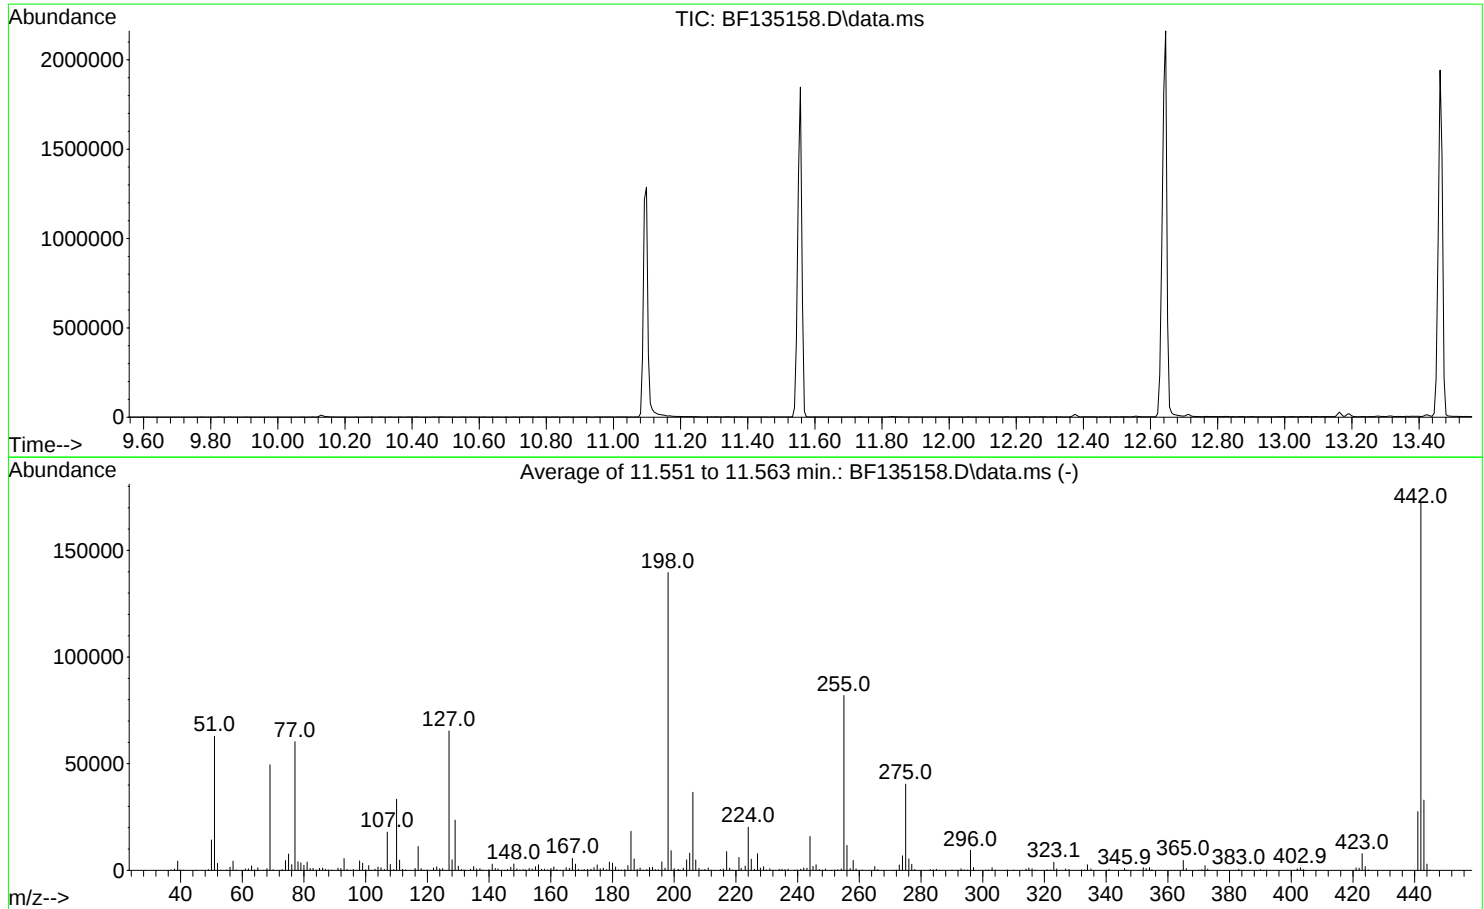




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	62861	PASS
68	69	0.00	2	1.7	837	PASS
69	198	0.00	100	35.5	49551	PASS
70	69	0.00	2	0.6	294	PASS
127	198	10	80	46.8	65333	PASS
197	198	0.00	2	0.8	1065	PASS
198	198	100	100	100.0	139595	PASS
199	198	5	9	6.6	9246	PASS
275	198	10	60	29.0	40445	PASS
365	198	1	100	3.3	4656	PASS
441	198	0.01	100	19.7	27557	PASS
442	442	50	100	100.0	172456	PASS
443	442	15	24	19.1	32955	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091123\
Data File : BF135158.D
Acq On : 11 Sep 2023 12:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 12 04:42:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

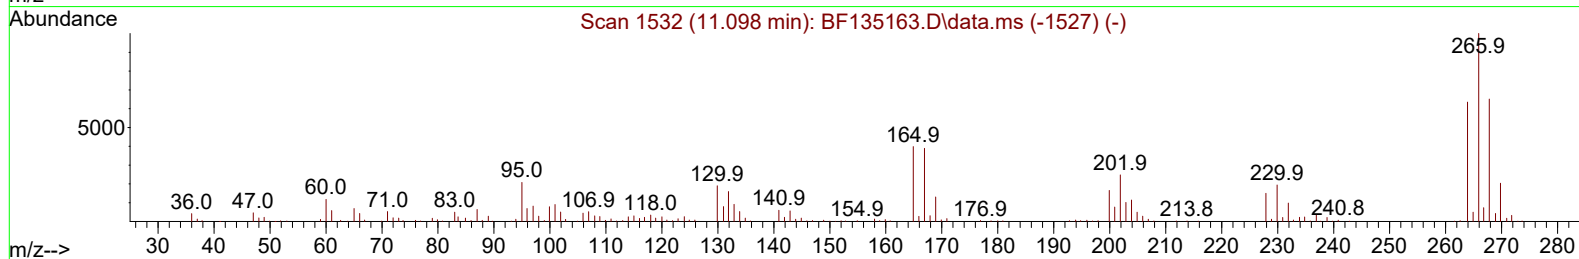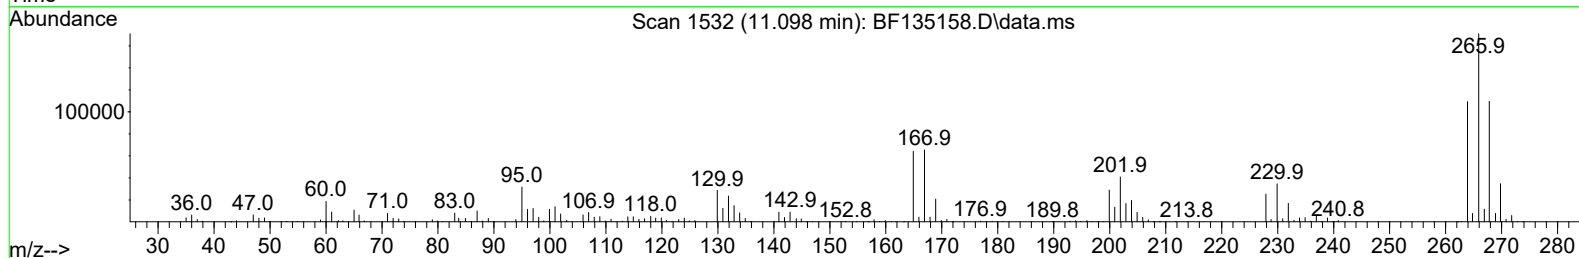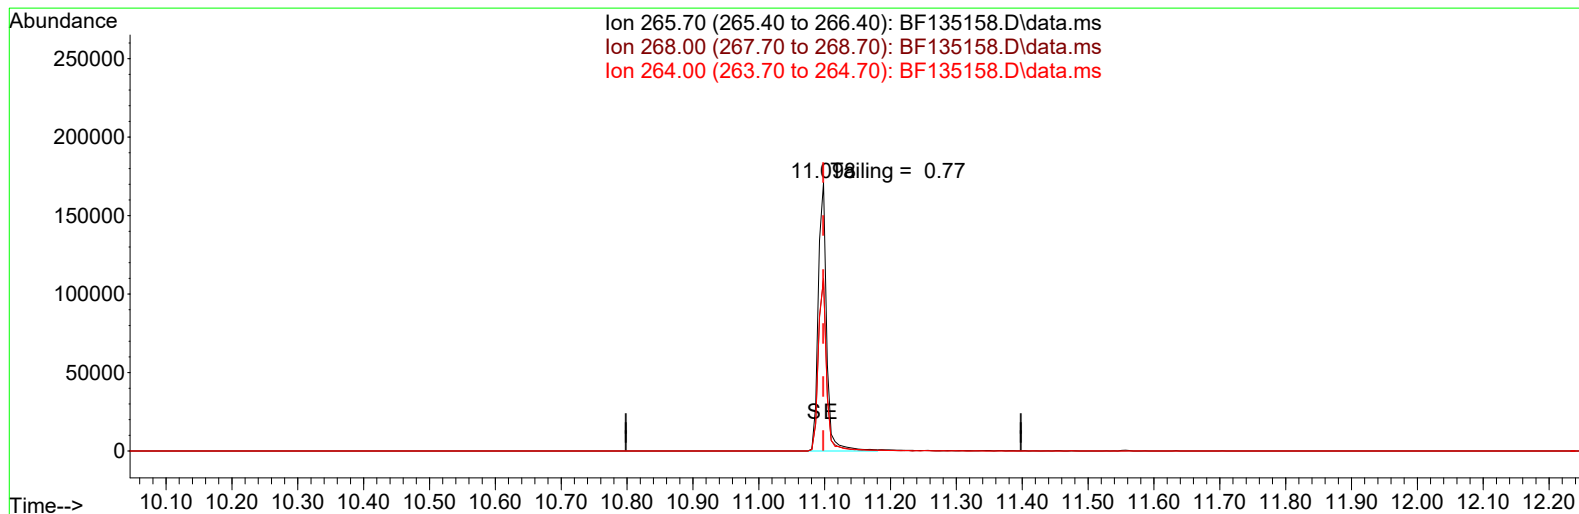

TIC: BF135158.D\data.ms

(70) Pentachlorophenol (C)

11.098min (+ 0.000) 35909.85 ng




response 152603

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.11
264.00	63.50	63.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091123\
Data File : BF135158.D
Acq On : 11 Sep 2023 12:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 12 04:42:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

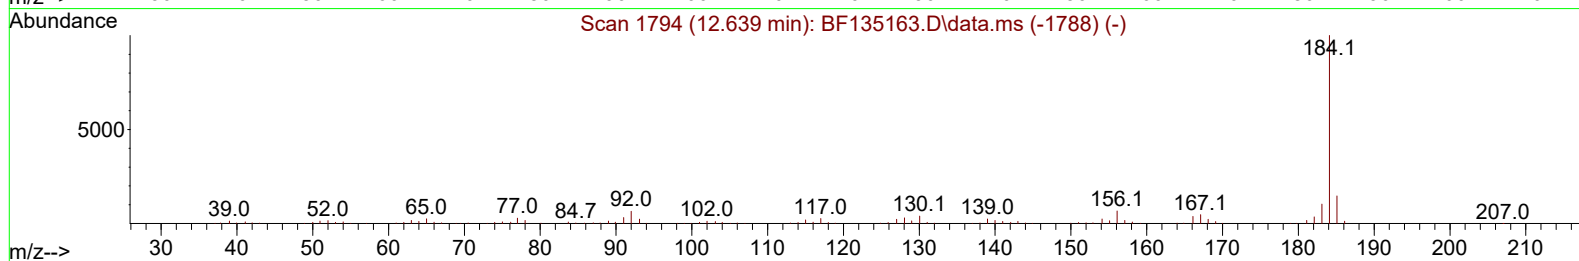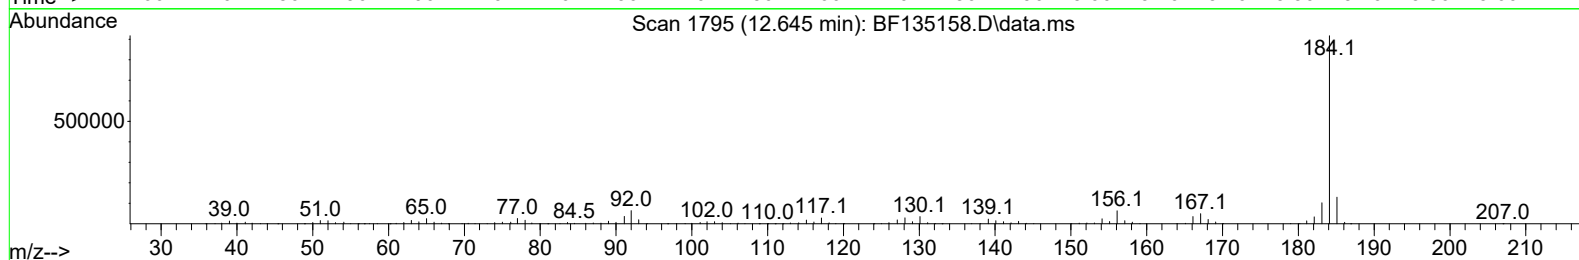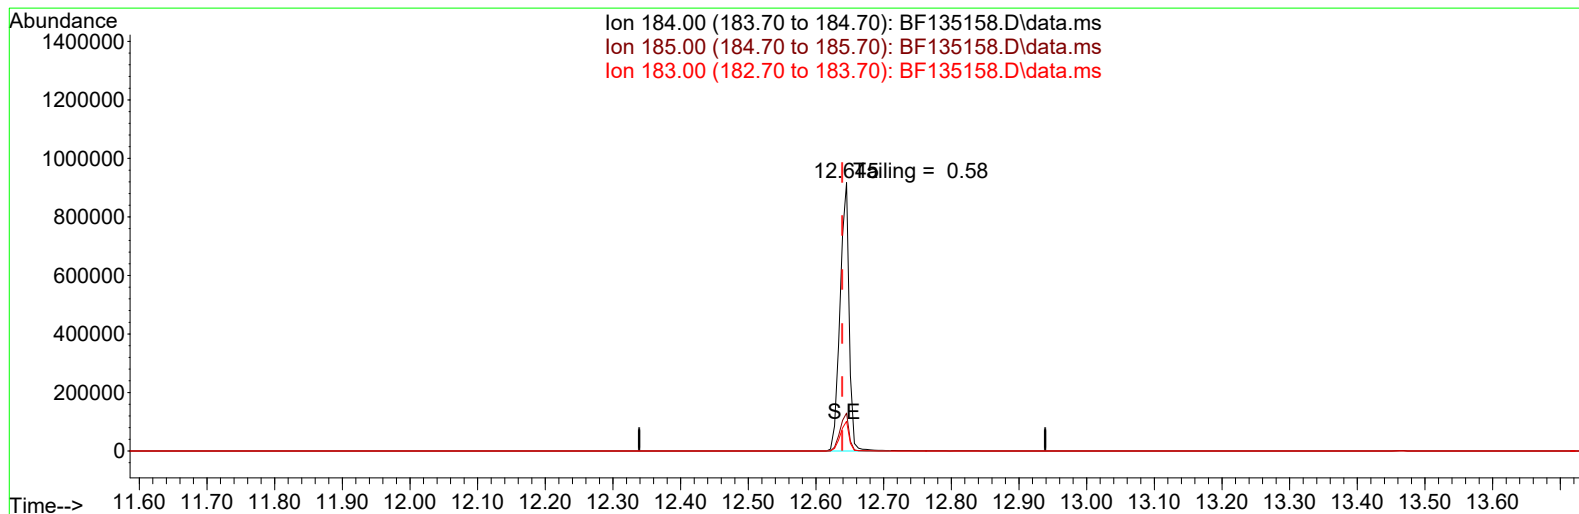

TIC: BF135158.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 0.00 ng

response 859196

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.12
183.00	10.30	11.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/11/2023	BNA_F	<u>BF135158.D</u>
Compound Name	Response	Retention Time
DDT	346703	13.463
DDD	8313	13.163
DDE	230	12.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8543	355246	2.40

Instrument :
BNA_F
ClientSampleId :
DFTPP