
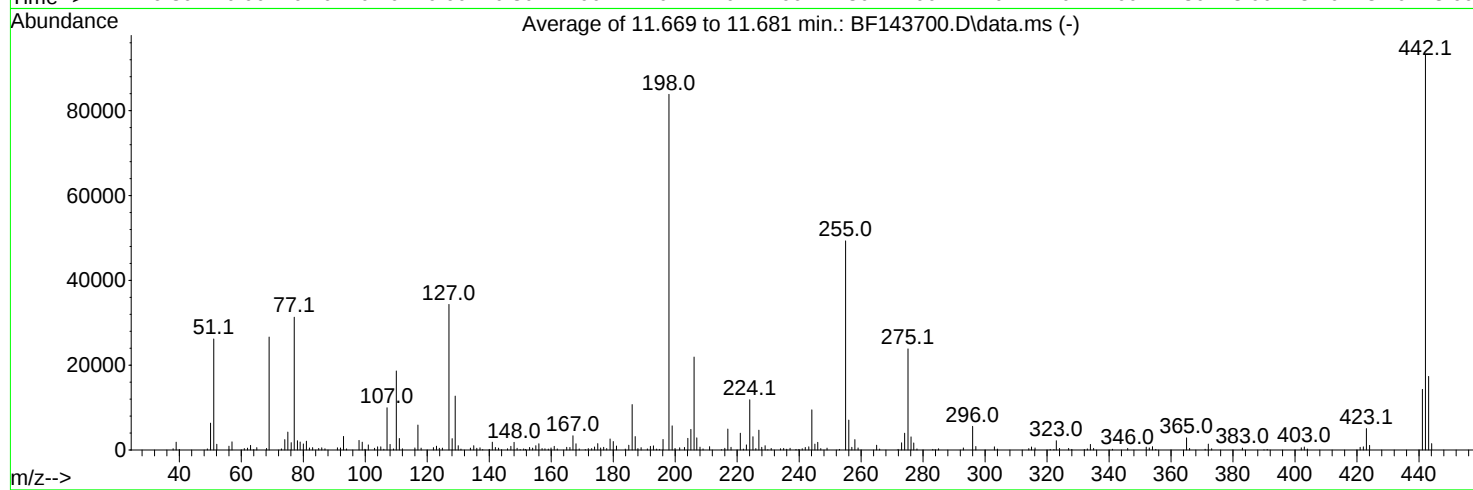


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091125\
Data File : BF143700.D
Acq On : 11 Sep 2025 12:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 09 15:20:16 2025

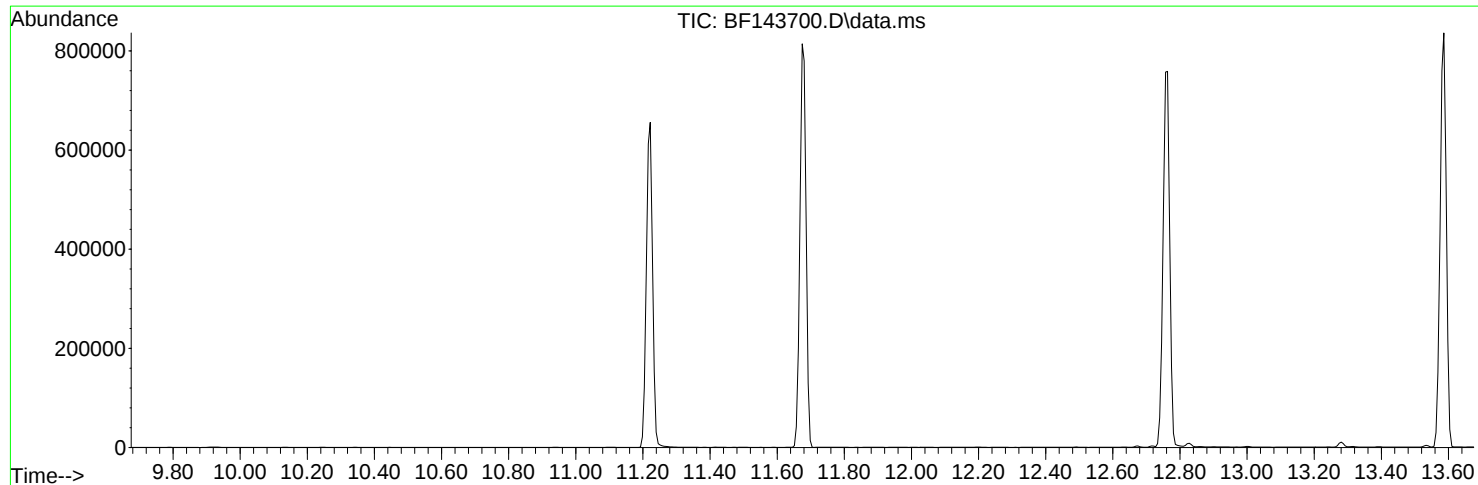




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.4	362	PASS
69	69	100	100	100.0	26608	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83875	PASS
199	198	5	9	6.8	5678	PASS
365	198	1	100	3.4	2857	PASS
441	443	0.01	150	82.4	14302	PASS
442	442	100	100	100.0	93117	PASS
443	442	15	24	18.6	17357	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091125\
Data File : BF143700.D
Acq On : 11 Sep 2025 12:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 11 12:26:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

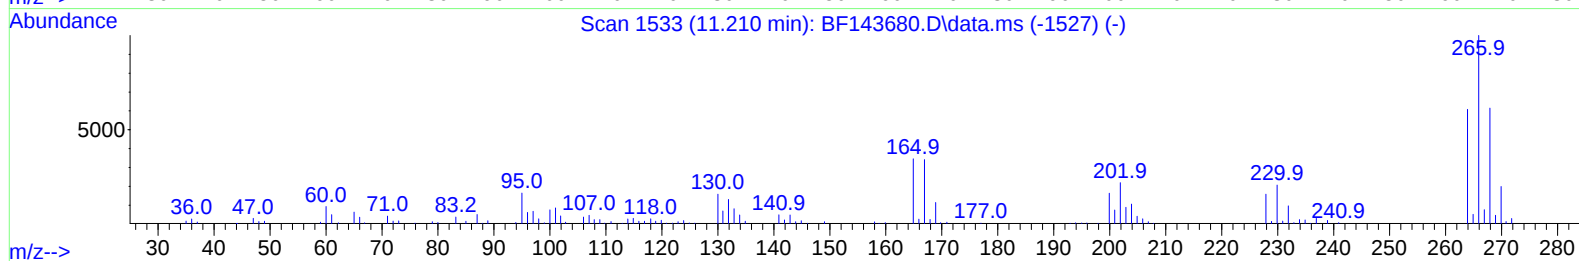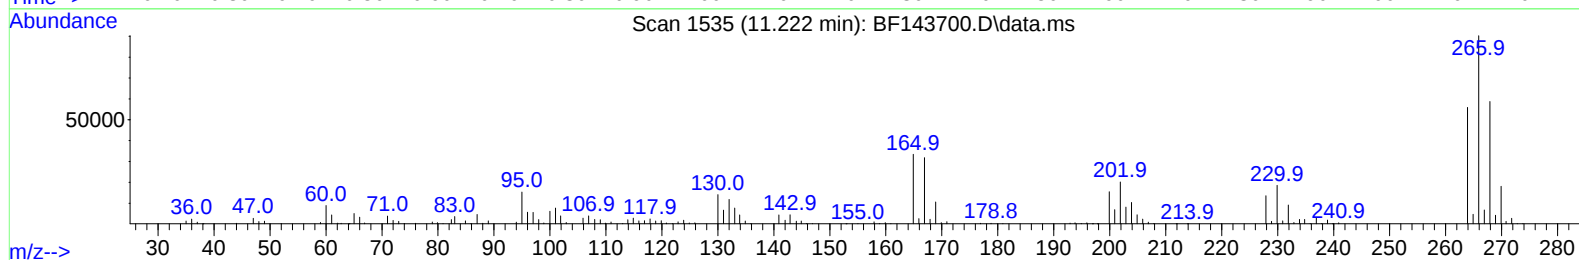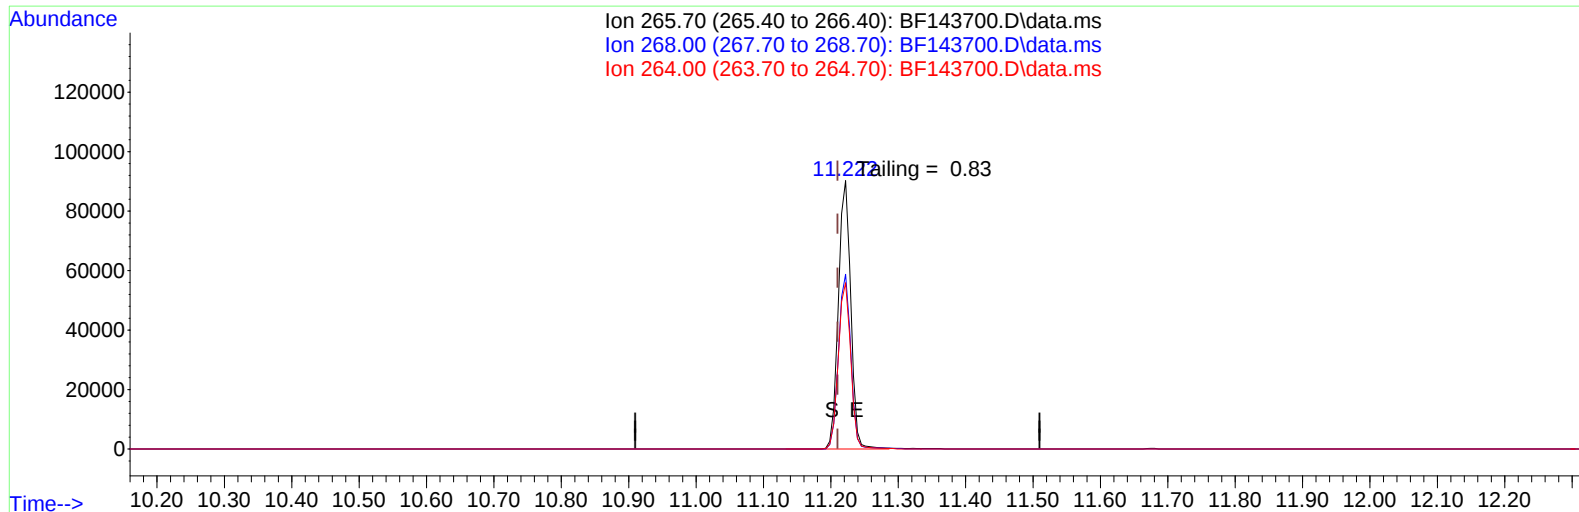

TIC: BF143700.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.012) 34491.78 ng




response 115489

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	65.12
264.00	60.80	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091125\
Data File : BF143700.D
Acq On : 11 Sep 2025 12:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 11 12:26:05 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

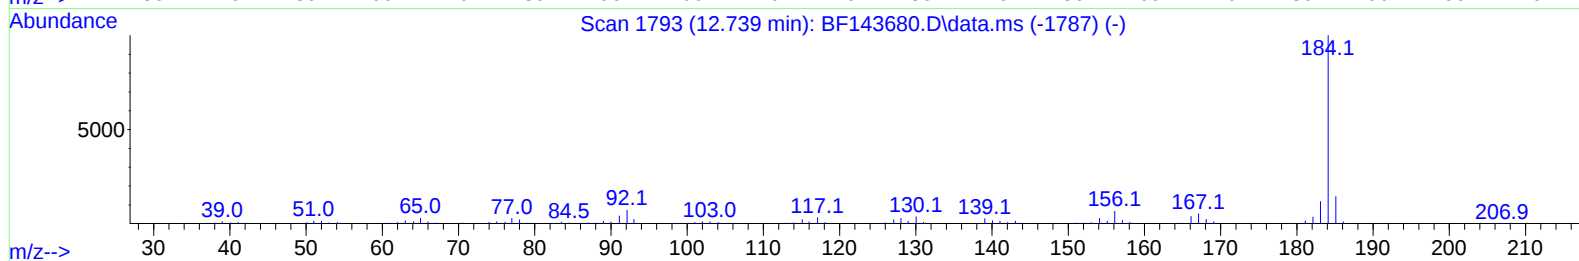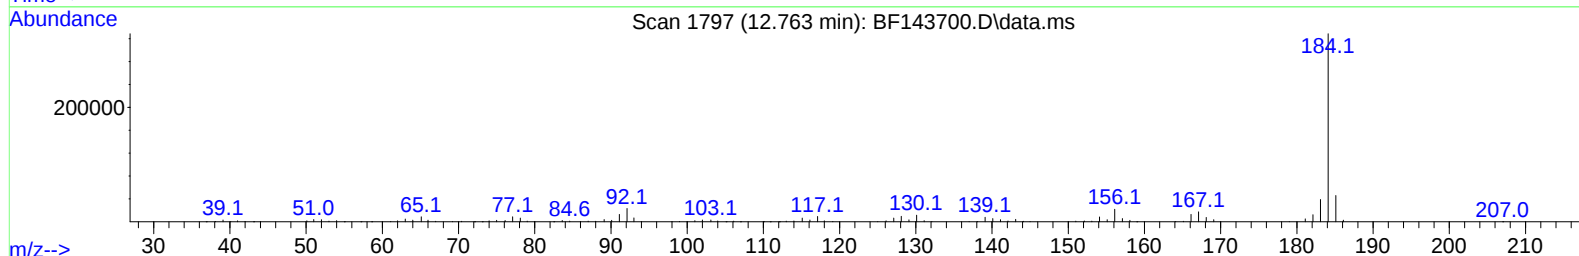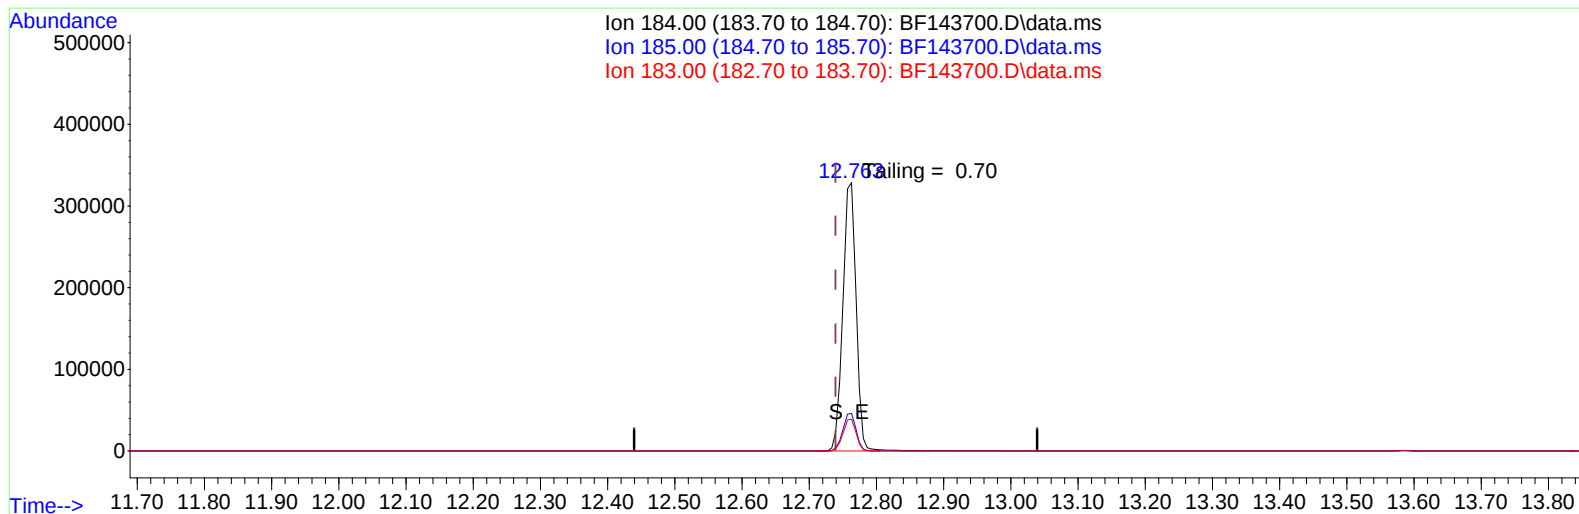

TIC: BF143700.D\data.ms

(77) Benzidine

12.763min (+ 0.024) 67634.26 ng

response 452138

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.01
183.00	11.80	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/11/2025	BNA_F	<u>BF143700.D</u>
Compound Name	Response	Retention Time
DDT	221498	13.568
DDD	4189	13.28
DDE	58	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4247	225745	1.88

Instrument :
BNA_F
ClientSampleId :
DFTPP