


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091218\
Data File : BF108948.D
Acq On : 12 Sep 2018 13:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 05 18:03:31 2018

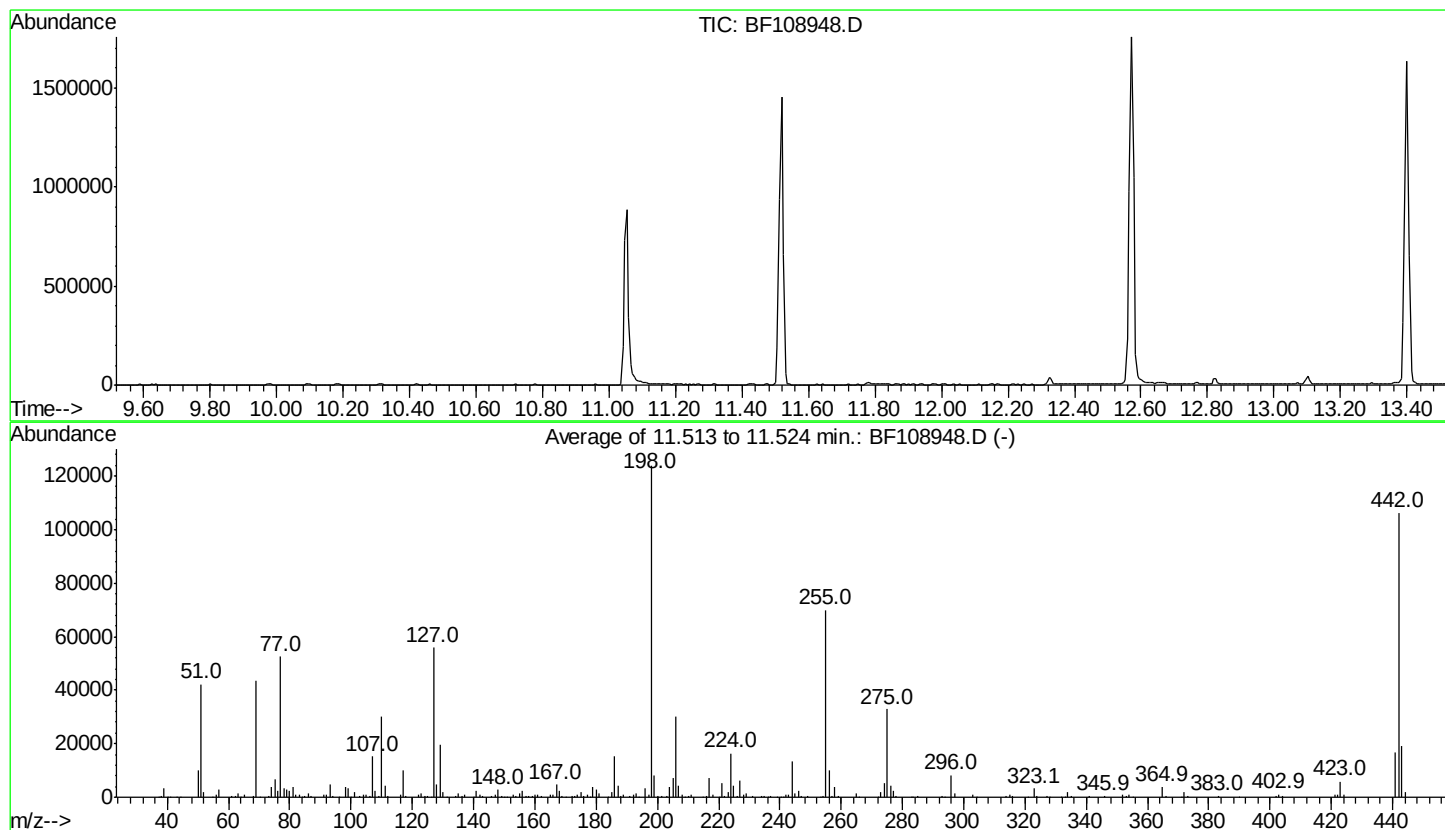

AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	42230	PASS
68	69	0.00	2	1.7	721	PASS
69	198	0.00	100	35.0	43405	PASS
70	69	0.00	2	0.2	103	PASS
127	198	10	80	45.1	55882	PASS
197	198	0.00	2	0.7	874	PASS
198	198	100	100	100.0	123861	PASS
199	198	5	9	6.5	8040	PASS
275	198	10	60	26.5	32829	PASS
365	198	1	100	3.2	4013	PASS
441	198	0.01	100	13.4	16551	PASS
442	198	50	100	85.8	106320	PASS
443	442	15	24	18.1	19199	PASS