
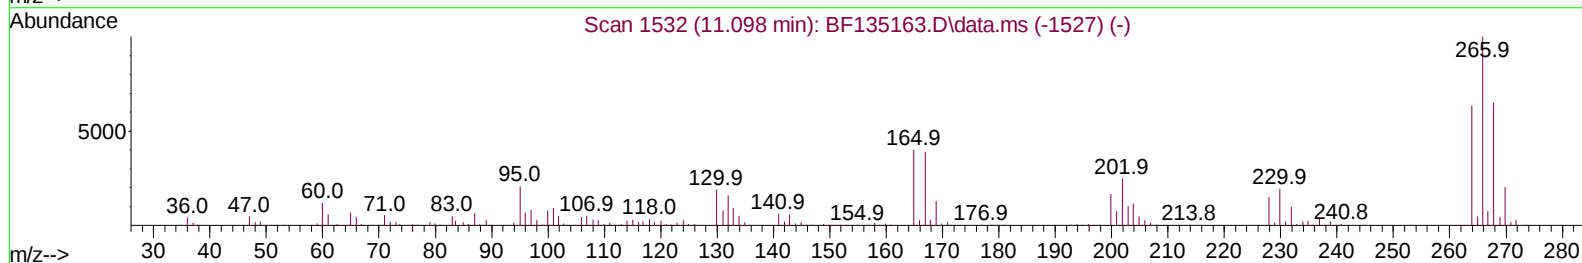
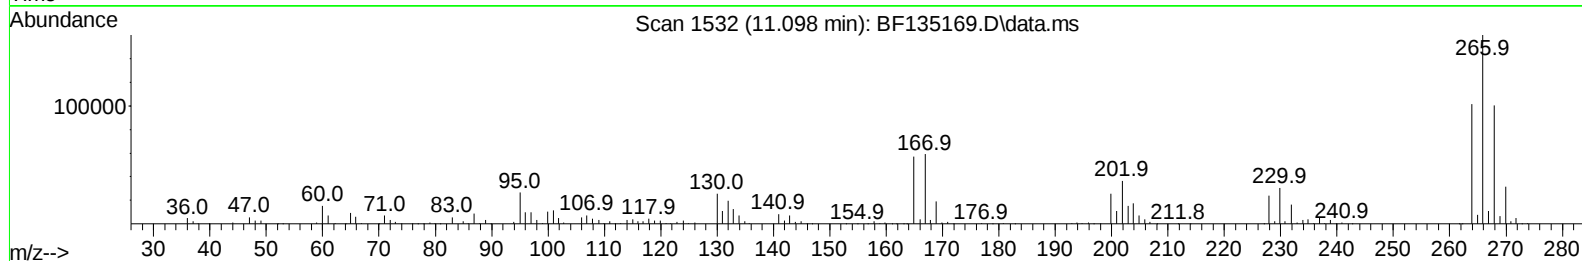


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135169.D
Acq On : 12 Sep 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 05:54:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

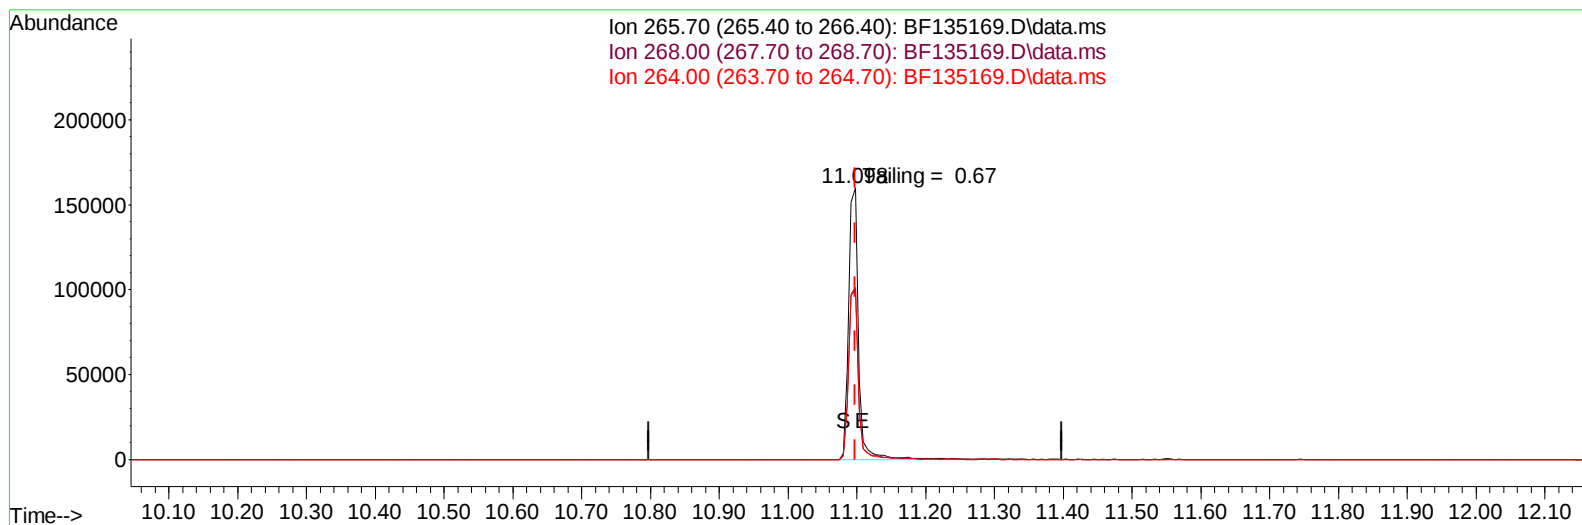




TIC: BF135169.D\data.ms

(70) Pentachlorophenol (C)**11.098min (+ 0.000) 46033.94 ng****response 156557**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	62.78
264.00	63.50	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135169.D
Acq On : 12 Sep 2023 08:10
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 05:54:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

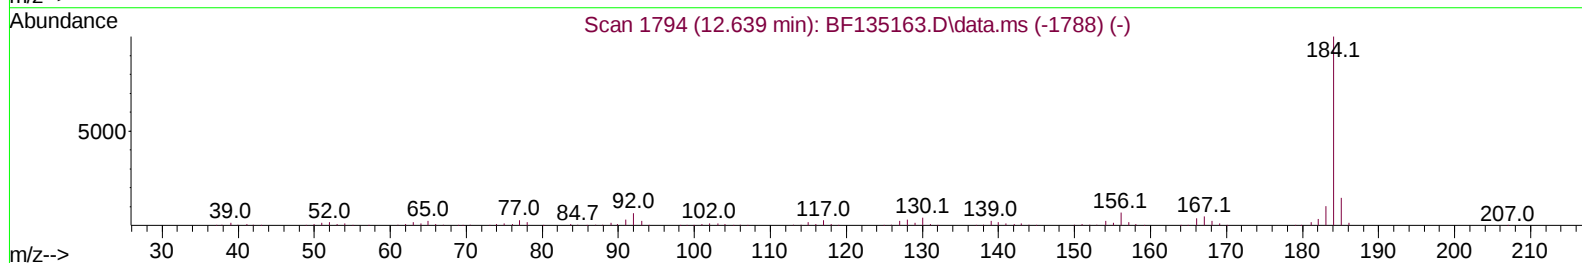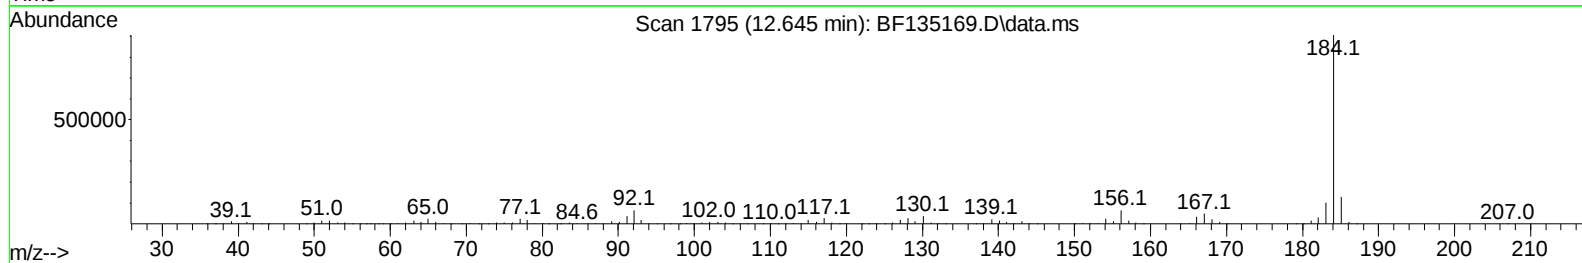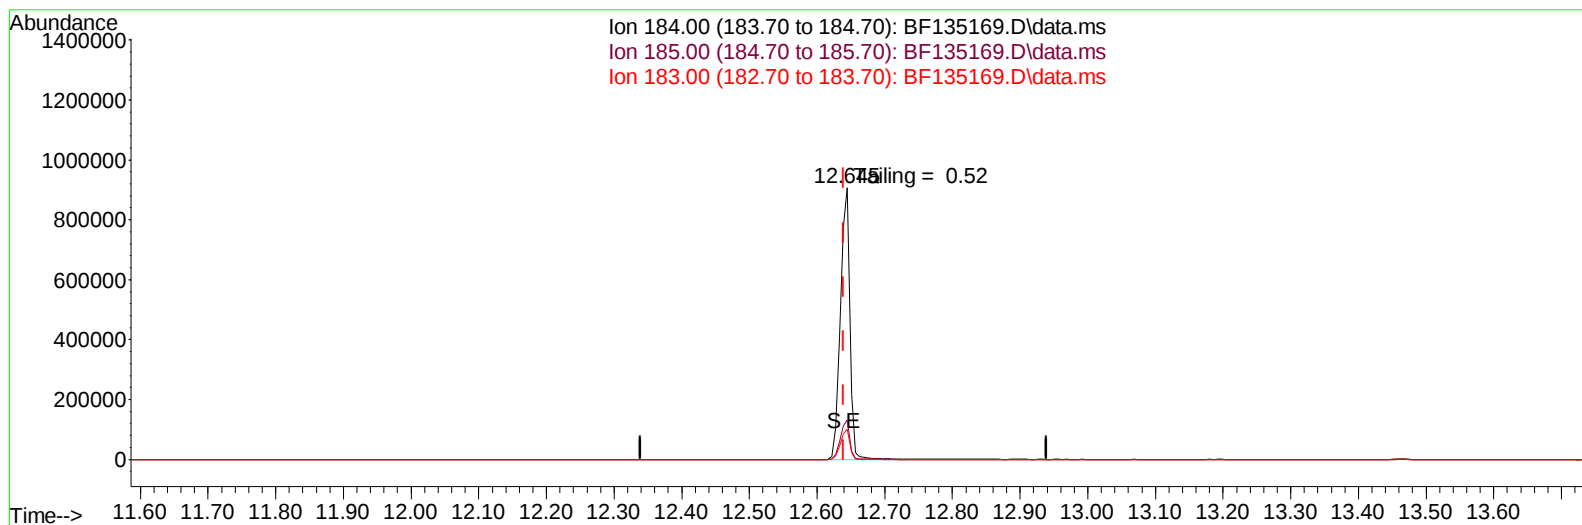

TIC: BF135169.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 0.00 ng

response 878423

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.41
183.00	10.30	11.26
0.00	0.00	0.00