

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
 Data File : BF135171.D
 Acq On : 12 Sep 2023 09:24
 Operator : CG\JU
 Sample : PB155443BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155443BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135171.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	9	13	20	rVB	49525	63123	1.81%	0.264%
2	5.016	492	498	512	rBV	72833	105329	3.02%	0.441%
3	5.398	558	563	566	rBV	2932216	3095116	88.63%	12.952%
4	6.404	728	734	737	rBV	2805095	3130057	89.63%	13.099%
5	6.763	791	795	806	rVB	1046277	837900	23.99%	3.506%
6	7.328	885	891	894	rBV	2068330	2040354	58.42%	8.538%
7	8.039	1008	1012	1016	rBV	1258460	1108682	31.75%	4.640%
8	9.122	1190	1196	1199	rBV	3732698	3457667	99.01%	14.470%
9	9.798	1306	1311	1314	rBV	1501532	1240591	35.52%	5.192%
10	10.592	1441	1446	1449	rBV	2331725	2187620	62.64%	9.155%
11	11.286	1561	1564	1568	rBV	1369063	1309456	37.50%	5.480%
12	12.892	1832	1837	1840	rBV	3529403	3492344	100.00%	14.615%
13	13.945	2012	2016	2019	rBV	1057070	952392	27.27%	3.986%
14	15.404	2259	2264	2278	rVB	631452	796109	22.80%	3.332%
15	16.998	2527	2535	2548	rBV8	18422	79272	2.27%	0.332%




Sum of corrected areas: 23896012

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135171.D
Acq On : 12 Sep 2023 09:24
Operator : CG\JU
Sample : PB155443BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155443BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

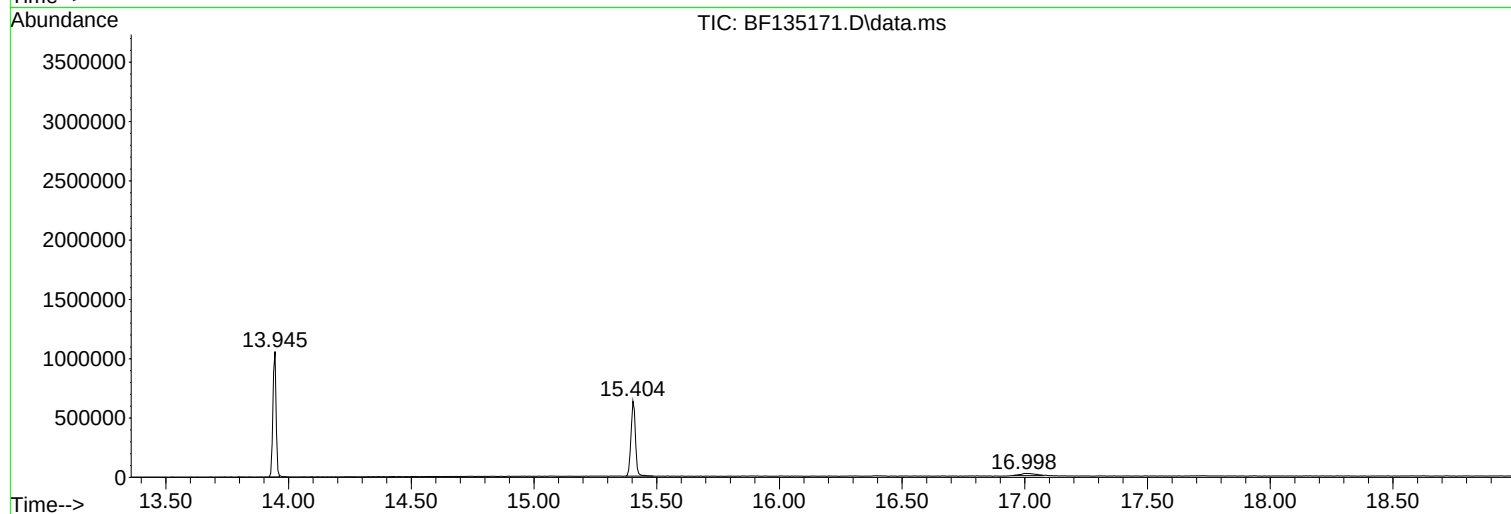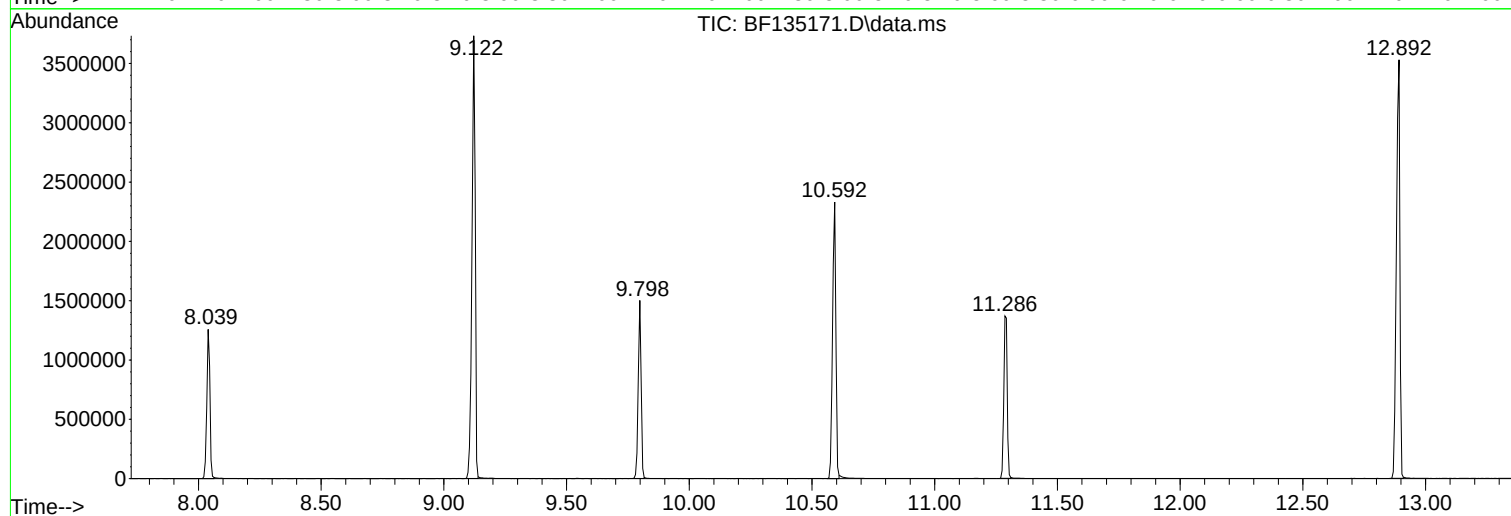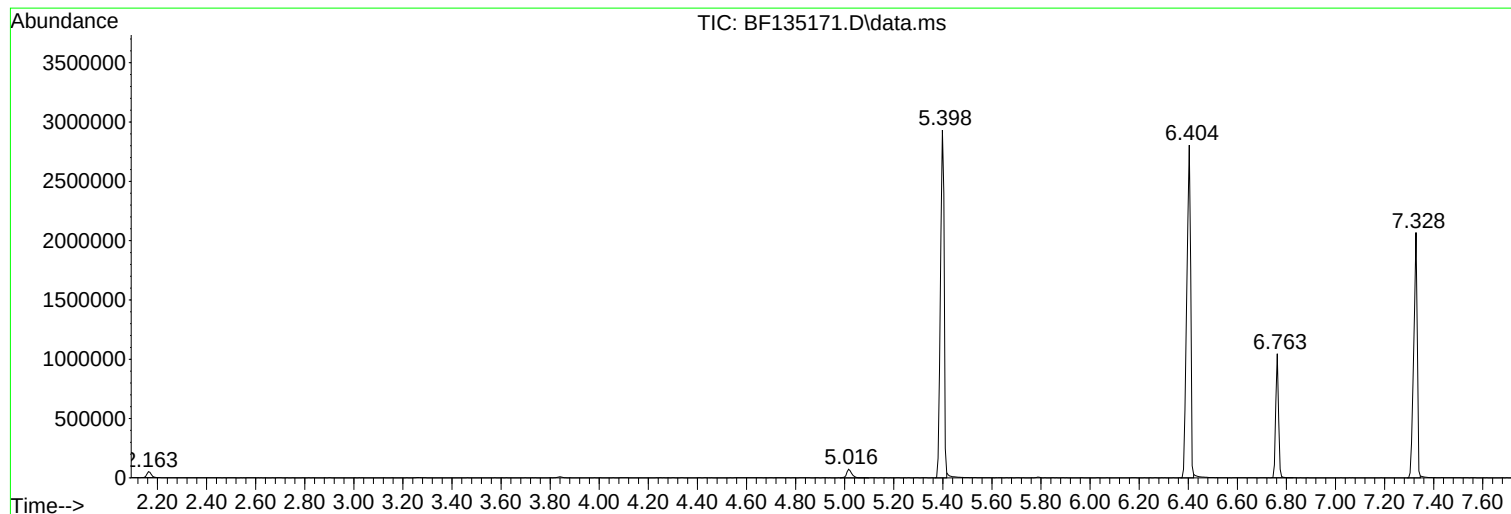

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135171.D
Acq On : 12 Sep 2023 09:24
Operator : CG\JU
Sample : PB155443BL
Misc :
ALS Vial : 3 Sample Multiplier: 1









Instrument :
BNA_F
ClientSampleId :
PB155443BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.016	2.51 ng	105329	1,4-Dichlorobenzene-d4			6.763
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	64
2	2-Hexanol, 2-methyl-		116	C7H16O	000625-23-0	40
3	Propane, 2-methyl-2-(1-methyleth...		116	C7H16O	017348-59-3	40
4	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
5	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	9

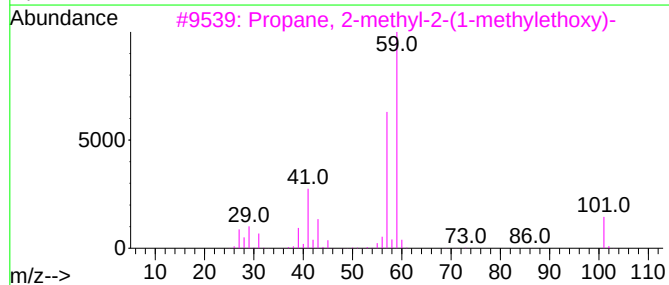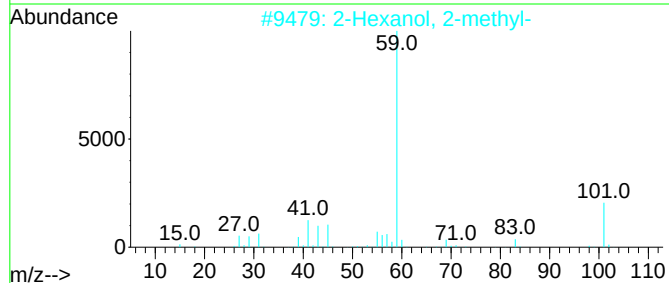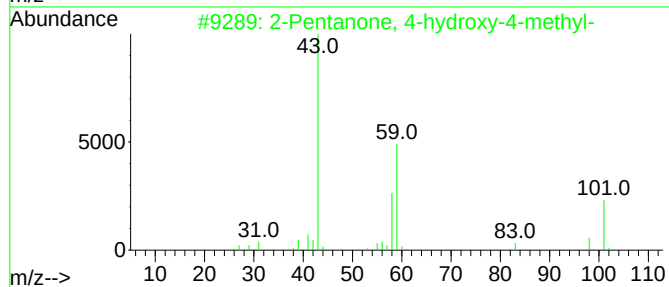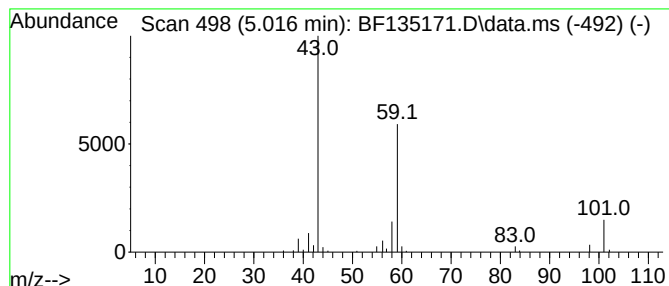

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135171.D
Acq On : 12 Sep 2023 09:24
Operator : CG\JU
Sample : PB155443BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155443BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.016	2.5	ng	105329	1	6.763	837900	20.0