

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
 Data File : BF135172.D
 Acq On : 12 Sep 2023 09:56
 Operator : CG\JU
 Sample : PB155351TB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155351TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	10	15	22	rVB	53028	72119	1.88%	0.281%
2	5.022	495	499	509	rVB	79667	114136	2.97%	0.445%
3	5.404	558	564	567	rBV	3096447	3390639	88.27%	13.232%
4	6.404	728	734	737	rBV	2919322	3423190	89.12%	13.359%
5	6.763	791	795	798	rBV	1040111	838275	21.82%	3.271%
6	7.328	885	891	894	rBV	2154866	2226933	57.98%	8.691%
7	8.039	1008	1012	1016	rBV	1279944	1123611	29.25%	4.385%
8	9.122	1190	1196	1199	rBV	3908658	3841145	100.00%	14.990%
9	9.798	1306	1311	1314	rBV	1549237	1306215	34.01%	5.098%
10	10.592	1441	1446	1449	rBV	2558720	2444577	63.64%	9.540%
11	11.292	1561	1565	1568	rBV	1484045	1355315	35.28%	5.289%
12	12.892	1831	1837	1840	rBV	3806585	3767314	98.08%	14.702%
13	13.945	2011	2016	2019	rBV	1043207	952984	24.81%	3.719%
14	15.404	2259	2264	2270	rBV	617726	767584	19.98%	2.996%




Sum of corrected areas: 25624037

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135172.D
Acq On : 12 Sep 2023 09:56
Operator : CG\JU
Sample : PB155351TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155351TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

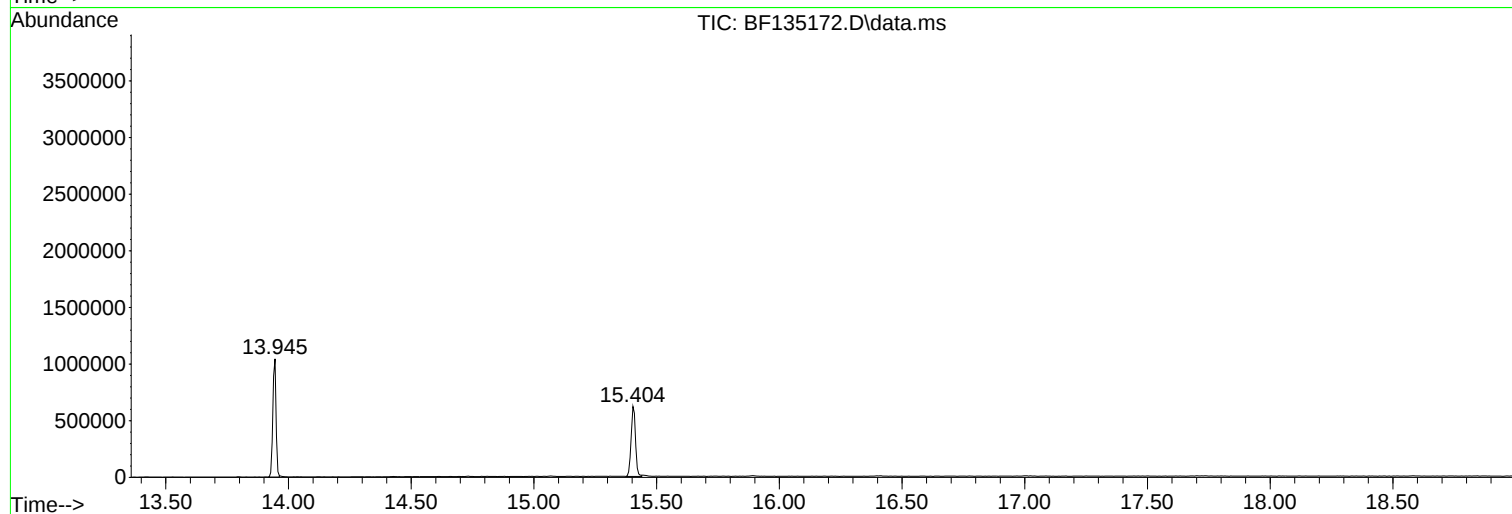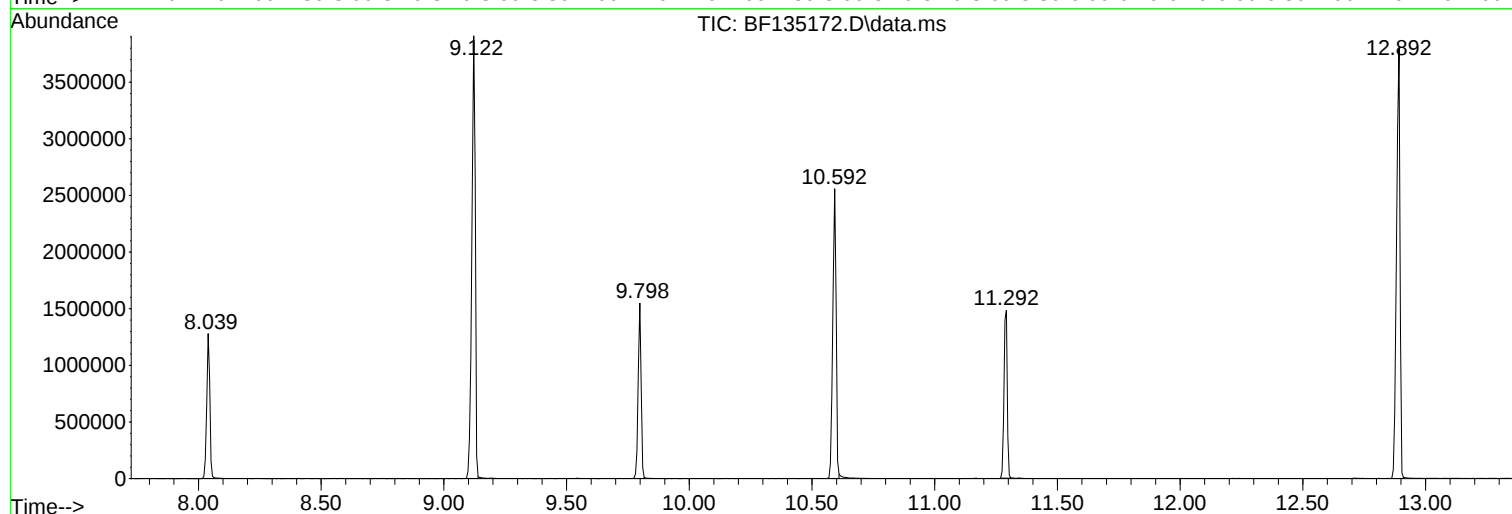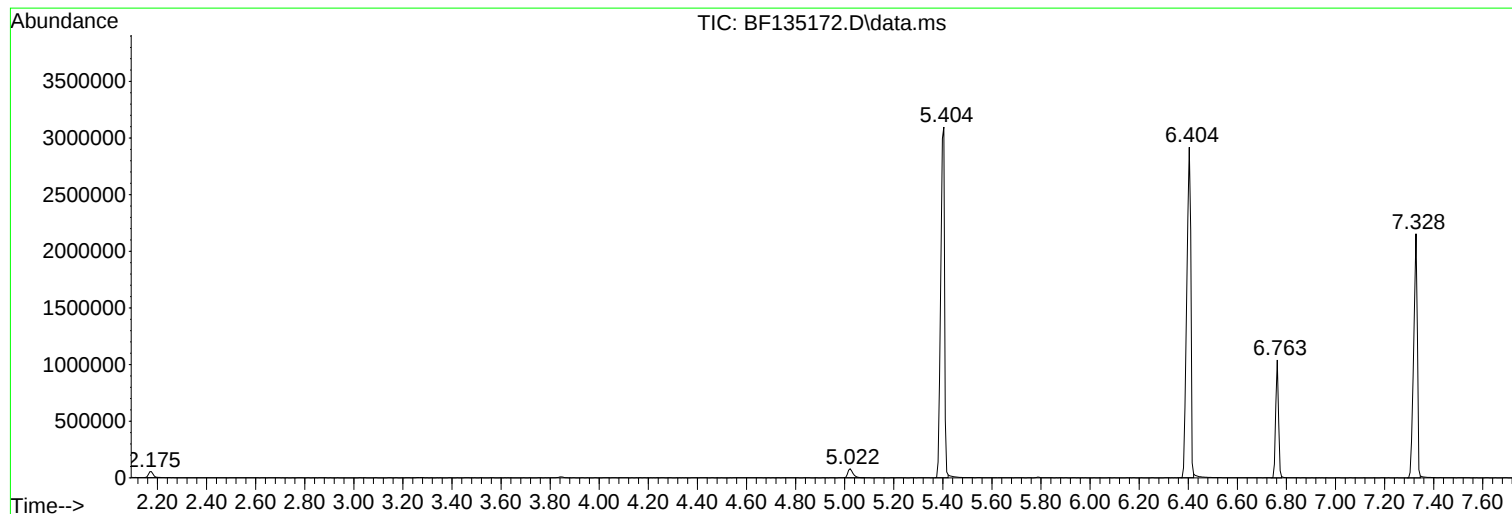

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135172.D
Acq On : 12 Sep 2023 09:56
Operator : CG\JU
Sample : PB155351TB
Misc :
ALS Vial : 4 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB155351TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.022	2.72 ng	114136	1,4-Dichlorobenzene-d4			6.763
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	50
2	Propane, 2-methyl-2-(1-methyleth...		116	C7H16O	017348-59-3	42
3	3-Hexanol, 4-methyl-		116	C7H16O	000615-29-2	33
4	2-Hexanol, 2-methyl-		116	C7H16O	000625-23-0	28
5	3-Octanol		130	C8H18O	000589-98-0	28

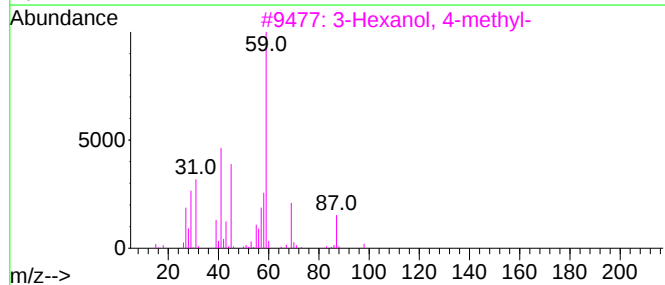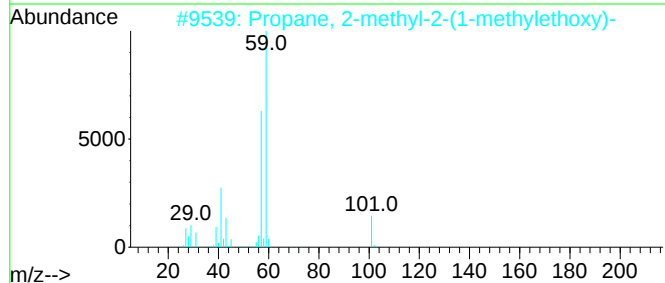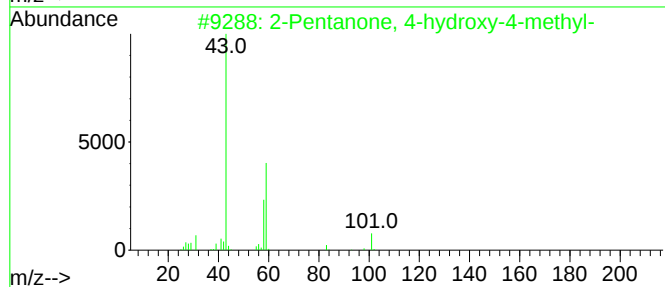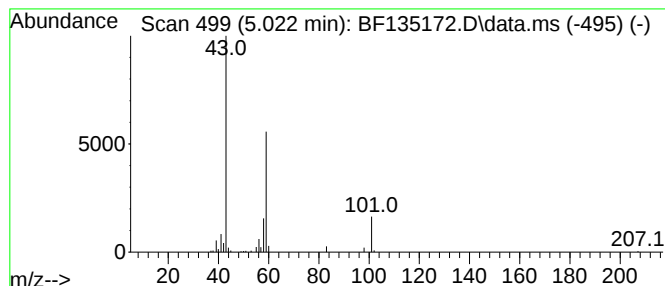

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135172.D
Acq On : 12 Sep 2023 09:56
Operator : CG\JU
Sample : PB155351TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155351TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.022	2.7	ng	114136	1	6.763	838275	20.0