

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
 Data File : BF135175.D
 Acq On : 12 Sep 2023 11:32
 Operator : CG\JU
 Sample : PB155416TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155416TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.158	8	12	21	rVB	45734	61116	1.80%	0.266%
2	5.010	492	497	507	rBV	66149	99396	2.93%	0.432%
3	5.398	558	563	566	rBV	2965747	2960131	87.37%	12.866%
4	6.404	729	734	737	rBV	2736538	2962460	87.43%	12.876%
5	6.763	791	795	803	rBV	993029	815308	24.06%	3.544%
6	7.328	886	891	894	rBV	2018531	1931057	56.99%	8.393%
7	8.039	1008	1012	1016	rBV	1243756	1084457	32.01%	4.713%
8	9.122	1190	1196	1199	rBV	3561904	3388200	100.00%	14.726%
9	9.798	1305	1311	1314	rBV	1530283	1222463	36.08%	5.313%
10	10.592	1441	1446	1449	rBV	2323794	2091765	61.74%	9.091%
11	11.292	1561	1565	1568	rBV	1445012	1328038	39.20%	5.772%
12	12.892	1832	1837	1840	rBV	3327092	3373898	99.58%	14.664%
13	13.945	2011	2016	2019	rBV	950667	932660	27.53%	4.054%
14	15.404	2259	2264	2270	rBV	610477	757119	22.35%	3.291%




Sum of corrected areas: 23008068

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135175.D
Acq On : 12 Sep 2023 11:32
Operator : CG\JU
Sample : PB155416TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155416TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

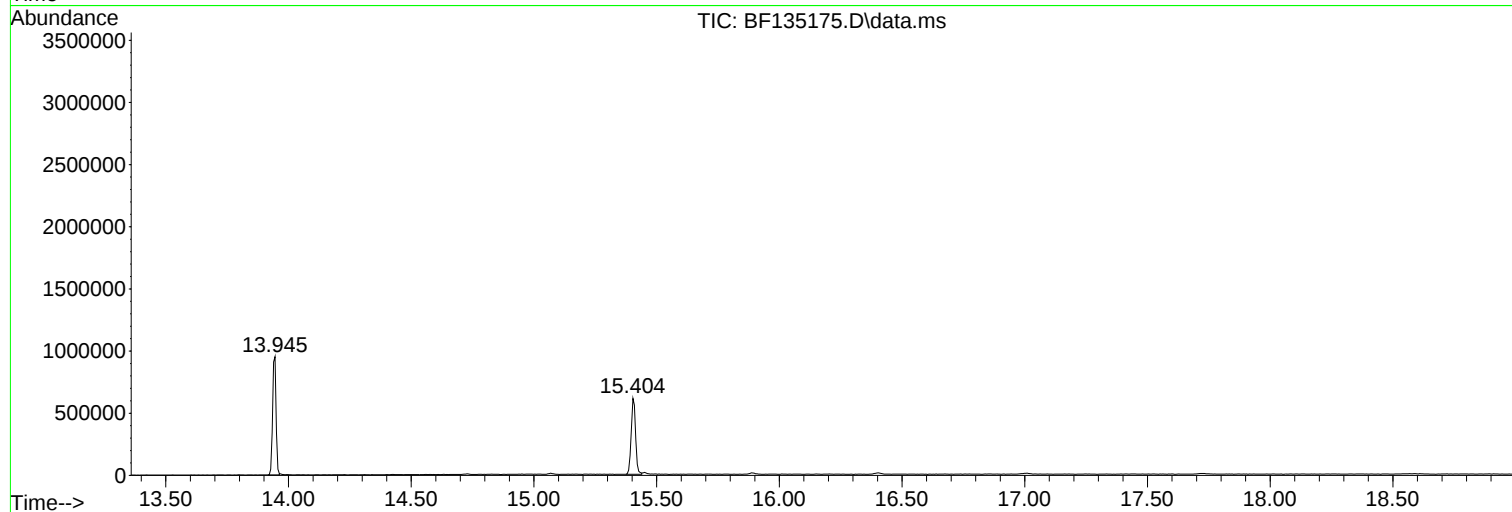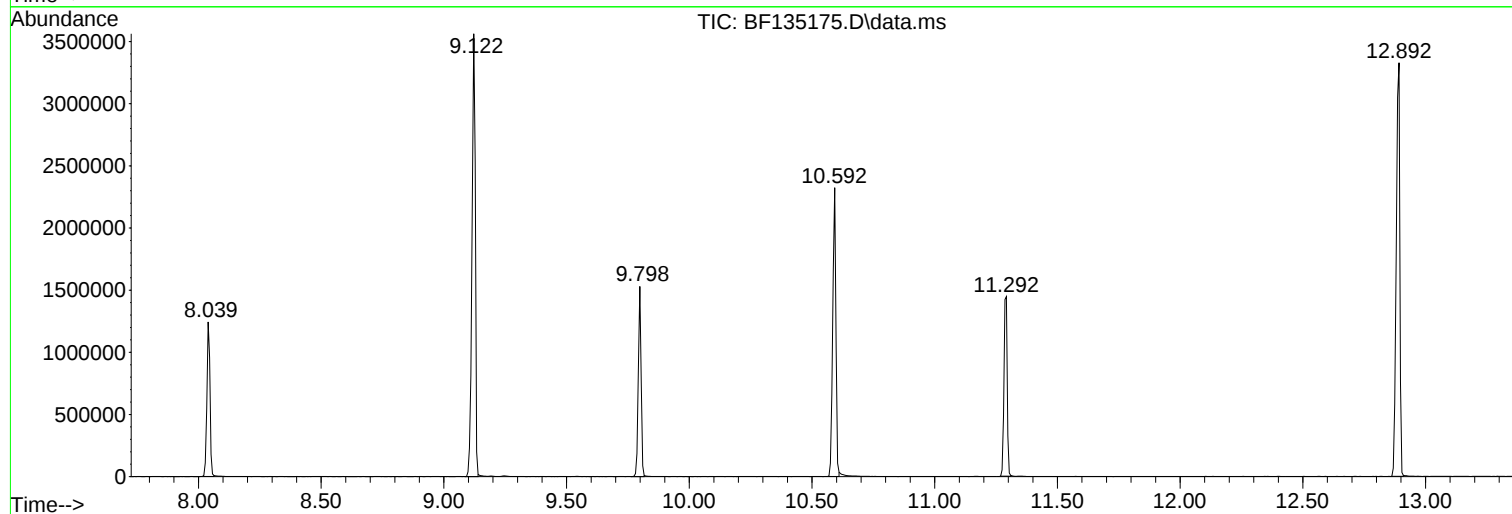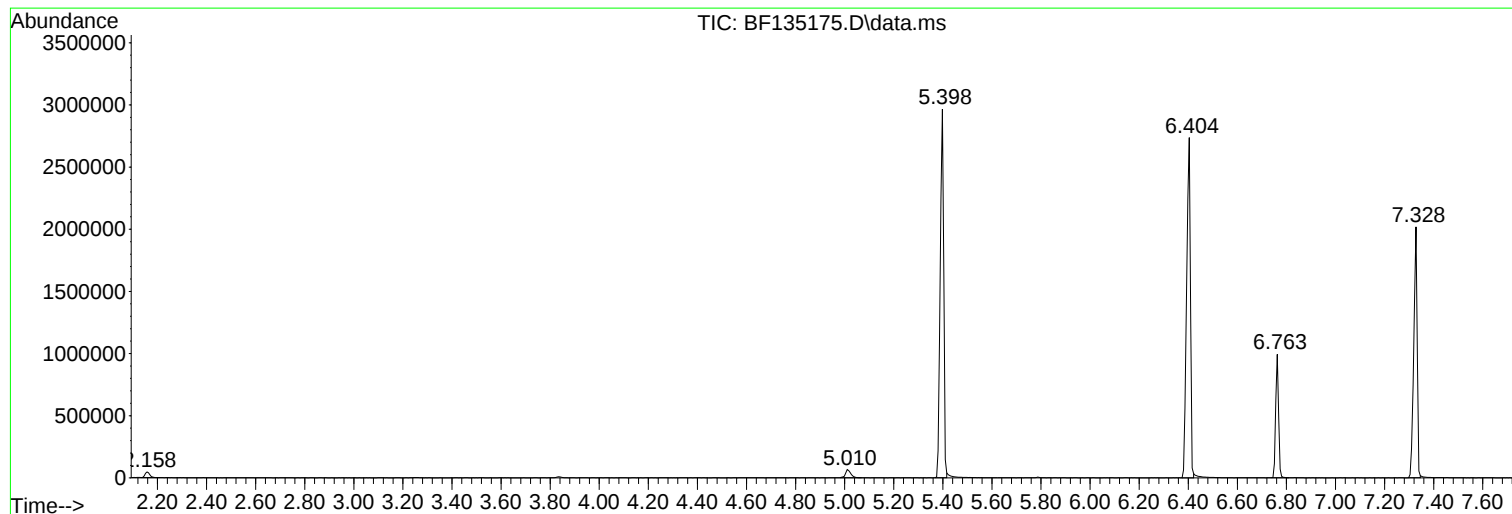

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135175.D
Acq On : 12 Sep 2023 11:32
Operator : CG\JU
Sample : PB155416TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155416TB










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.010 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.010	2.44 ng	99396	1,4-Dichlorobenzene-d4	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45		
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39		
3	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	33		
4	3-Hexanol	102	C6H14O	000623-37-0	28		
5	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28		

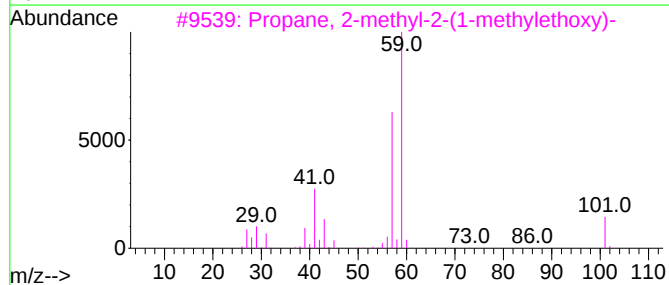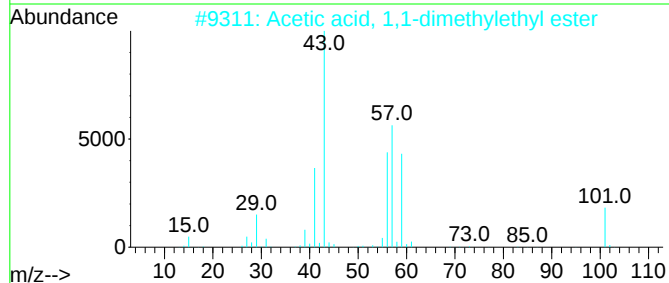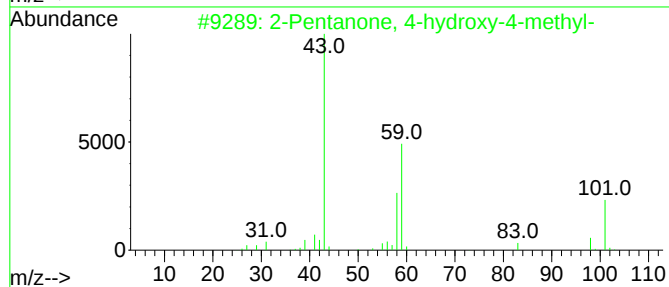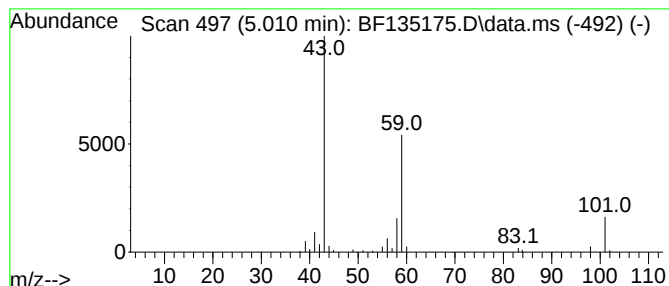

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135175.D
Acq On : 12 Sep 2023 11:32
Operator : CG\JU
Sample : PB155416TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155416TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.010	5.010	2.4	ng	99396	1	6.763	815308	20.0