

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
 Data File : BF135177.D
 Acq On : 12 Sep 2023 12:37
 Operator : CG\JU
 Sample : PB155213BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155213BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	559	564	567	rBV	3363278	3408938	89.25%	14.316%
2	6.404	729	734	737	rBV	2843495	3467835	90.79%	14.563%
3	6.763	791	795	803	rBV	797071	644960	16.89%	2.709%
4	7.328	885	891	894	rBV	2177456	2287942	59.90%	9.608%
5	8.039	1007	1012	1016	rBV	960173	823325	21.56%	3.458%
6	9.122	1190	1196	1199	rBV	3741735	3819511	100.00%	16.040%
7	9.798	1306	1311	1314	rBV	1154292	952221	24.93%	3.999%
8	10.592	1441	1446	1449	rBV	2454646	2368418	62.01%	9.946%
9	11.286	1561	1564	1568	rBV	1190515	1034137	27.08%	4.343%
10	12.892	1832	1837	1840	rBV	3717369	3734592	97.78%	15.683%
11	13.939	2011	2015	2025	rBV	730125	690724	18.08%	2.901%
12	15.404	2259	2264	2277	rBV	483781	579657	15.18%	2.434%




Sum of corrected areas: 23812260

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135177.D
Acq On : 12 Sep 2023 12:37
Operator : CG\JU
Sample : PB155213BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155213BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

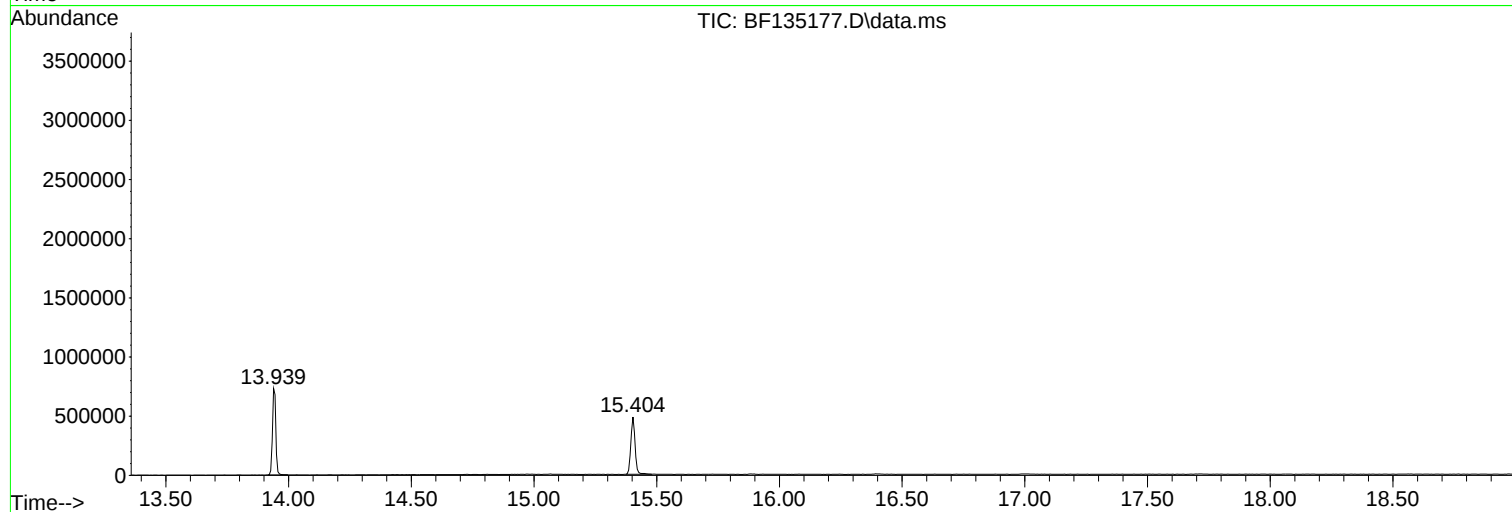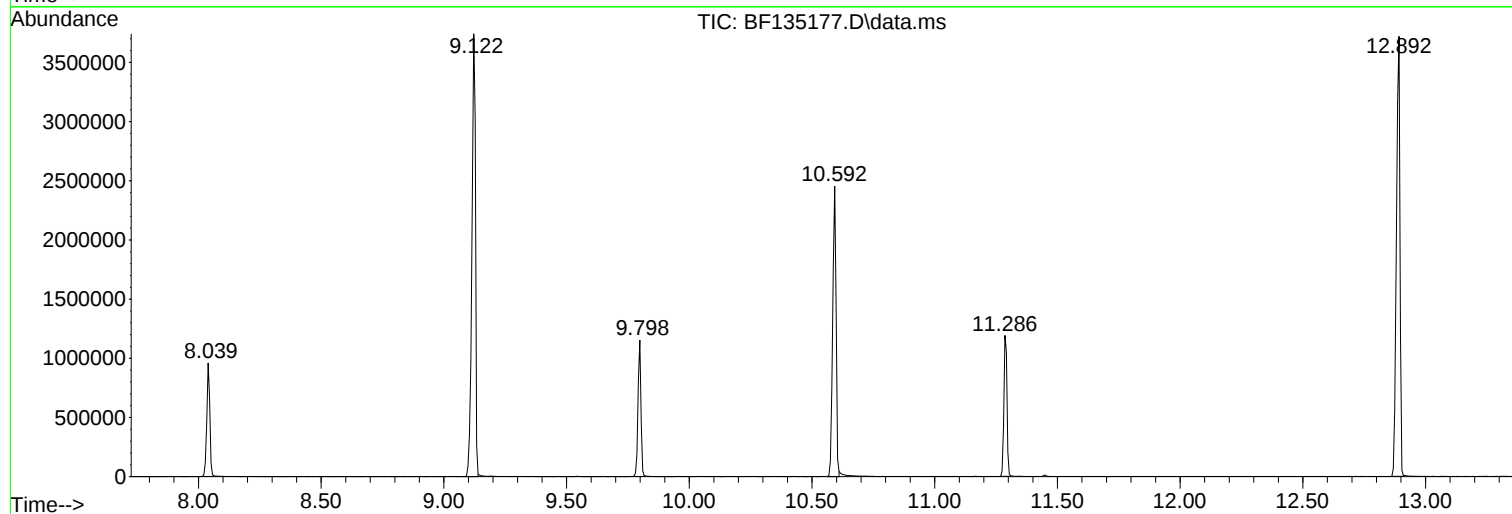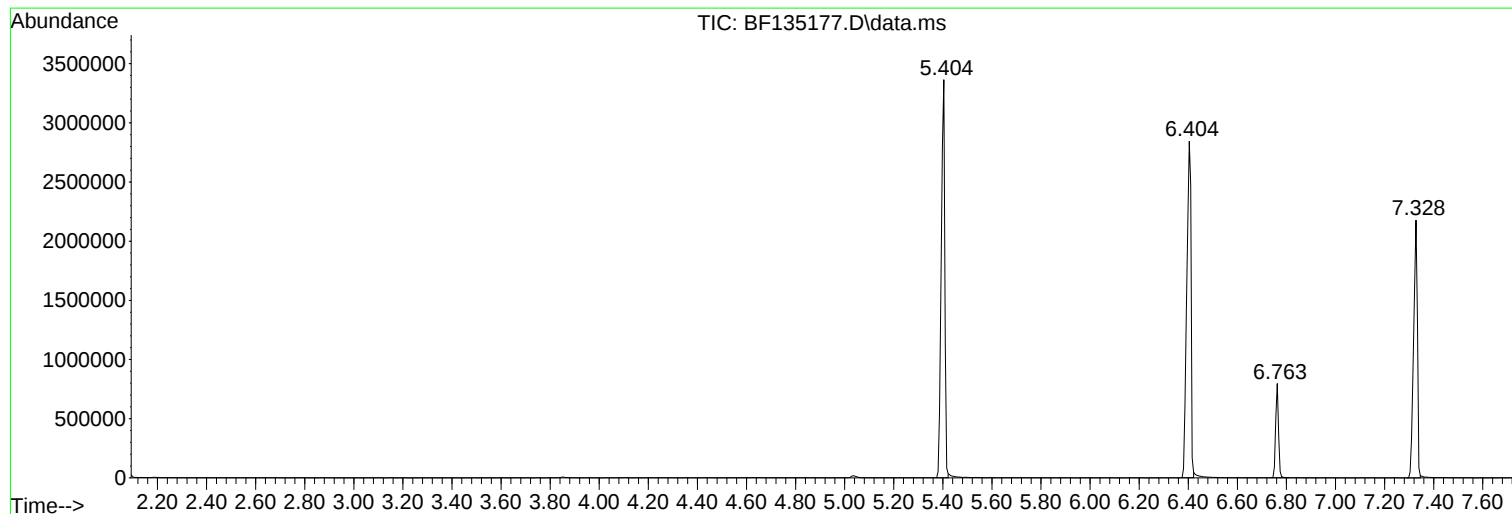

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135177.D
Acq On : 12 Sep 2023 12:37
Operator : CG\JU
Sample : PB155213BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155213BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135177.D
Acq On : 12 Sep 2023 12:37
Operator : CG\JU
Sample : PB155213BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155213BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------