

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
 Data File : BF135186.D
 Acq On : 12 Sep 2023 17:40
 Operator : CG\JU
 Sample : PB155443BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155443BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135186.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	10	14	23	rVB	53862	69061	1.80%	0.282%
2	5.016	491	498	506	rBV	72931	103048	2.68%	0.421%
3	5.399	558	563	566	rBV	2895452	3041072	79.18%	12.418%
4	6.404	729	734	737	rBV	2791039	3026773	78.81%	12.360%
5	6.763	791	795	798	rBV	1000150	833853	21.71%	3.405%
6	7.328	885	891	894	rBV	1995887	1978732	51.52%	8.080%
7	8.040	1007	1012	1016	rBV	1279242	1094171	28.49%	4.468%
8	9.122	1190	1196	1199	rBV	3638799	3461838	90.13%	14.136%
9	9.798	1305	1311	1314	rBV	1480884	1250803	32.57%	5.108%
10	10.592	1440	1446	1449	rBV	2353904	2307101	60.07%	9.421%
11	11.292	1560	1565	1568	rBV	1530192	1382121	35.99%	5.644%
12	12.892	1831	1837	1840	rBV	3746009	3840800	100.00%	15.684%
13	13.945	2011	2016	2019	rBV	1242944	1155274	30.08%	4.717%
14	15.404	2259	2264	2281	rBV	699947	944630	24.59%	3.857%




Sum of corrected areas: 24489277

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135186.D
Acq On : 12 Sep 2023 17:40
Operator : CG\JU
Sample : PB155443BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155443BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

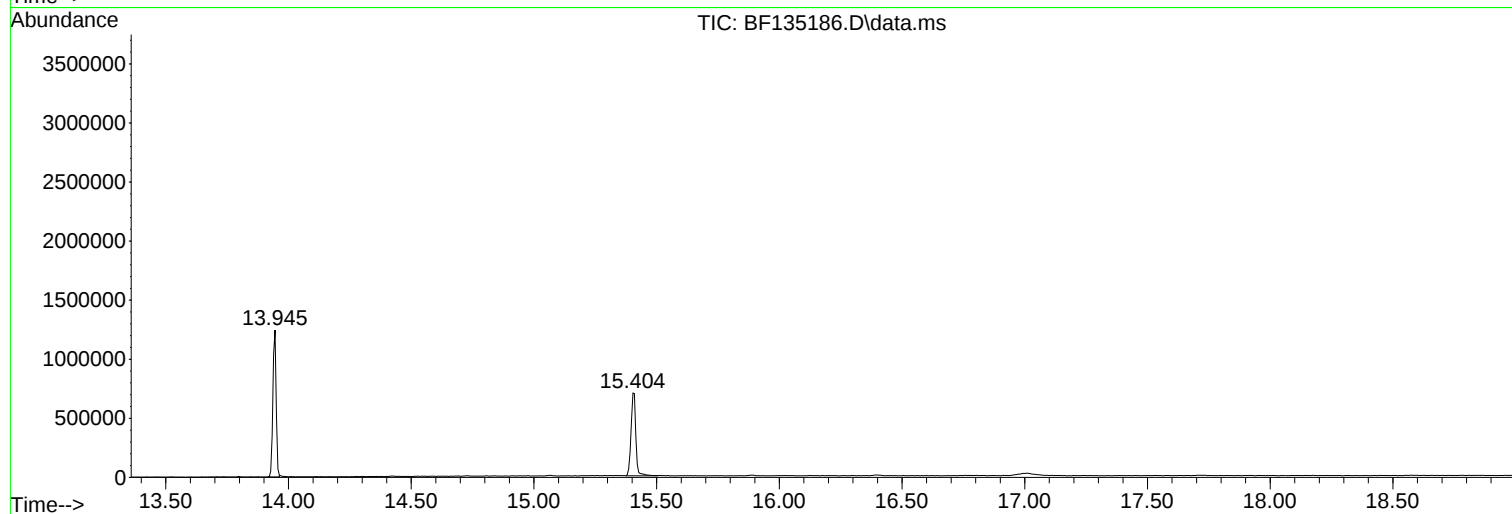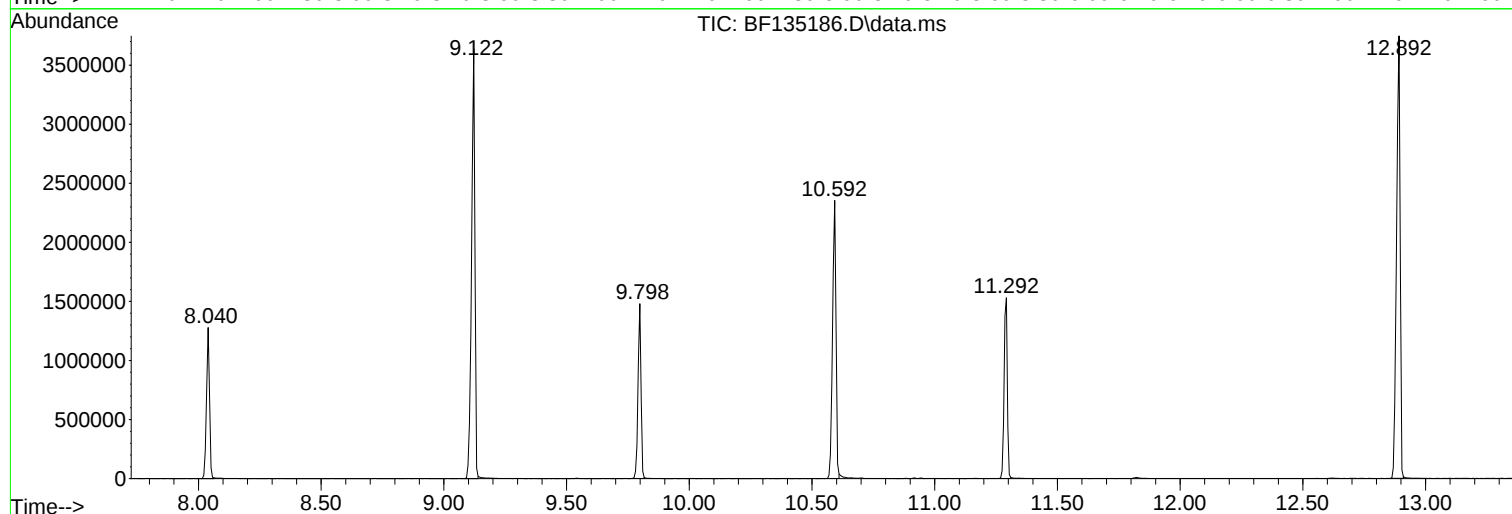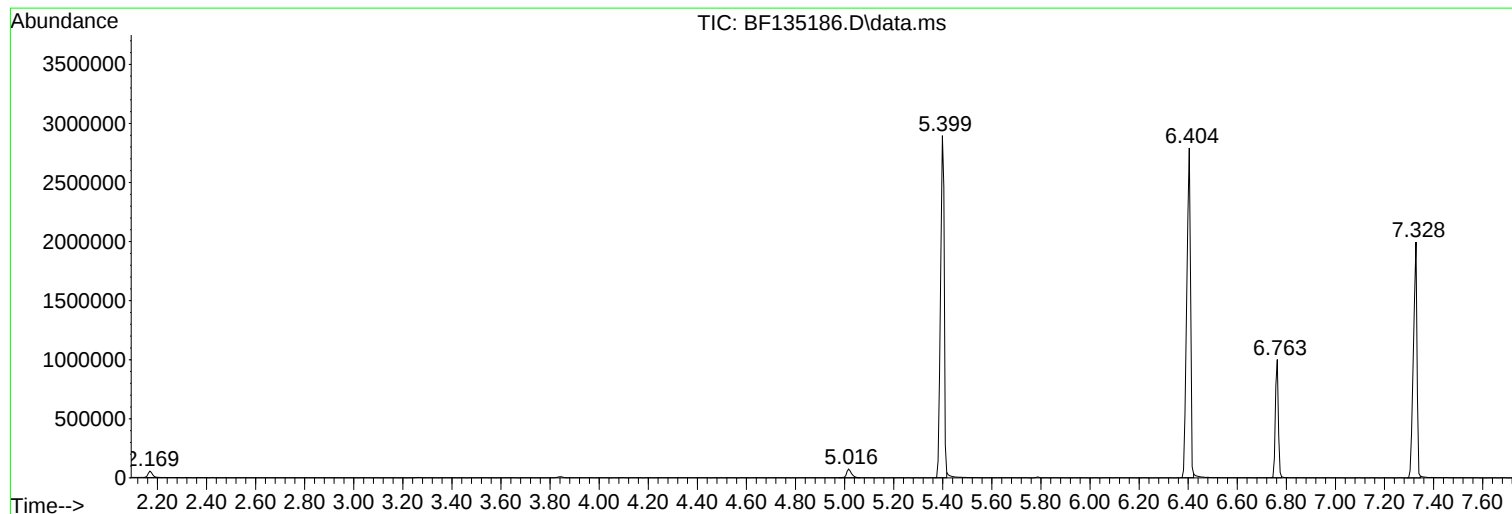

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135186.D
Acq On : 12 Sep 2023 17:40
Operator : CG\JU
Sample : PB155443BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155443BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.016 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.016	2.47 ng	103048	1,4-Dichlorobenzene-d4	6.763

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45	
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	38	
3	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28	
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25	
5	Acetamide, N-(cyanomethyl)-	98	C4H6N2O	004814-80-6	9	

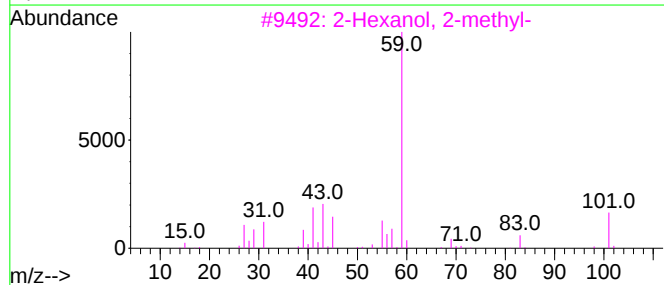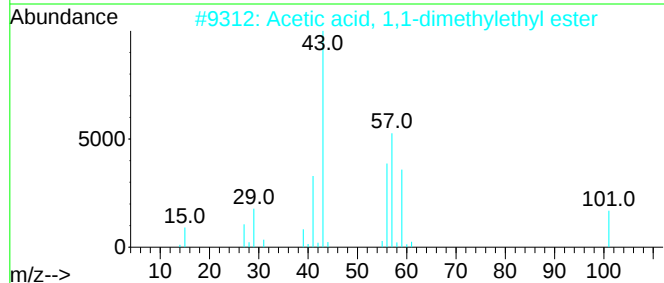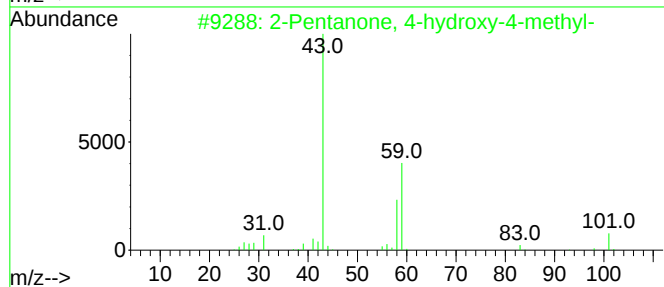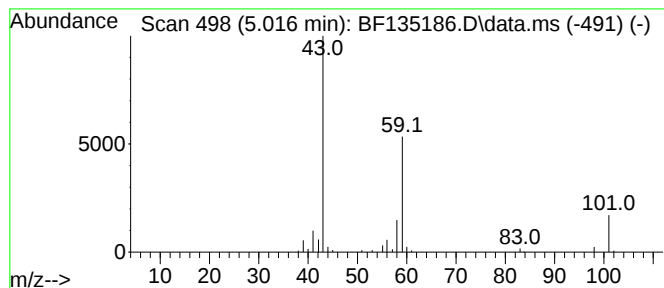

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135186.D
Acq On : 12 Sep 2023 17:40
Operator : CG\JU
Sample : PB155443BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155443BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.016	5.016	2.5	ng	103048	1	6.763	833853	20.0