


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135169.D
Acq On : 12 Sep 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023

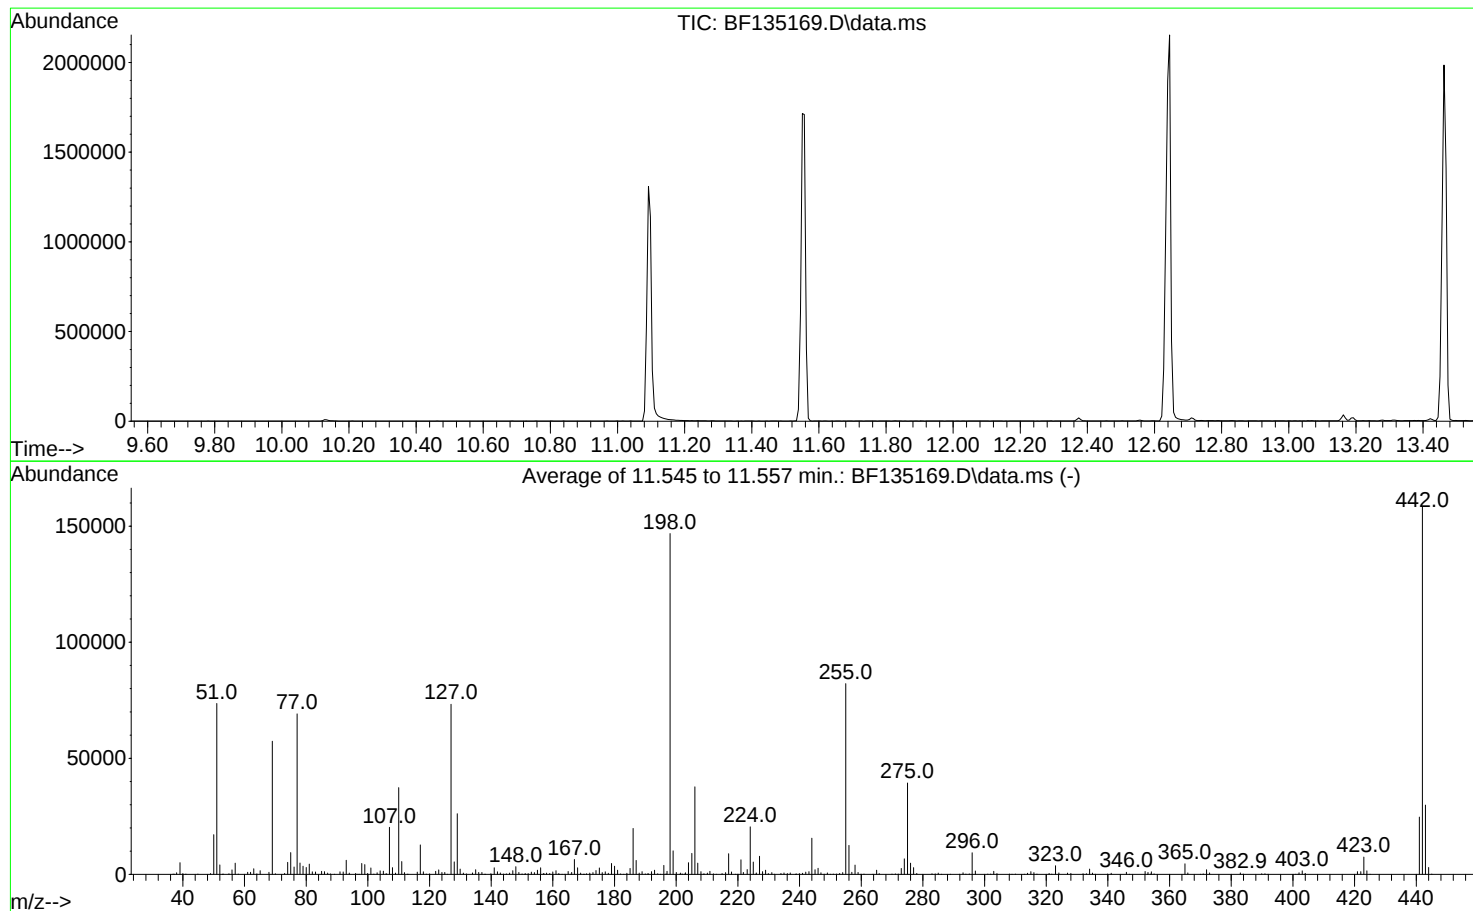




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	73624	PASS
68	69	0.00	2	1.6	903	PASS
69	198	0.00	100	39.1	57360	PASS
70	69	0.00	2	0.4	252	PASS
127	198	10	80	49.9	73259	PASS
197	198	0.00	2	0.9	1288	PASS
198	198	100	100	100.0	146832	PASS
199	198	5	9	6.9	10106	PASS
275	198	10	60	26.8	39332	PASS
365	198	1	100	3.1	4532	PASS
441	198	0.01	100	16.8	24696	PASS
442	442	50	100	100.0	158483	PASS
443	442	15	24	18.8	29823	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF0911223\
 Data File : BF135169.D
 Acq On : 12 Sep 2023 08:10
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 13 05:54:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 00:19:07 2023
 Response via : Initial Calibration

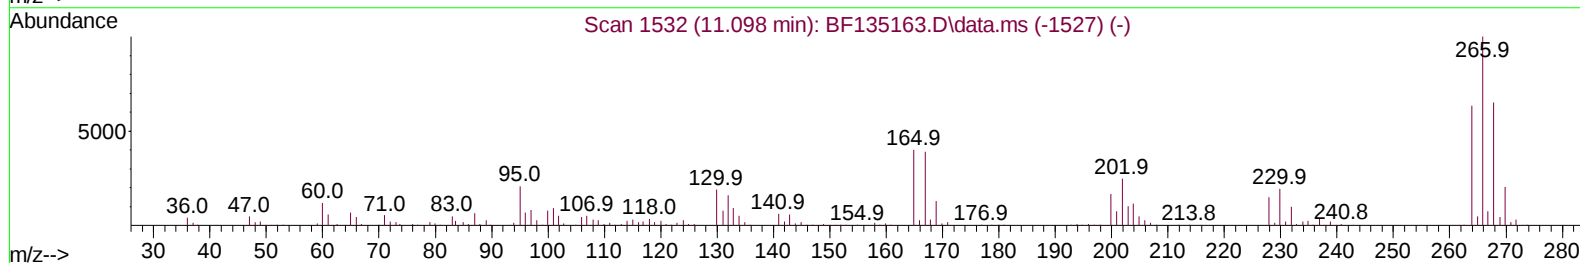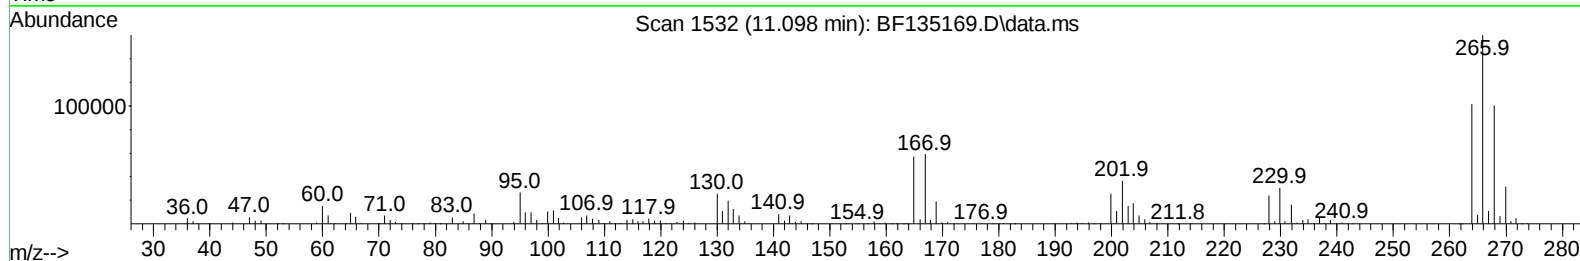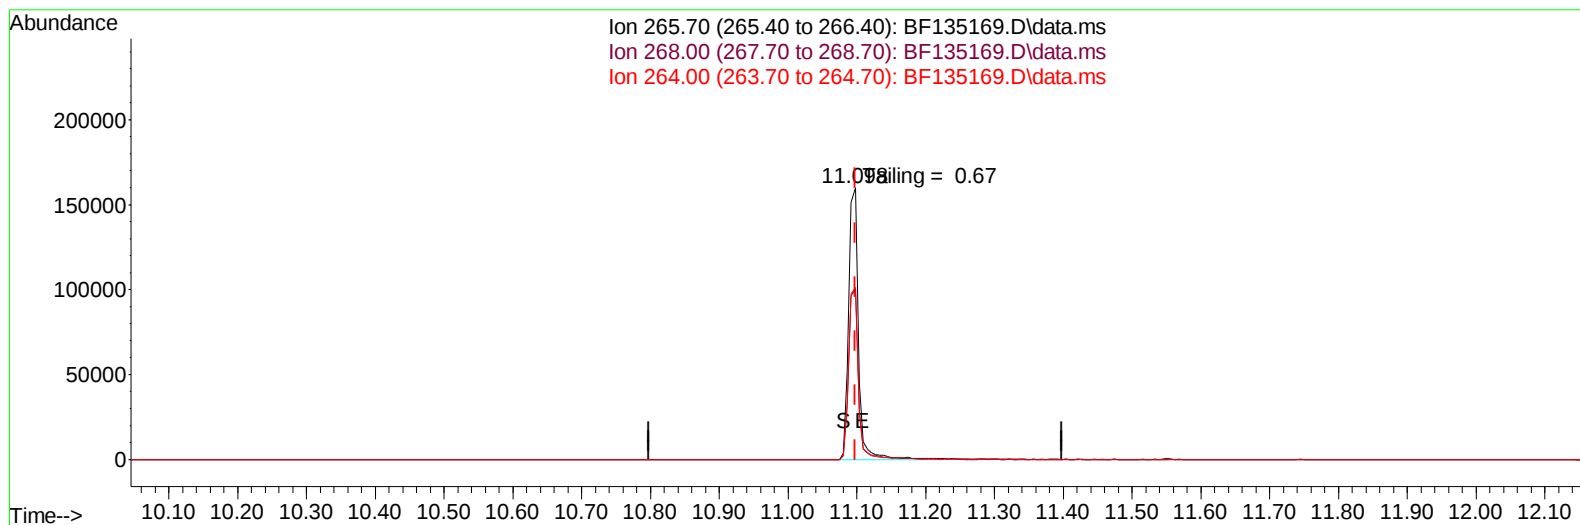

TIC: BF135169.D\data.ms

(70) Pentachlorophenol (C)

11.098min (+ 0.000) 46033.94 ng




response 156557

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	62.78
264.00	63.50	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135169.D
Acq On : 12 Sep 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 13 05:54:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

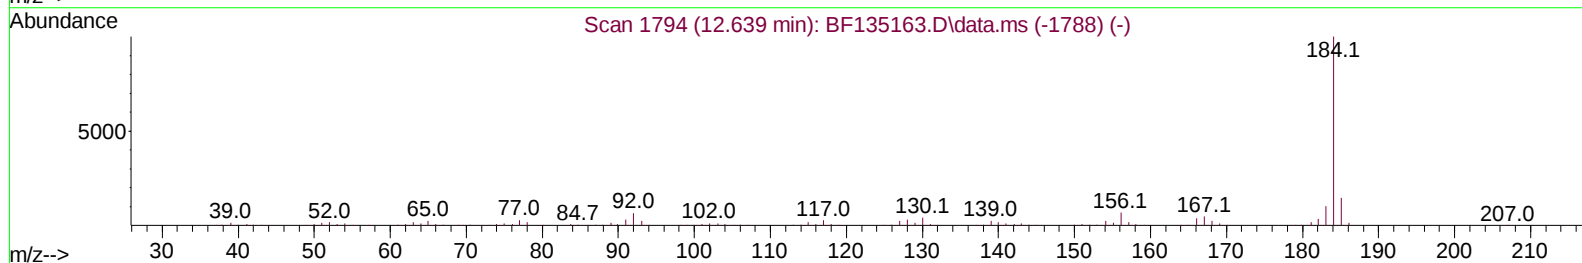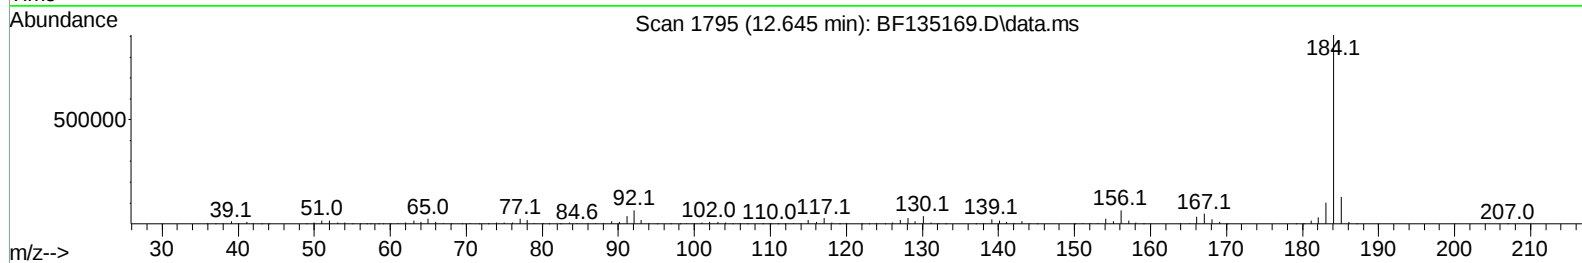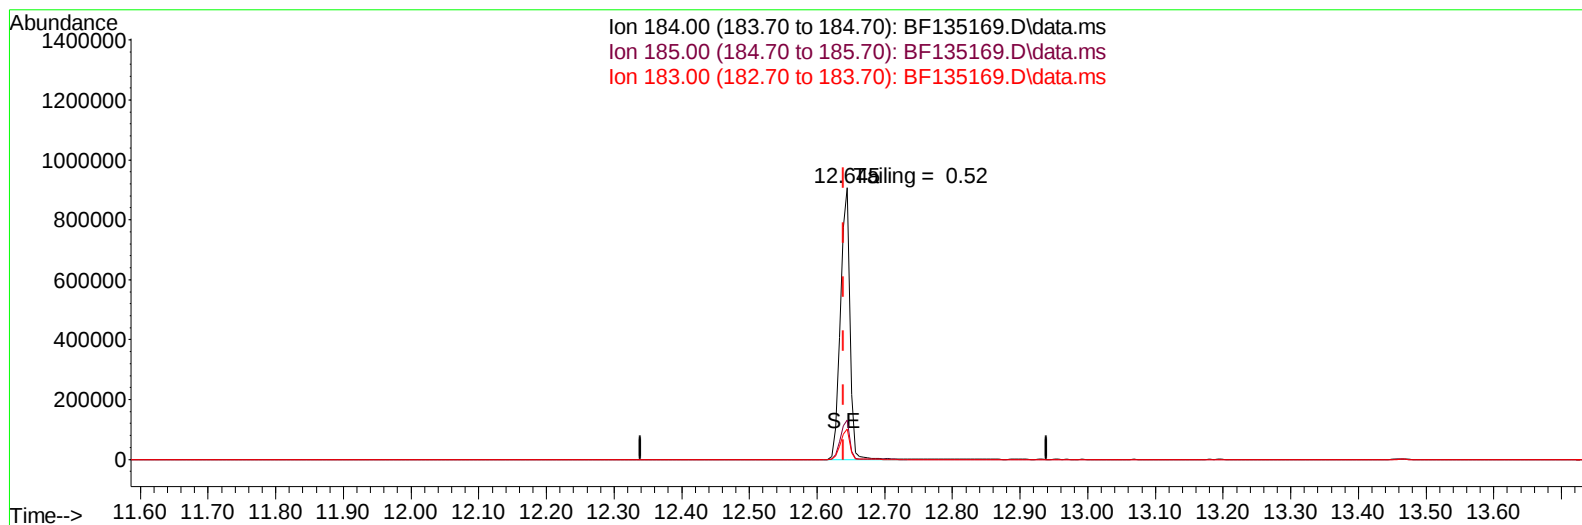

TIC: BF135169.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 0.00 ng

response 878423

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.41
183.00	10.30	11.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/12/2023	BNA_F	<u>BF135169.D</u>
Compound Name	Response	Retention Time
DDT	359204	13.462
DDD	9825	13.162
DDE	158	12.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9983	369187	2.70

Instrument :
BNA_F
ClientSampleId :
DFTPP