
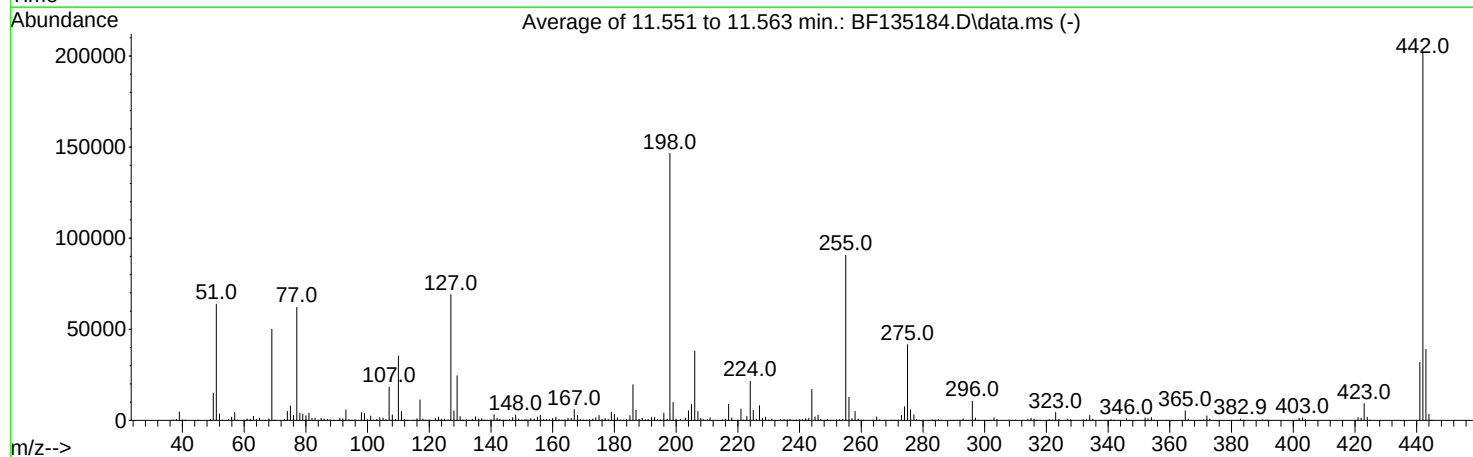


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
 Data File : BF135184.D
 Acq On : 12 Sep 2023 16:34
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 00:19:07 2023

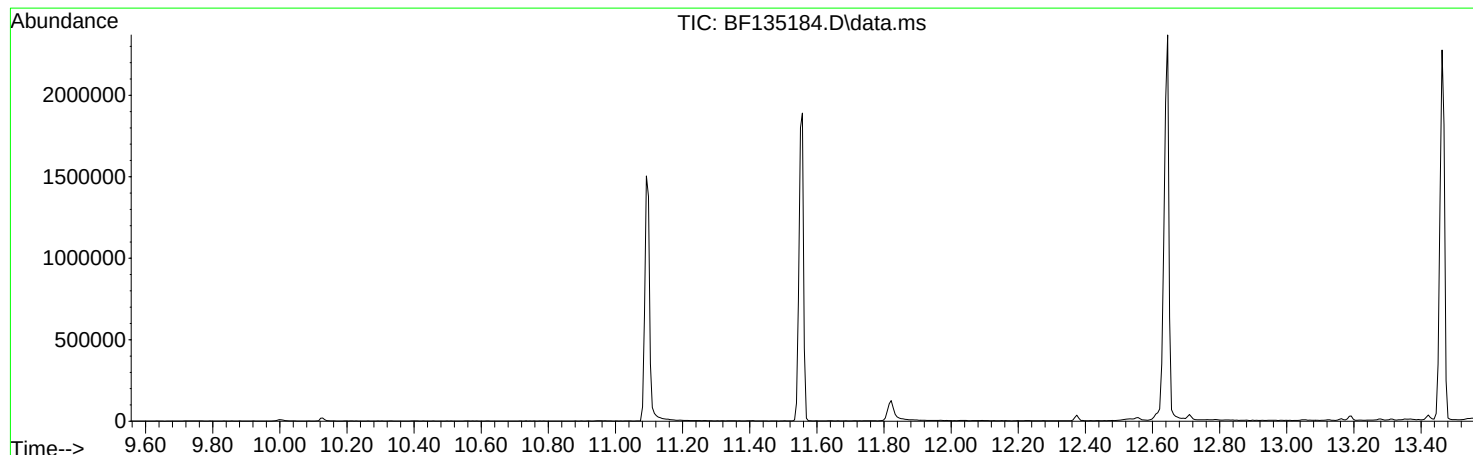




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	63719	PASS
68	69	0.00	2	1.8	881	PASS
69	198	0.00	100	34.1	50018	PASS
70	69	0.00	2	0.4	193	PASS
127	198	10	80	47.1	69000	PASS
197	198	0.00	2	0.5	720	PASS
198	198	100	100	100.0	146552	PASS
199	198	5	9	6.7	9861	PASS
275	198	10	60	28.3	41536	PASS
365	198	1	100	3.6	5261	PASS
441	198	0.01	100	21.7	31800	PASS
442	442	50	100	100.0	201901	PASS
443	442	15	24	19.3	38976	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
 Data File : BF135184.D
 Acq On : 12 Sep 2023 16:34
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 13 05:58:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 00:19:07 2023
 Response via : Initial Calibration

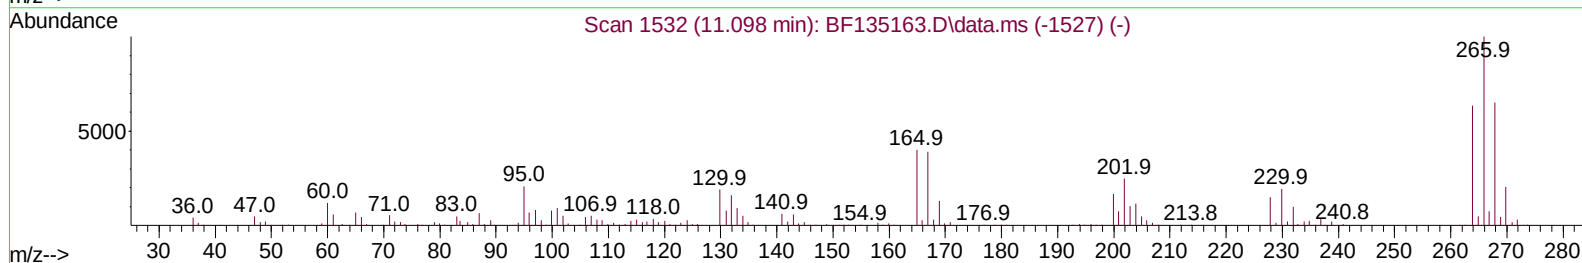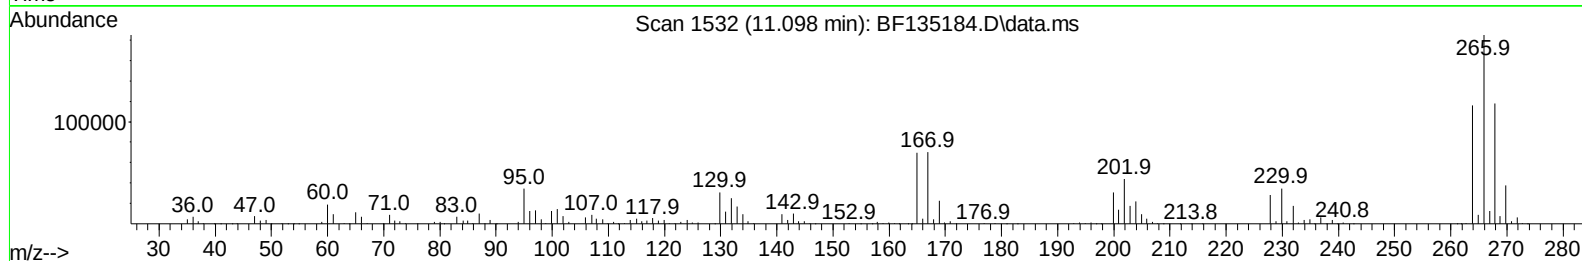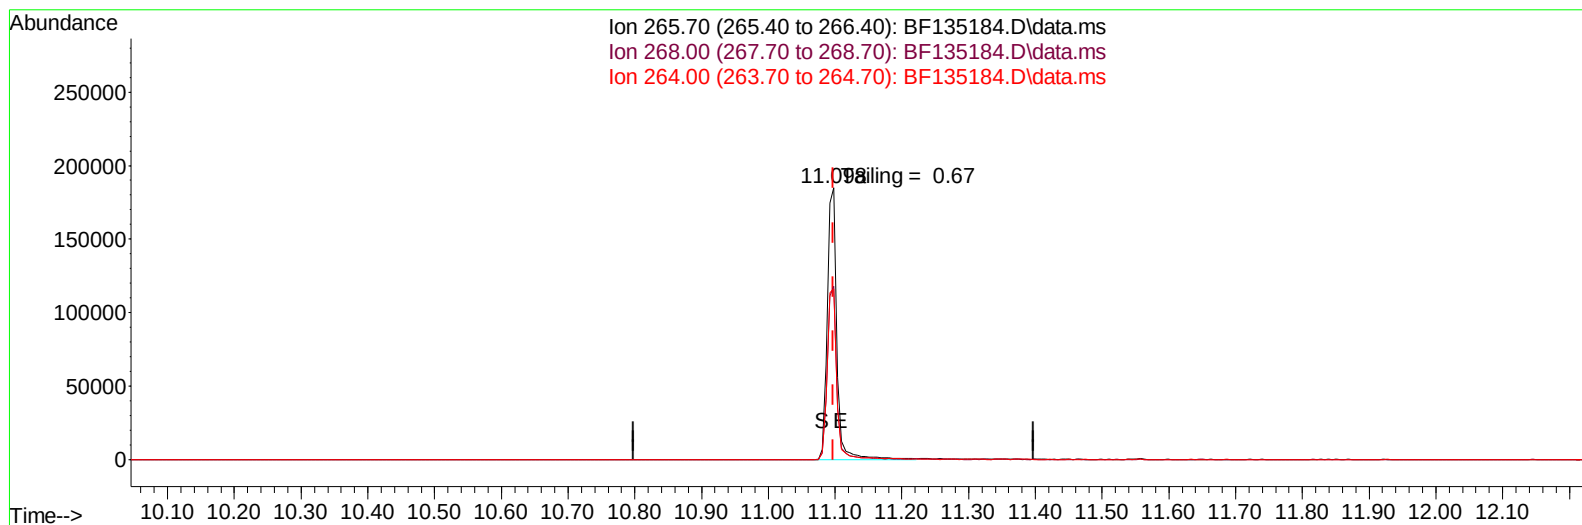

TIC: BF135184.D\data.ms

(70) Pentachlorophenol (C)

11.098min (+ 0.000) 40059.34 ng




response 187479

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	63.83
264.00	63.50	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
Data File : BF135184.D
Acq On : 12 Sep 2023 16:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 13 05:58:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

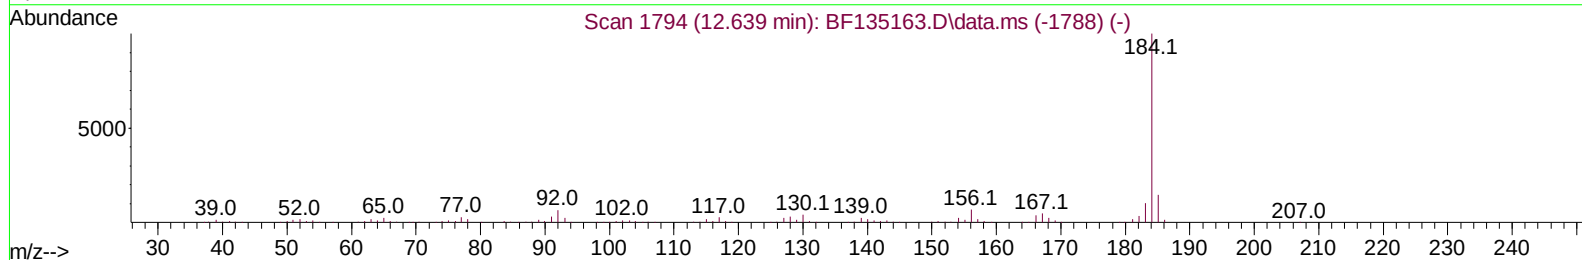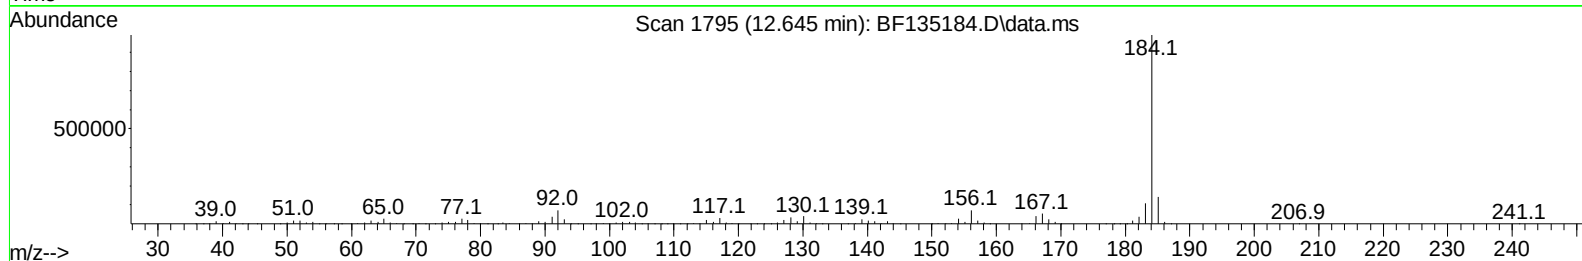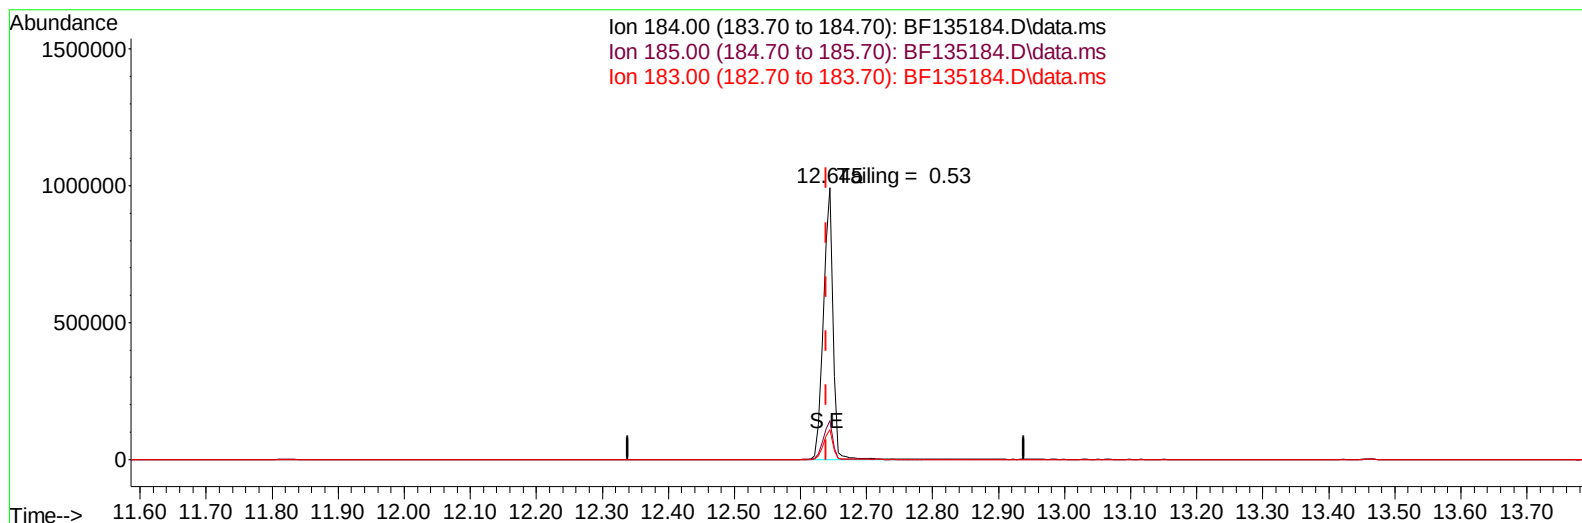

TIC: BF135184.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 0.00 ng

response 966556

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.22
183.00	10.30	10.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/12/2023	BNA_F	<u>BF135184.D</u>
Compound Name	Response	Retention Time
DDT	431837	13.463
DDD	6910	13.192
DDE	308	12.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7218	439055	1.64

Instrument :
BNA_F
ClientSampleId :
DFTPP